

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011625\
 Data File : BP023615.D
 Acq On : 16 Jan 2025 12:20
 Operator : RC/JU
 Sample : Q1084-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0BA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023615.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	7	12	34	rVB	10624226	12298757	91.99%	11.006%
2	3.311	51	55	59	rBV	94801	120410	0.90%	0.108%
3	3.346	59	61	69	rVB	28452	34617	0.26%	0.031%
4	3.723	121	125	138	rBV	131895	210516	1.57%	0.188%
5	4.052	177	181	186	rVB	19372	26277	0.20%	0.024%
6	4.146	193	197	201	rVB3	29261	39648	0.30%	0.035%
7	4.958	330	335	341	rVB3	16816	28200	0.21%	0.025%
8	6.205	542	547	553	rVB2	23252	38709	0.29%	0.035%
9	6.964	667	676	689	rBV	308913	528615	3.95%	0.473%
10	7.140	698	706	719	rBV	1603373	2404039	17.98%	2.151%
11	7.340	734	740	751	rBV	1401268	2171396	16.24%	1.943%
12	7.811	812	820	827	rBV	1223477	1857010	13.89%	1.662%
13	8.493	929	936	953	rBV	1028043	1623494	12.14%	1.453%
14	8.946	1006	1013	1023	rBV	1678082	2601405	19.46%	2.328%
15	9.416	1087	1093	1097	rBV	36304	57020	0.43%	0.051%
16	9.669	1128	1136	1144	rBV	700379	1163106	8.70%	1.041%
17	10.199	1218	1226	1244	rBV	1796274	2939196	21.98%	2.630%
18	10.587	1285	1292	1302	rVB	1650146	2738345	20.48%	2.451%
19	10.710	1305	1313	1326	rBV	956542	1535014	11.48%	1.374%
20	11.910	1511	1517	1526	rVB3	18097	33186	0.25%	0.030%
21	12.169	1552	1561	1568	rBV2	29867	58661	0.44%	0.052%
22	13.840	1838	1845	1857	rBV	3731872	5622989	42.06%	5.032%
23	14.122	1886	1893	1905	rBV	4649916	6777719	50.69%	6.065%
24	14.440	1939	1947	1955	rBV	2859450	3757092	28.10%	3.362%
25	14.616	1968	1977	1990	rBV	171398	343023	2.57%	0.307%
26	14.857	2013	2018	2024	rVB8	8242	14897	0.11%	0.013%
27	15.281	2086	2090	2096	rBV5	11910	15496	0.12%	0.014%
28	15.445	2111	2118	2126	rBV	6651120	9088812	67.98%	8.134%
29	15.551	2129	2136	2147	rBV	611216	932713	6.98%	0.835%
30	15.692	2155	2160	2166	rVB2	27527	40506	0.30%	0.036%
31	15.816	2176	2181	2187	rVB	74132	101104	0.76%	0.090%
32	17.028	2381	2387	2394	rBV2	12459	23955	0.18%	0.021%
33	17.245	2416	2424	2434	rBV2	2908994	4490467	33.59%	4.019%
34	17.345	2434	2441	2454	rBV	7888334	10661495	79.74%	9.541%
35	18.186	2580	2584	2590	rBV5	48976	76911	0.58%	0.069%
36	18.663	2661	2665	2669	rBV7	11592	16828	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011625\
Data File : BP023615.D
Acq On : 16 Jan 2025 12:20
Operator : RC/JU
Sample : Q1084-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BA4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Title : SVOA CALIBRATION

37	19.269	2763	2768	2773	rBV2	72749	107828	0.81%	0.096%
38	19.339	2775	2780	2787	rVV	66365	105467	0.79%	0.094%
39	19.516	2807	2810	2817	rBV3	65750	81602	0.61%	0.073%
40	19.716	2838	2844	2864	rVB	10878484	13094660	97.94%	11.718%
41	21.698	3175	3181	3199	rVB	3379748	5033215	37.65%	4.504%
42	24.898	3715	3725	3748	rBV	5252071	13370012	100.00%	11.965%
43	25.127	3754	3764	3787	rVB	1943026	5479978	40.99%	4.904%




Sum of corrected areas: 111744390

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011625\
Data File : BP023615.D
Acq On : 16 Jan 2025 12:20
Operator : RC/JU
Sample : Q1084-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

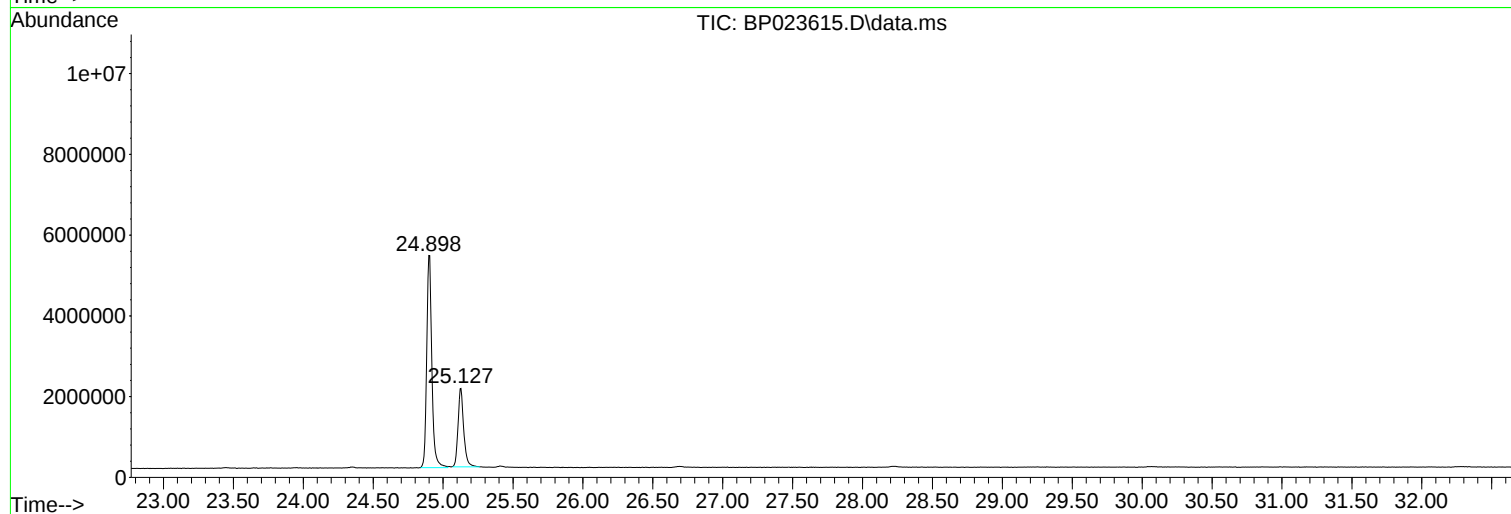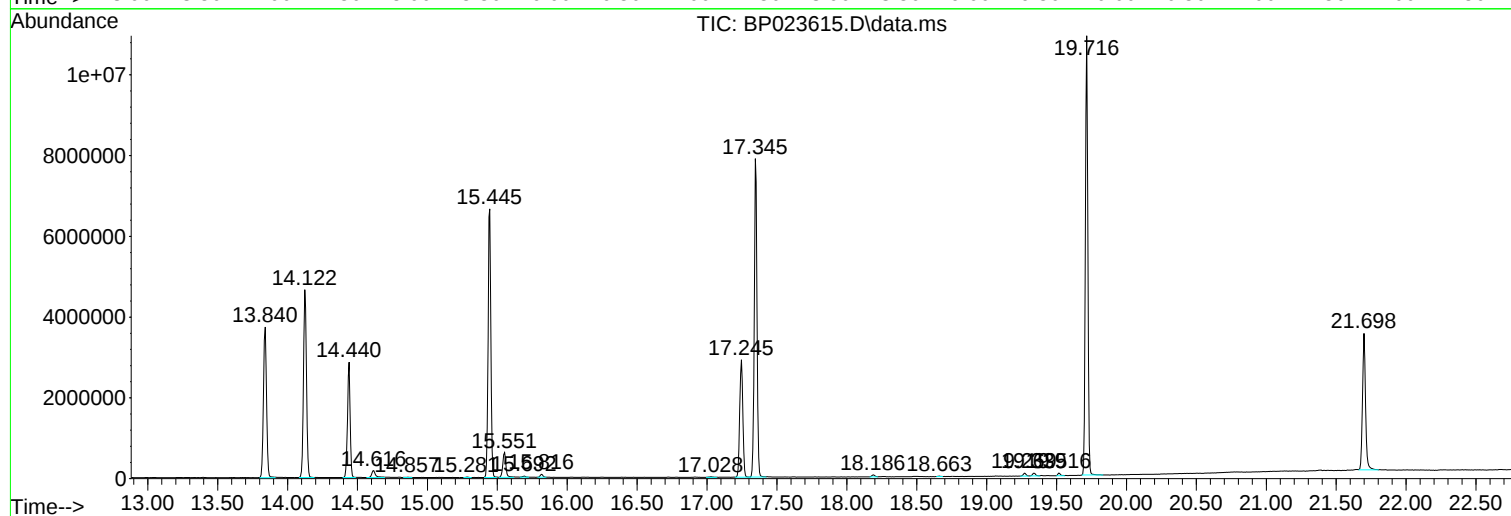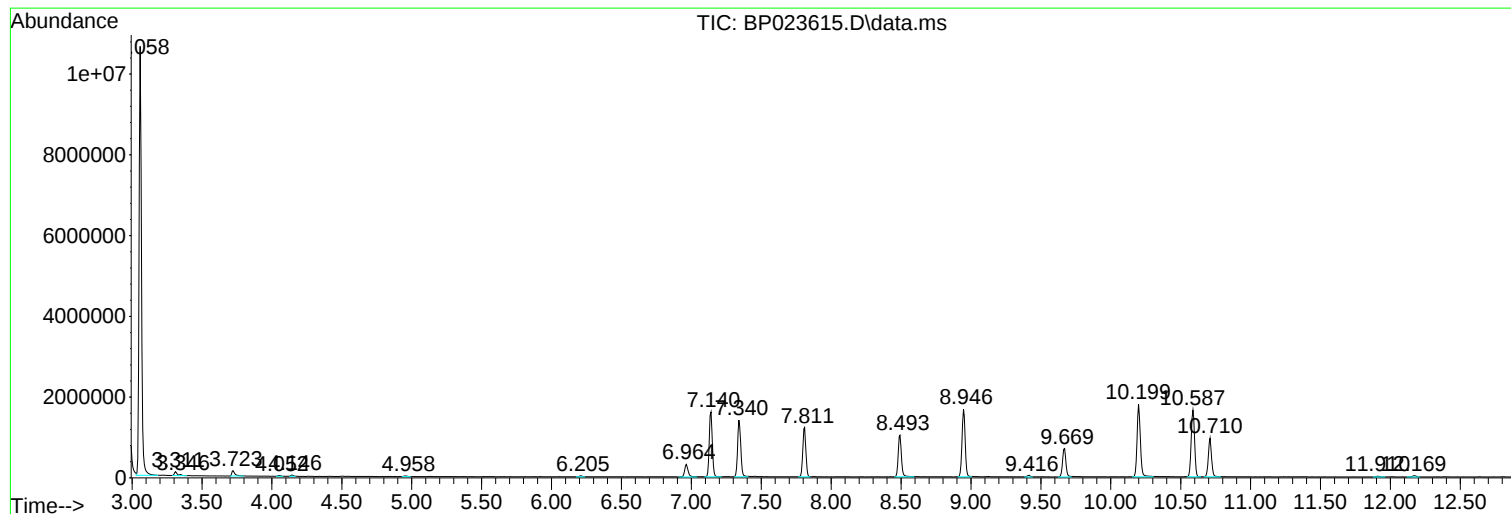

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011625\
Data File : BP023615.D
Acq On : 16 Jan 2025 12:20
Operator : RC/JU
Sample : Q1084-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011625\
Data File : BP023615.D
Acq On : 16 Jan 2025 12:20
Operator : RC/JU
Sample : Q1084-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0BA4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc