
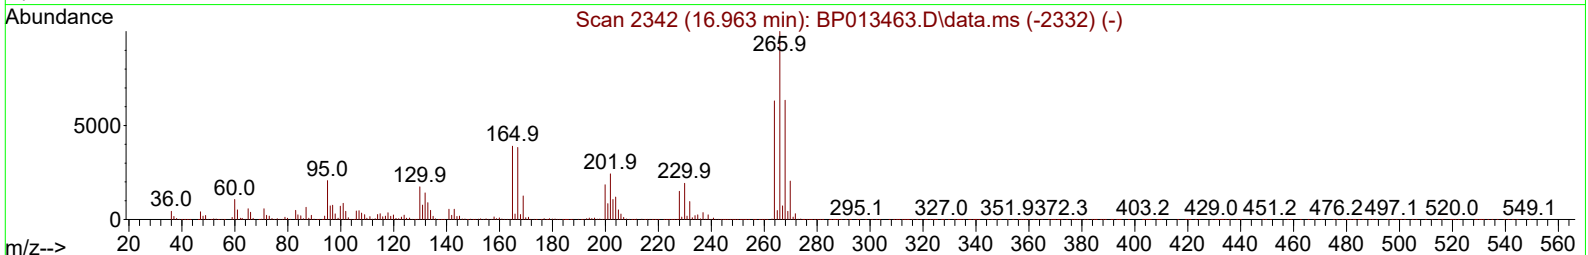
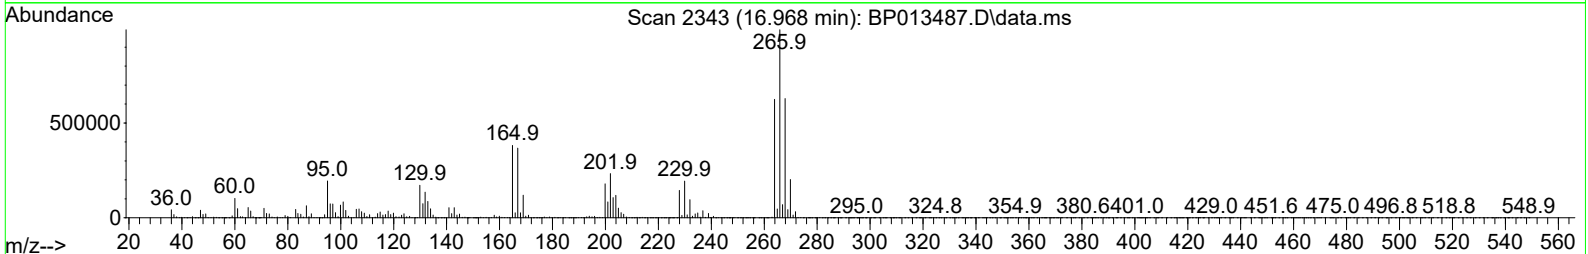


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011723\
 Data File : BP013487.D
 Acq On : 17 Jan 2023 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 06:58:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 13 03:32:57 2023
 Response via : Initial Calibration

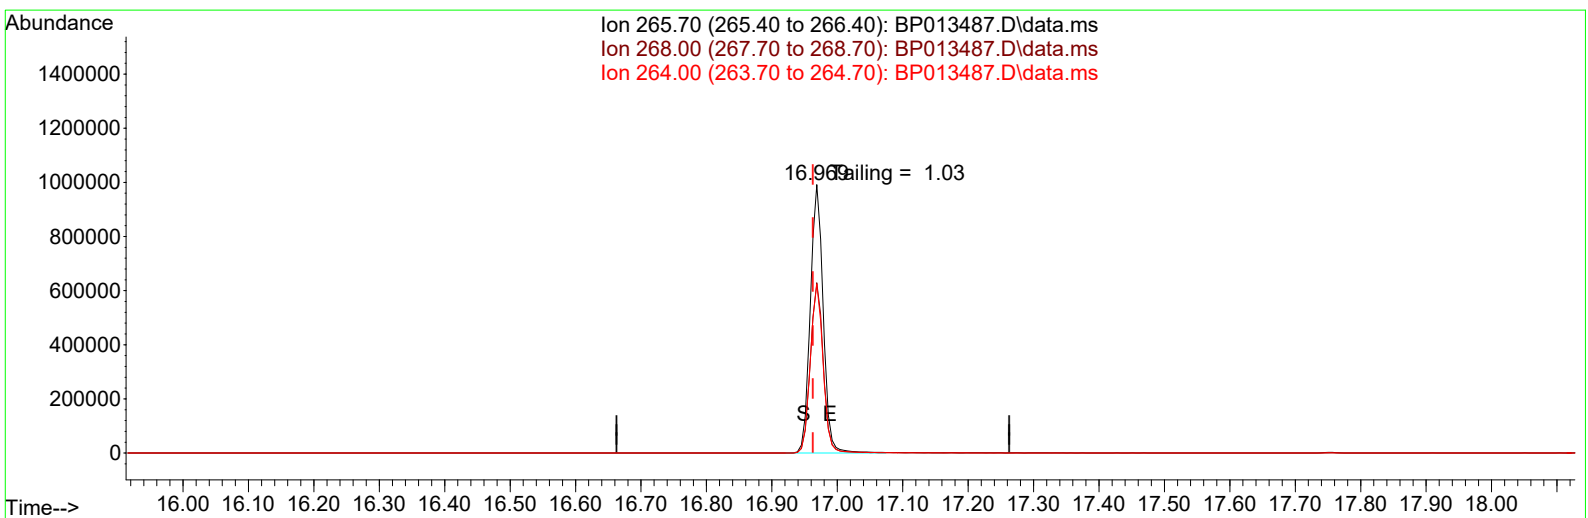

TIC: BP013487.D\data.ms

(70) Pentachlorophenol (C)




16.968min (+ 0.006) 33888.14 ng

response 1364983

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.43
264.00	63.00	62.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011723\
 Data File : BP013487.D
 Acq On : 17 Jan 2023 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 06:58:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 13 03:32:57 2023
 Response via : Initial Calibration

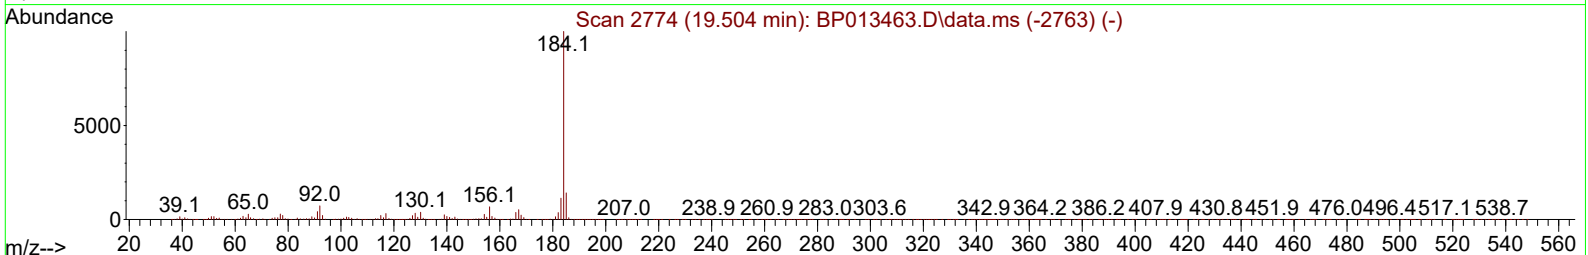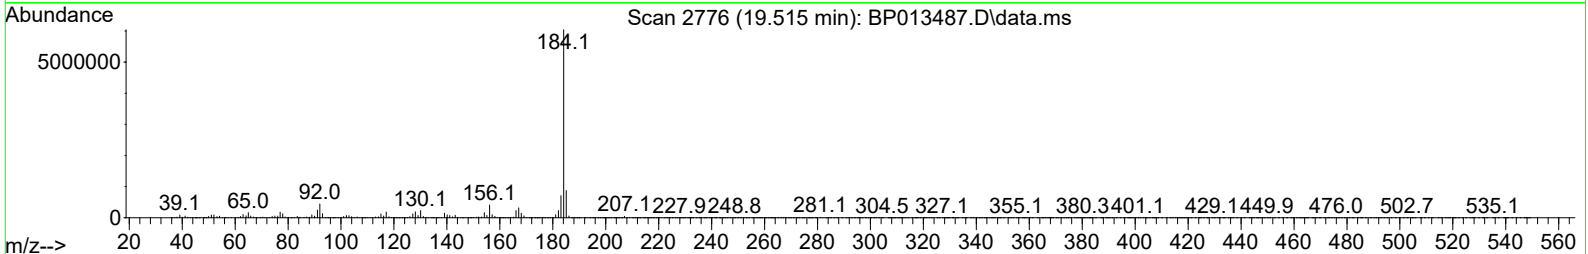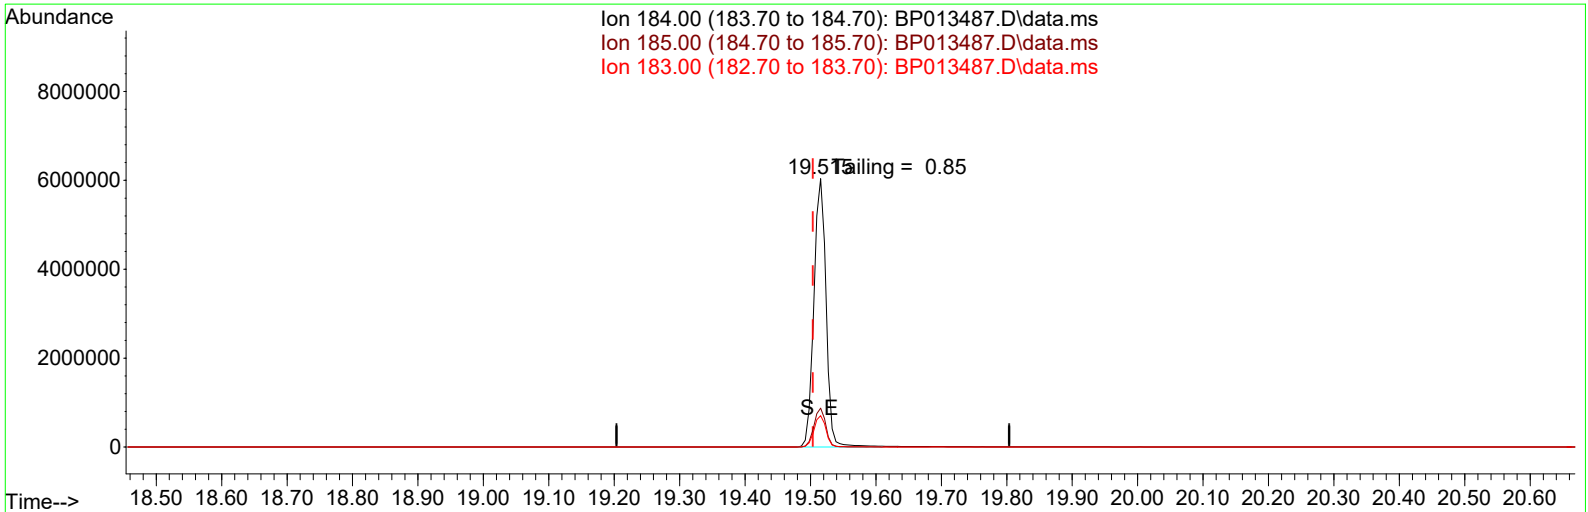

TIC: BP013487.D\data.ms

(77) Benzidine

19.515min (+ 0.012) 17837.74 ng

response 7877842

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.50
183.00	11.40	11.71
0.00	0.00	0.00