


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011723\
 Data File : BP013487.D
 Acq On : 17 Jan 2023 09:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 13 03:32:57 2023

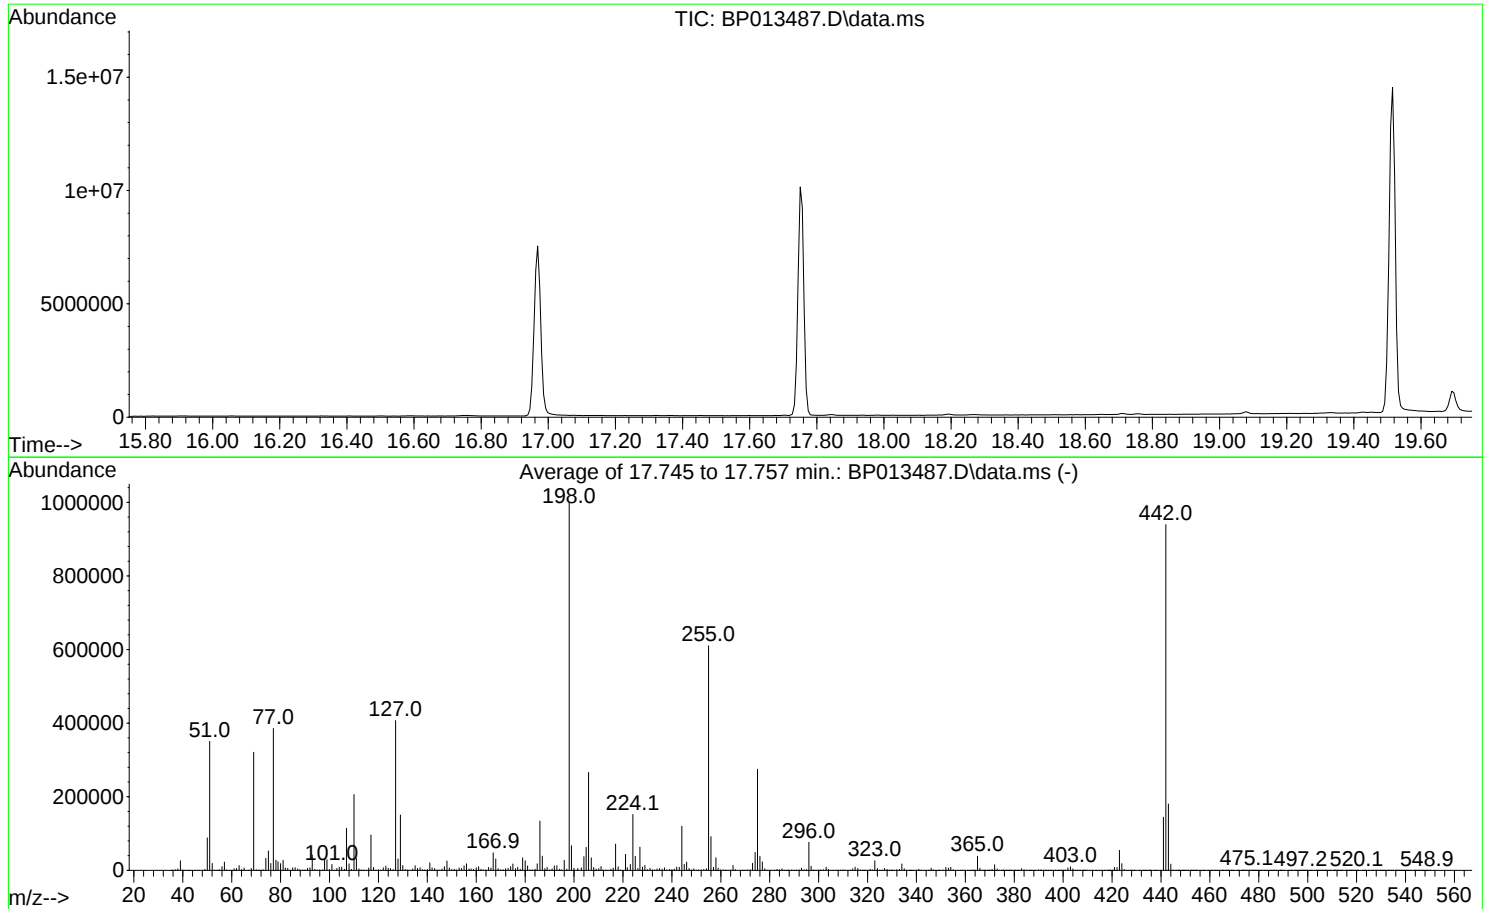




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	350145	PASS
68	69	0.00	2	1.6	5153	PASS
69	198	0.00	100	32.1	320732	PASS
70	69	0.00	2	0.6	1774	PASS
127	198	10	80	40.7	407154	PASS
197	198	0.00	2	0.3	3372	PASS
198	198	100	100	100.0	999924	PASS
199	198	5	9	6.7	66677	PASS
275	198	10	60	27.5	274816	PASS
365	198	1	100	3.8	37923	PASS
441	198	0.01	100	14.4	144096	PASS
442	442	100	100	100.0	939563	PASS
443	442	15	24	19.2	180341	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011723\
Data File : BP013487.D
Acq On : 17 Jan 2023 09:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 18 06:58:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 13 03:32:57 2023
Response via : Initial Calibration

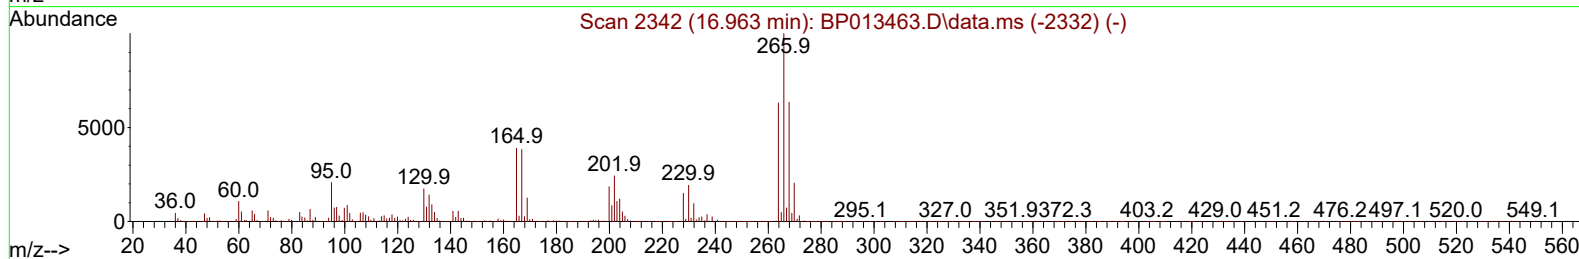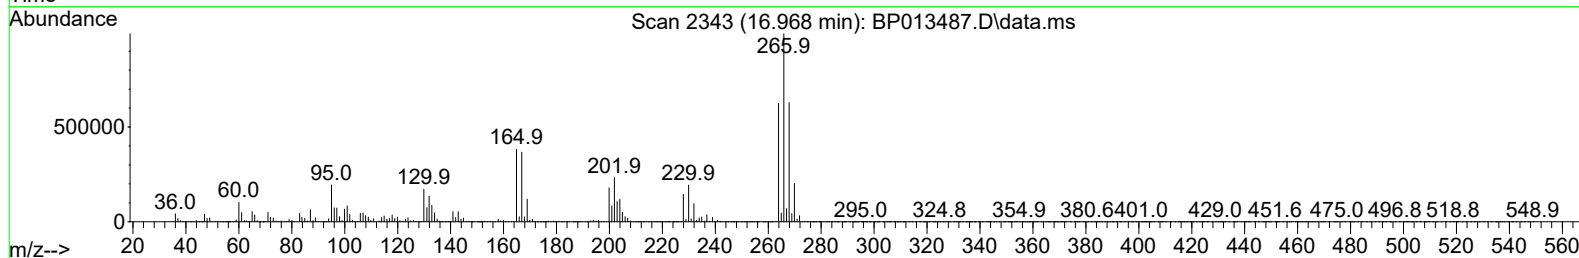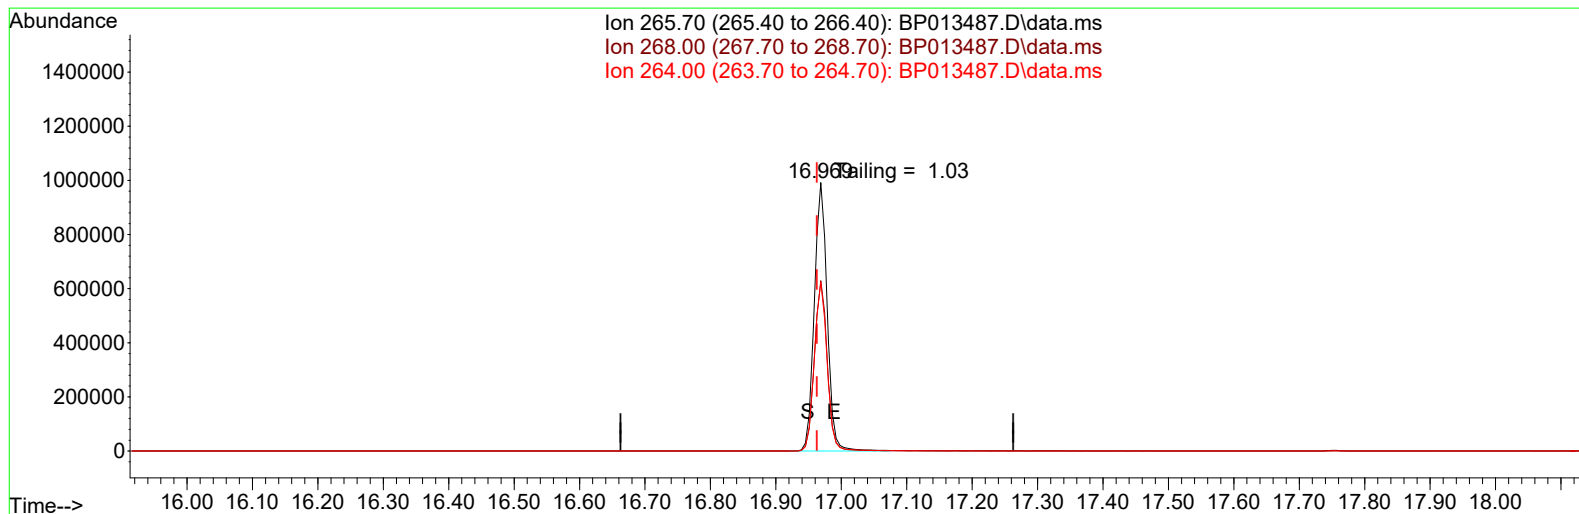

TIC: BP013487.D\data.ms

(70) Pentachlorophenol (C)

16.968min (+ 0.006) 33888.14 ng




response 1364983

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.43
264.00	63.00	62.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011723\
Data File : BP013487.D
Acq On : 17 Jan 2023 09:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 18 06:58:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 13 03:32:57 2023
Response via : Initial Calibration

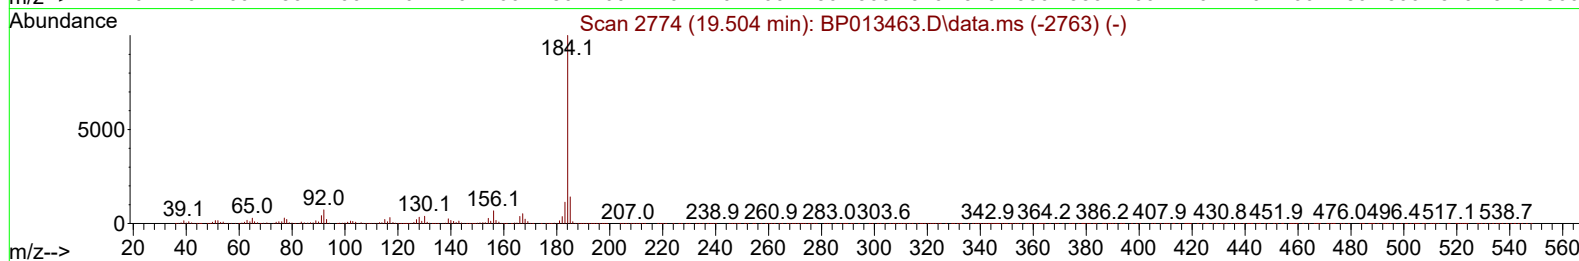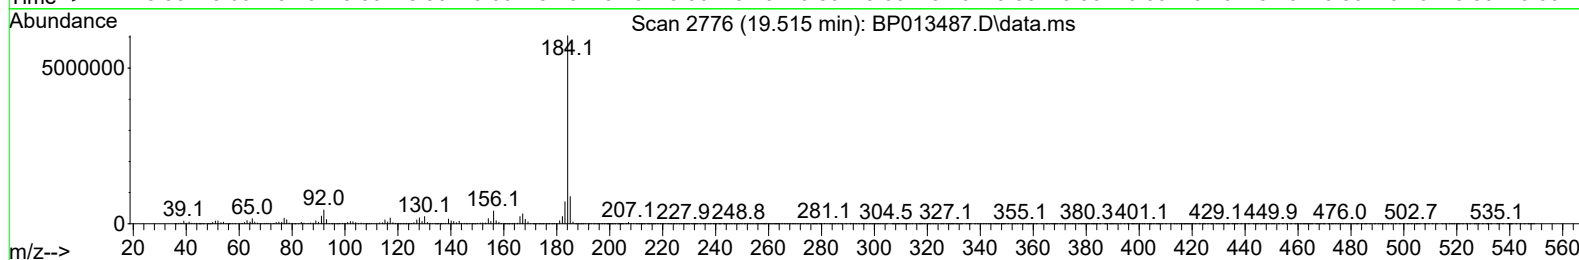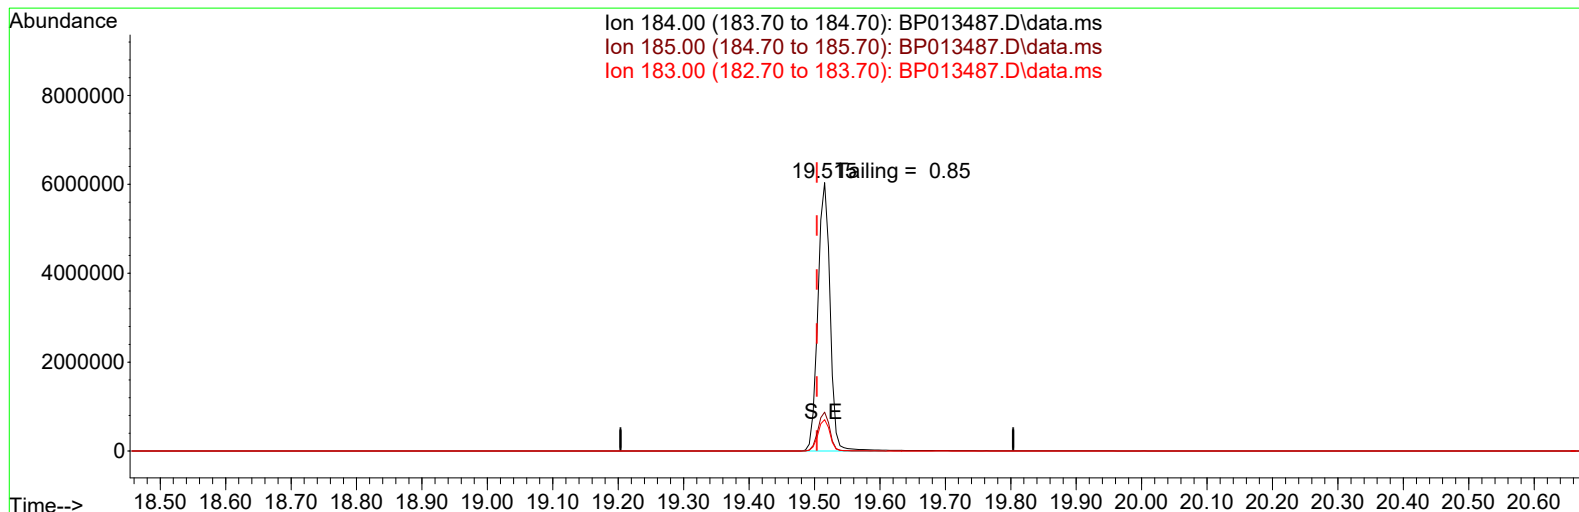

TIC: BP013487.D\data.ms

(77) Benzidine

19.515min (+ 0.012) 17837.74 ng

response 7877842

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.50
183.00	11.40	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/17/2023	BNA_P	<u>BP013487.D</u>
Compound Name	Response	Retention Time
DDT	3786796	20.709
DDD	40086	20.327
DDE	3027	19.78
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
43113	3829909	1.13

Instrument :
BNA_P
ClientSampleId :
DFTPP