

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
 Data File : BP023630.D
 Acq On : 17 Jan 2025 15:59
 Operator : RC/JU
 Sample : Q1086-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF0

Quant Time: Jan 17 16:25:41 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 14 16:27:27 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	532628	20.000	ng/u1	0.00
20) Naphthalene-d8	10.587	136	2242178	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.428	164	1422437	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.234	188	2829912	20.000	ng/u1	0.00
79) Chrysene-d12	21.680	240	2692977	20.000	ng/u1	-0.03
88) Perylene-d12	25.104	264	2968983	20.000	ng/u1	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	64392	4.458	ng/uL	0.00
4) Pyridine-d5	3.717	84	362050	8.990	ng/u1	0.00
7) Phenol-d5	6.964	99	330074	7.198	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	780613	29.059	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	934730	25.811	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	619457	17.416	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	490673	28.671	ng/u1	0.00
24) 2-Nitrophenol-d4	9.669	143	377815	33.634	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.199	165	927020	27.131	ng/u1	0.00
31) 4-Chloroaniline-d4	10.705	131	1269287	23.269	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	3364221	30.390	ng/u1	0.00
49) Acenaphthylene-d8	14.122	160	3809198	28.925	ng/u1	0.00
54) 4-Nitrophenol-d4	14.610	143	55845	3.035	ng/u1	0.00
60) Fluorene-d10	15.440	176	3345109	34.915	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.546	200	160053	17.382	ng/u1	0.00
73) Anthracene-d10	17.334	188	5378175	35.206	ng/u1	-0.01
81) Pyrene-d10	19.698	212	6182364	41.440	ng/u1	-0.02
92) Benzo(a)pyrene-d12	24.874	264	6081753	37.693	ng/u1	-0.04
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.346	88	21473	1.405	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
Data File : BP023630.D
Acq On : 17 Jan 2025 15:59
Operator : RC/JU
Sample : Q1086-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF0

Quant Time: Jan 17 16:25:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 14 16:27:27 2025
Response via : Initial Calibration

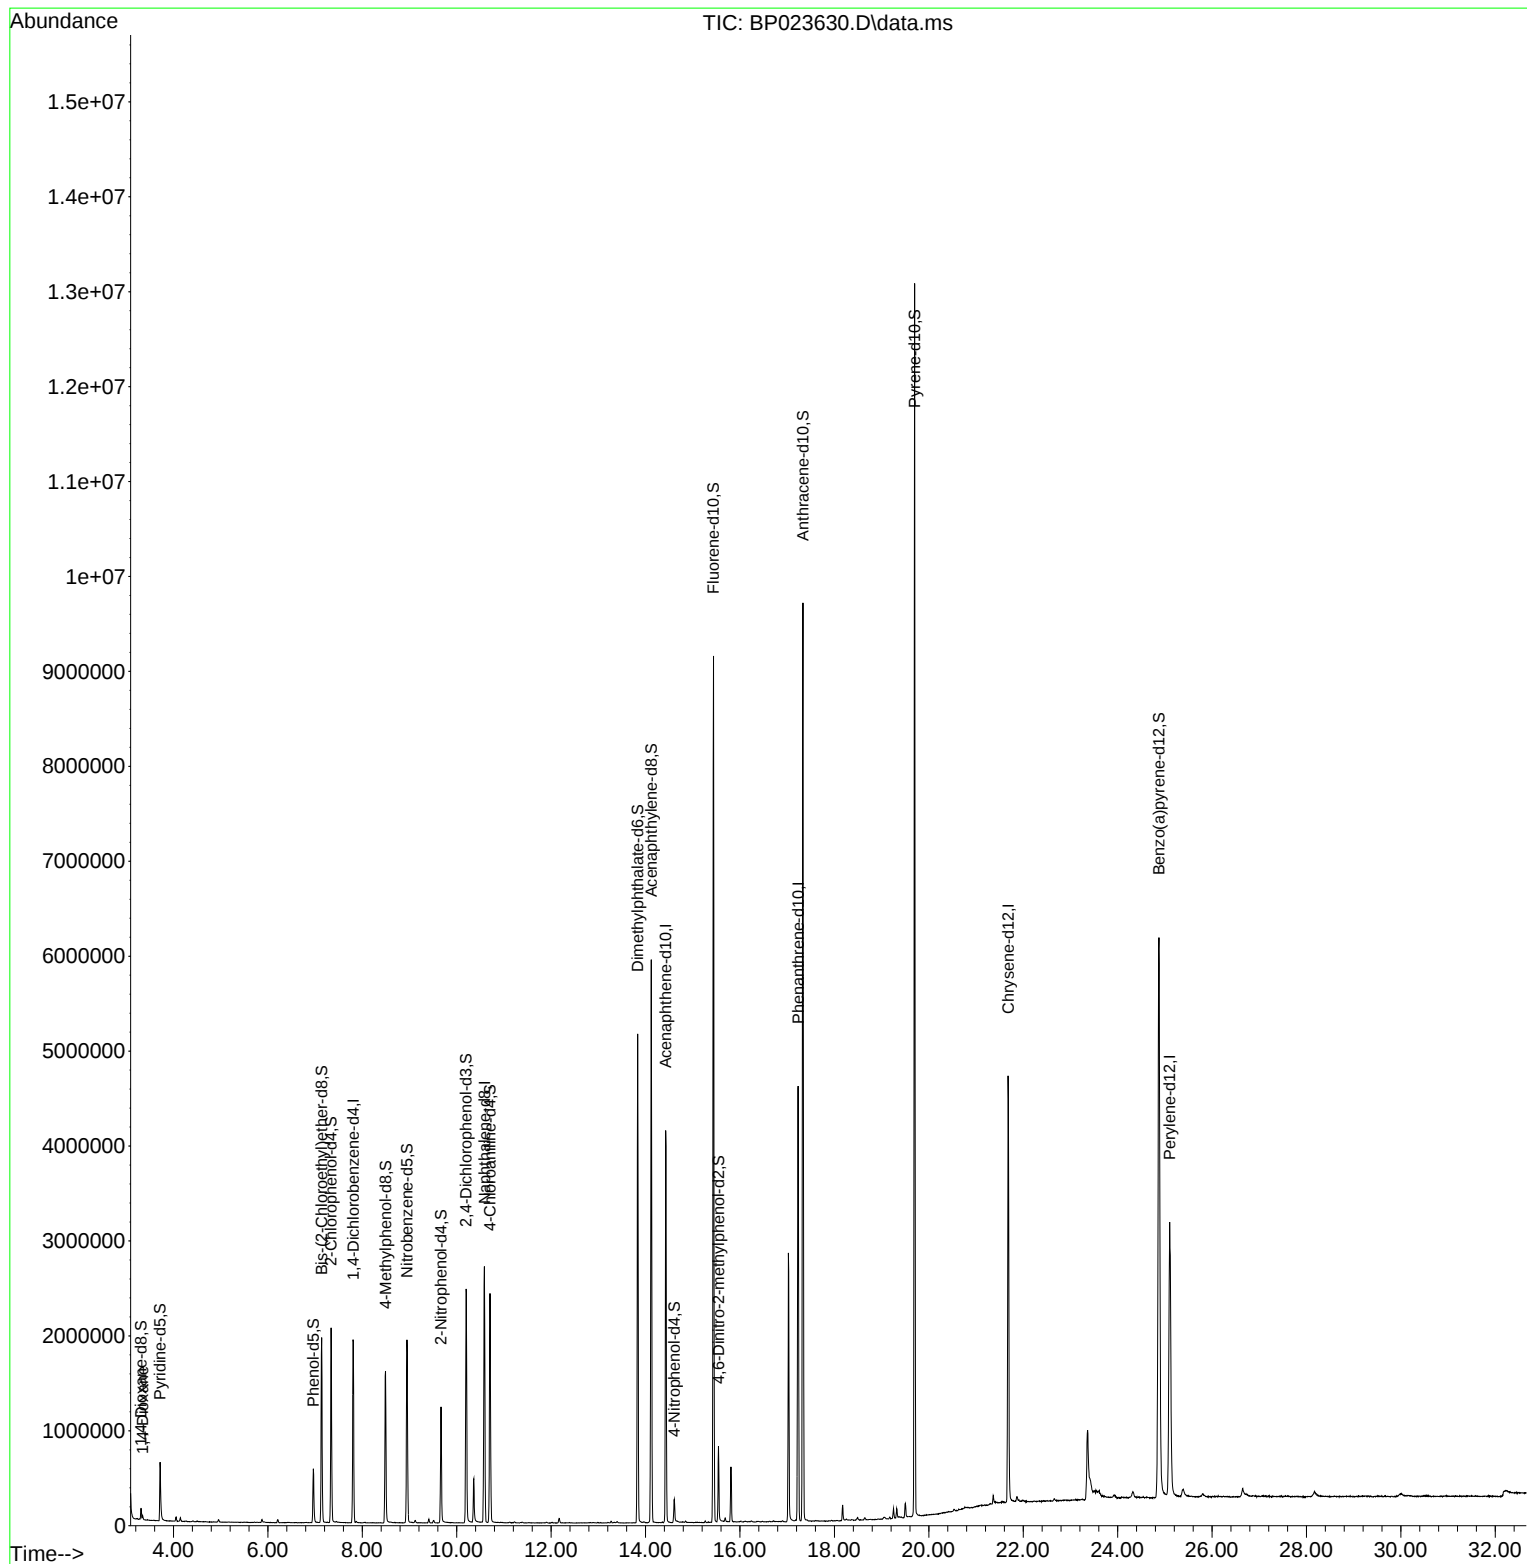

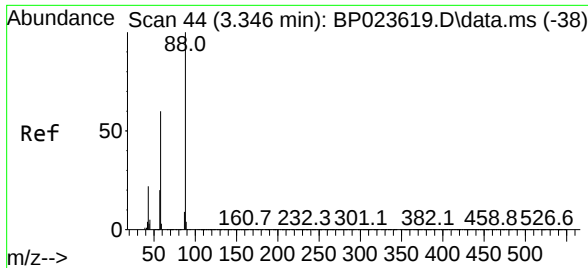

#2
 1,4-Dioxane
 Concen: 1.405 ng/uL
 RT: 3.346 min Scan# 44
 Delta R.T. -0.006 min
 Lab File: BP023630.D
 Acq: 17 Jan 2025 15:59

Instrument :
 BNA_P
 ClientSampleId :
 C0AF0

Tgt Ion:	88	Resp:	21473
Ion	Ratio	Lower	Upper
88	100		
43	24.9	17.3	25.9
58	58.9	47.4	71.0

