

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
 Data File : BP023638.D
 Acq On : 17 Jan 2025 22:04
 Operator : RC/JU
 Sample : Q1086-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF6

Quant Time: Jan 17 23:51:45 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jan 14 16:27:27 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	456949	20.000	ng/u1	0.00
20) Naphthalene-d8	10.581	136	1856576	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.428	164	1126649	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.222	188	2245025	20.000	ng/u1	-0.02
79) Chrysene-d12	21.680	240	2250592	20.000	ng/u1	-0.03
88) Perylene-d12	25.110	264	2503311	20.000	ng/u1	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	77201	6.229	ng/uL	0.00
4) Pyridine-d5	3.717	84	254541	7.367	ng/u1	0.00
7) Phenol-d5	6.964	99	310637	7.896	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	815560	35.389	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	958744	30.859	ng/u1	0.00
15) 4-Methylphenol-d8	8.487	113	605063	19.829	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	522336	36.860	ng/u1	0.00
24) 2-Nitrophenol-d4	9.663	143	425510	45.747	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.199	165	952675	33.673	ng/u1	0.00
31) 4-Chloroaniline-d4	10.705	131	1194233	26.441	ng/u1	0.00
46) Dimethylphthalate-d6	13.828	166	3226142	36.794	ng/u1	0.00
49) Acenaphthylene-d8	14.116	160	3787999	36.316	ng/u1	0.00
54) 4-Nitrophenol-d4	14.604	143	93558	6.419	ng/u1	0.00
60) Fluorene-d10	15.434	176	2811145	37.045	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.545	200	223793	30.637	ng/u1	0.00
73) Anthracene-d10	17.322	188	4831538	39.868	ng/u1	-0.02
81) Pyrene-d10	19.692	212	5657963	45.380	ng/u1	-0.03
92) Benzo(a)pyrene-d12	24.880	264	5932815	43.610	ng/u1	-0.03
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.346	88	463228	35.321	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
Data File : BP023638.D
Acq On : 17 Jan 2025 22:04
Operator : RC/JU
Sample : Q1086-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF6

Quant Time: Jan 17 23:51:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jan 14 16:27:27 2025
Response via : Initial Calibration

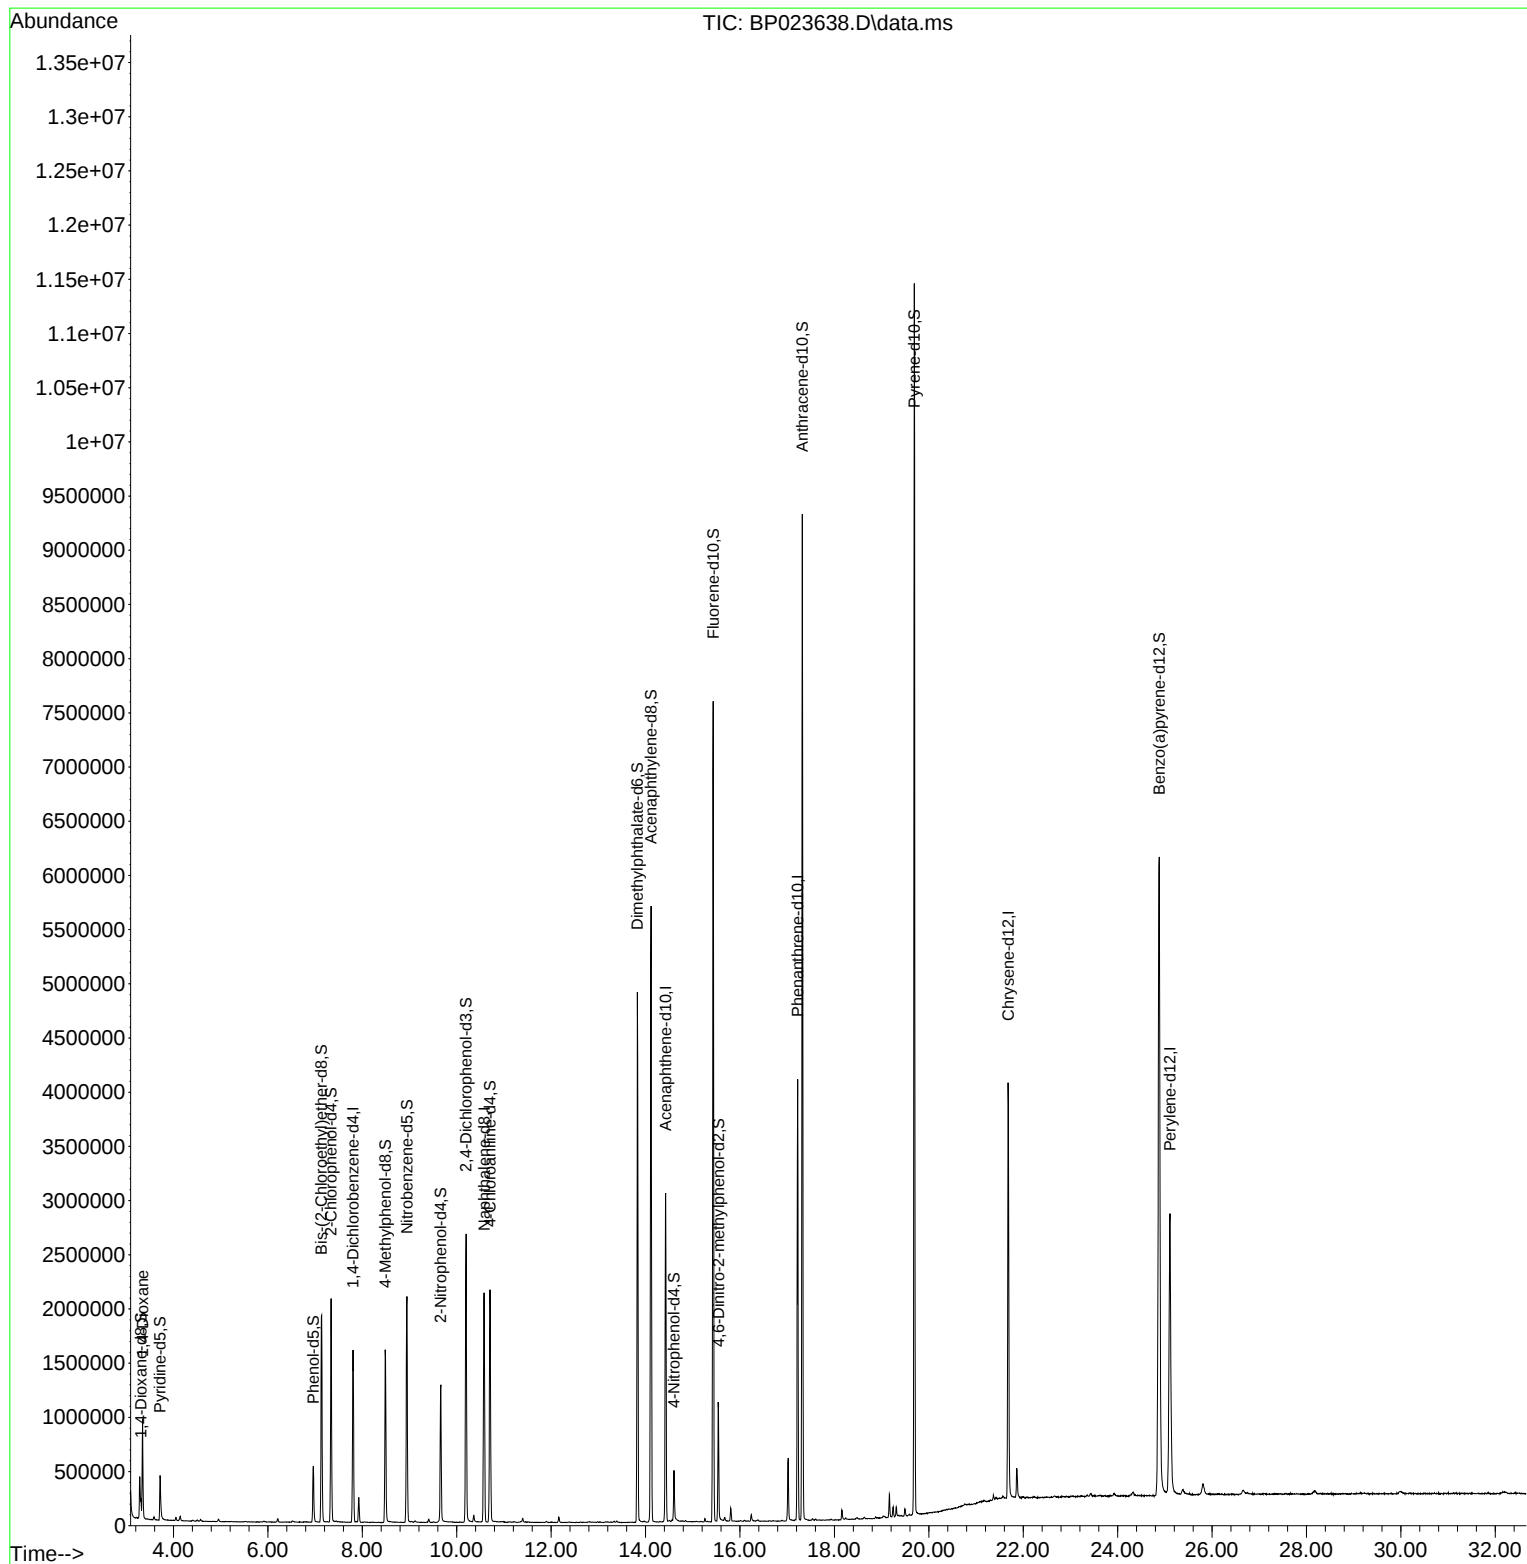

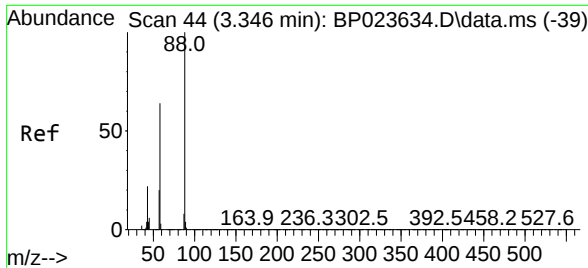

#2
 1,4-Dioxane
 Concen: 35.321 ng/uL
 RT: 3.346 min Scan# 44
 Delta R.T. -0.006 min
 Lab File: BP023638.D
 Acq: 17 Jan 2025 22:04

Instrument :
 BNA_P
 ClientSampleId :
 C0AF6

Tgt Ion: 88 Resp: 463228

Ion	Ratio	Lower	Upper
88	100		
43	22.4	17.3	25.9
58	60.9	47.4	71.0

