

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
 Data File : BP023623.D
 Acq On : 17 Jan 2025 11:16
 Operator : RC/JU
 Sample : Q1086-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.310	34	38	43	rBV	100078	113629	0.93%	0.113%
2	3.716	104	107	124	rBV	251156	419132	3.42%	0.417%
3	4.052	160	164	172	rVB	25032	34117	0.28%	0.034%
4	4.146	176	180	186	rVB3	31890	48668	0.40%	0.048%
5	4.957	313	318	325	rVB2	72953	107353	0.88%	0.107%
6	6.210	526	531	537	rVB2	26462	39783	0.33%	0.040%
7	6.963	653	659	674	rBV	368634	616279	5.04%	0.613%
8	7.140	682	689	701	rBV	1603919	2521550	20.60%	2.509%
9	7.340	716	723	737	rBV	1575129	2406916	19.67%	2.395%
10	7.451	739	742	747	rVB6	9342	14430	0.12%	0.014%
11	7.804	794	802	810	rBV	1337359	2073601	16.94%	2.063%
12	7.869	810	813	819	rVB6	9101	14868	0.12%	0.015%
13	8.492	909	919	933	rBV	1296255	1879819	15.36%	1.871%
14	8.945	986	996	1009	rBV	1640954	2722070	22.24%	2.709%
15	9.122	1022	1026	1034	rVB	7246	13512	0.11%	0.013%
16	9.410	1069	1075	1081	rVB2	25196	40032	0.33%	0.040%
17	9.510	1086	1092	1099	rBV3	28126	47049	0.38%	0.047%
18	9.663	1110	1118	1128	rBV	829407	1322474	10.81%	1.316%
19	10.198	1201	1209	1229	rBV	1903520	3190919	26.07%	3.175%
20	10.581	1264	1274	1282	rBV	1859125	2989079	24.42%	2.974%
21	10.704	1287	1295	1310	rBV	1062312	1858475	15.19%	1.849%
22	11.904	1495	1499	1505	rBV7	7806	12805	0.10%	0.013%
23	12.169	1538	1544	1552	rVB2	36181	61881	0.51%	0.062%
24	13.828	1820	1826	1838	rBV	3858999	5417556	44.27%	5.391%
25	14.116	1865	1875	1886	rBV	4817192	6890343	56.30%	6.857%
26	14.427	1920	1928	1936	rBV	2661328	4029830	32.93%	4.010%
27	14.598	1950	1957	1971	rBV	221607	398961	3.26%	0.397%
28	14.845	1995	1999	2008	rVB9	8928	18096	0.15%	0.018%
29	15.263	2065	2070	2074	rBV3	13914	19187	0.16%	0.019%
30	15.433	2092	2099	2111	rBV	5964373	8685160	70.97%	8.643%
31	15.539	2111	2117	2130	rBV	683574	943333	7.71%	0.939%
32	15.680	2137	2141	2146	rVB3	25483	39031	0.32%	0.039%
33	15.804	2155	2162	2168	rBV	325799	431316	3.52%	0.429%
34	16.221	2231	2233	2239	rVB7	7127	12356	0.10%	0.012%
35	16.998	2361	2365	2372	rVB5	14168	26012	0.21%	0.026%
36	17.221	2396	2403	2412	rBV2	3329304	4661640	38.09%	4.639%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
Data File : BP023623.D
Acq On : 17 Jan 2025 11:16
Operator : RC/JU
Sample : Q1086-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Title : SVOA CALIBRATION

37	17.321	2413	2420	2431	rVV	7559262	10233936	83.62%	10.184%
38	18.163	2558	2563	2571	rBV2	194164	269323	2.20%	0.268%
39	18.480	2611	2617	2624	rBV10	12862	31571	0.26%	0.031%
40	18.633	2639	2643	2653	rBV10	13714	26702	0.22%	0.027%
41	19.245	2742	2747	2753	rBV	71164	114405	0.93%	0.114%
42	19.315	2755	2759	2765	rVV	66372	94706	0.77%	0.094%
43	19.498	2785	2790	2796	rBV	204306	253160	2.07%	0.252%
44	19.692	2816	2823	2833	rBV	8771061	12183713	99.55%	12.124%
45	21.362	3103	3107	3114	rBV3	91524	133246	1.09%	0.133%
46	21.680	3154	3161	3178	rBV2	3164313	5271802	43.08%	5.246%
47	24.862	3693	3702	3729	rBV	4895903	12238445	100.00%	12.179%
48	25.097	3733	3742	3761	rVB	1885962	5518251	45.09%	5.491%




Sum of corrected areas: 100490522

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
Data File : BP023623.D
Acq On : 17 Jan 2025 11:16
Operator : RC/JU
Sample : Q1086-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

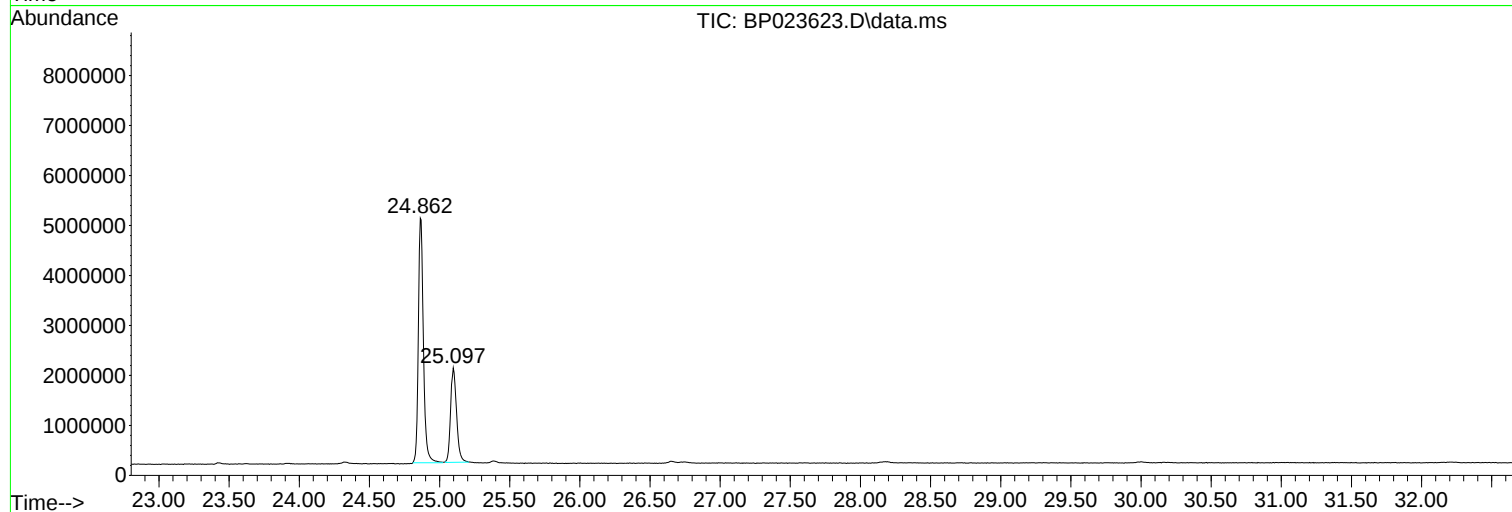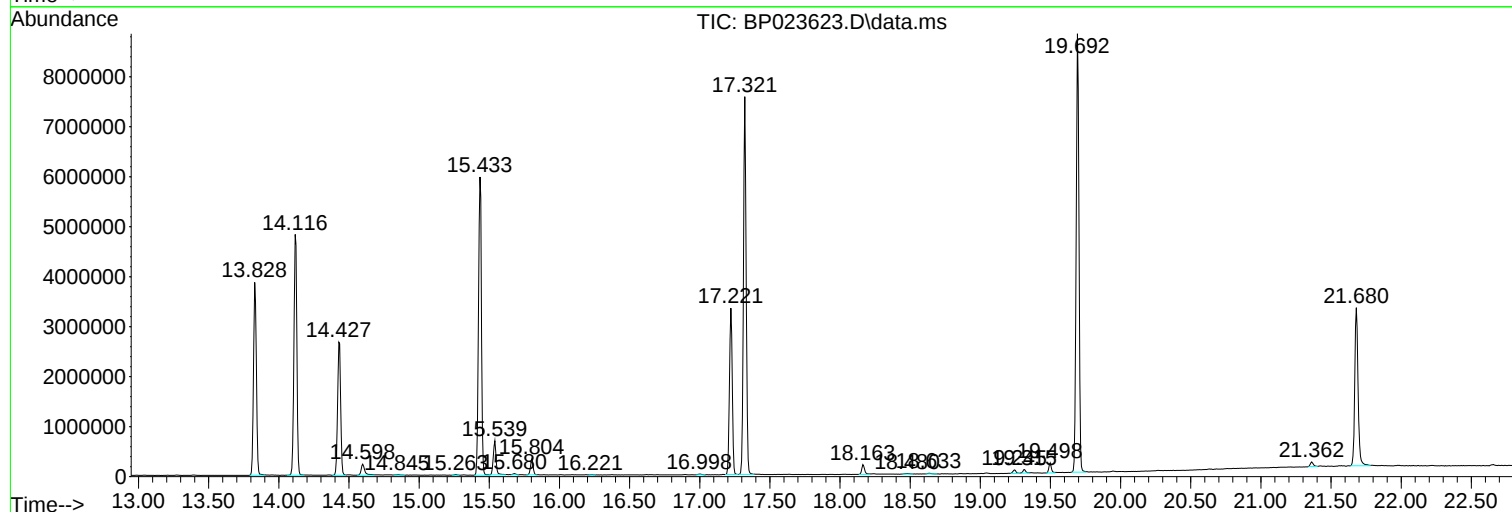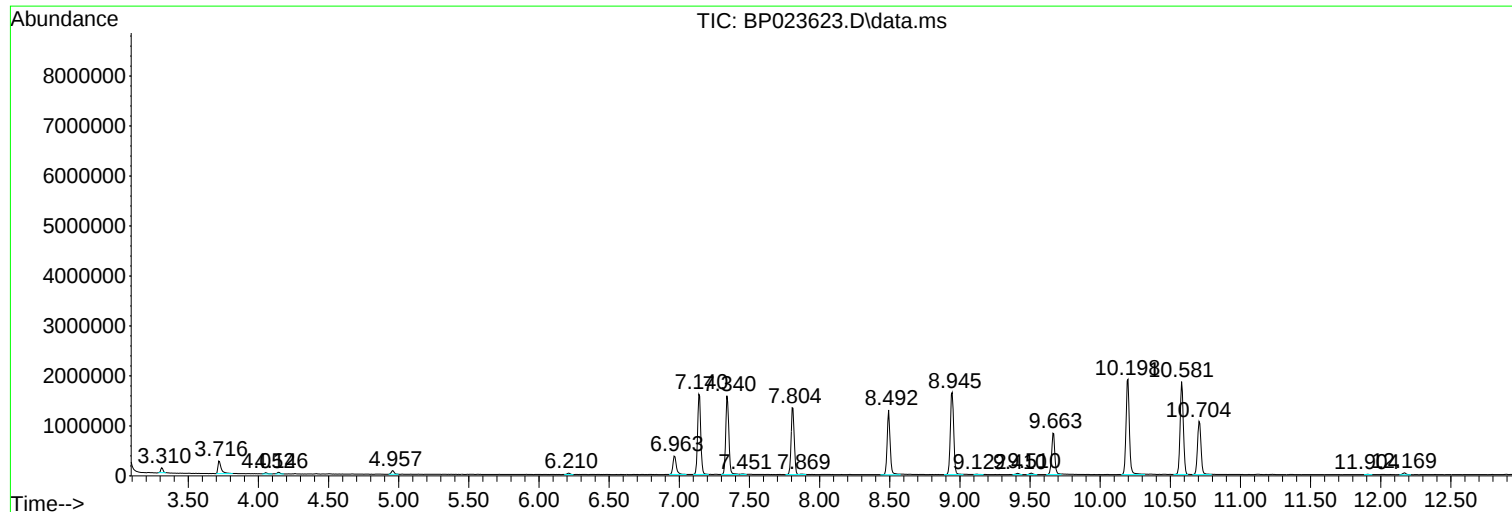

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
Data File : BP023623.D
Acq On : 17 Jan 2025 11:16
Operator : RC/JU
Sample : Q1086-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
Data File : BP023623.D
Acq On : 17 Jan 2025 11:16
Operator : RC/JU
Sample : Q1086-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
