

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
 Data File : BP023645.D
 Acq On : 18 Jan 2025 02:50
 Operator : RC/JU
 Sample : Q1088-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	34	38	48	rVB	160658	228600	1.22%	0.152%
2	3.893	133	137	142	rVB3	22775	30611	0.16%	0.020%
3	4.058	161	165	169	rVB	27517	36204	0.19%	0.024%
4	4.146	176	180	186	rVB	52130	75456	0.40%	0.050%
5	4.499	237	240	245	rVB	16486	20593	0.11%	0.014%
6	4.570	250	252	261	rVB7	17252	32600	0.17%	0.022%
7	4.958	313	318	323	rVB2	34222	51978	0.28%	0.035%
8	6.211	525	531	543	rVB2	76849	136149	0.73%	0.091%
9	6.646	600	605	609	rBV3	19138	29542	0.16%	0.020%
10	6.775	623	627	633	rBV6	16665	29356	0.16%	0.020%
11	6.964	653	659	674	rBV	1110851	1757967	9.41%	1.169%
12	7.140	682	689	700	rBV	2561862	3985188	21.33%	2.650%
13	7.340	715	723	733	rBV	2957670	4646226	24.87%	3.090%
14	7.811	795	803	810	rBV	1690916	2521747	13.50%	1.677%
15	8.493	912	919	931	rBV	2900681	4291254	22.97%	2.854%
16	8.593	933	936	941	rVB5	14386	22759	0.12%	0.015%
17	8.946	988	996	1007	rBV	2782319	4467584	23.91%	2.971%
18	9.040	1007	1012	1020	rVV5	29312	63860	0.34%	0.042%
19	9.122	1022	1026	1031	rVB3	31198	46765	0.25%	0.031%
20	9.410	1069	1075	1080	rVB	46663	67063	0.36%	0.045%
21	9.669	1110	1119	1133	rBV	2012218	3315412	17.75%	2.205%
22	10.010	1172	1177	1182	rVB3	31093	51916	0.28%	0.035%
23	10.199	1200	1209	1225	rBV	3532577	5773372	30.90%	3.840%
24	10.375	1234	1239	1246	rVB6	22425	40741	0.22%	0.027%
25	10.581	1266	1274	1282	rBV	2081361	3580437	19.17%	2.381%
26	10.646	1282	1285	1289	rVB3	18432	21615	0.12%	0.014%
27	10.705	1289	1295	1304	rBV	157031	290882	1.56%	0.193%
28	10.981	1337	1342	1347	rBV2	30119	44400	0.24%	0.030%
29	11.187	1370	1377	1381	rBV3	22799	40422	0.22%	0.027%
30	11.387	1399	1411	1418	rBV	179906	316776	1.70%	0.211%
31	11.710	1460	1466	1471	rBV9	10280	21776	0.12%	0.014%
32	11.981	1505	1512	1514	rVV6	16314	33601	0.18%	0.022%
33	12.004	1514	1516	1523	rVB6	14313	22008	0.12%	0.015%
34	12.169	1537	1544	1551	rBV	55773	104802	0.56%	0.070%
35	13.393	1747	1752	1759	rVB2	20715	33683	0.18%	0.022%
36	13.481	1763	1767	1773	rVB	47795	69147	0.37%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
 Data File : BP023645.D
 Acq On : 18 Jan 2025 02:50
 Operator : RC/JU
 Sample : Q1088-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Title : SVOA CALIBRATION

37	13.834	1820	1827	1844	rBV	6158698	8810454	47.16%	5.860%
38	14.122	1865	1876	1887	rBV	7180346	11130371	59.58%	7.403%
39	14.434	1921	1929	1936	rBV	3027376	4666985	24.98%	3.104%
40	14.610	1950	1959	1982	rBV	1078615	1809224	9.68%	1.203%
41	14.863	1997	2002	2007	rVB7	11854	20715	0.11%	0.014%
42	15.275	2068	2072	2077	rBV2	51779	69271	0.37%	0.046%
43	15.440	2093	2100	2112	rBV	9454431	14178517	75.90%	9.430%
44	15.551	2112	2119	2137	rVV	1762755	2425147	12.98%	1.613%
45	15.687	2137	2142	2150	rVB	44891	80642	0.43%	0.054%
46	15.822	2161	2165	2170	rBV4	18514	28551	0.15%	0.019%
47	16.245	2233	2237	2245	rVB8	10037	19346	0.10%	0.013%
48	16.828	2331	2336	2341	rBV	55824	86933	0.47%	0.058%
49	16.910	2346	2350	2355	rVB7	11437	18820	0.10%	0.013%
50	17.010	2363	2367	2374	rVB3	18042	33053	0.18%	0.022%
51	17.239	2399	2406	2415	rBV	3828726	5429563	29.06%	3.611%
52	17.334	2415	2422	2434	rVV	10910195	15201759	81.37%	10.110%
53	17.569	2456	2462	2466	rBV2	53524	93553	0.50%	0.062%
54	18.181	2561	2566	2573	rBV2	88031	134128	0.72%	0.089%
55	18.251	2575	2578	2583	rVB	21809	28686	0.15%	0.019%
56	18.645	2643	2645	2649	rVB5	20236	27229	0.15%	0.018%
57	19.257	2745	2749	2754	rBV2	121316	157972	0.85%	0.105%
58	19.322	2756	2760	2767	rVV	109544	153979	0.82%	0.102%
59	19.504	2787	2791	2796	rBV3	94097	124313	0.67%	0.083%
60	19.698	2819	2824	2838	rVB	14408904	18339158	98.17%	12.197%
61	21.680	3155	3161	3172	rBV	4012668	5921285	31.70%	3.938%
62	24.857	3692	3701	3727	rBV	7258151	18681190	100.00%	12.424%
63	25.092	3732	3741	3761	rVB	2379299	6385501	34.18%	4.247%




Sum of corrected areas: 150358837

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
Data File : BP023645.D
Acq On : 18 Jan 2025 02:50
Operator : RC/JU
Sample : Q1088-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

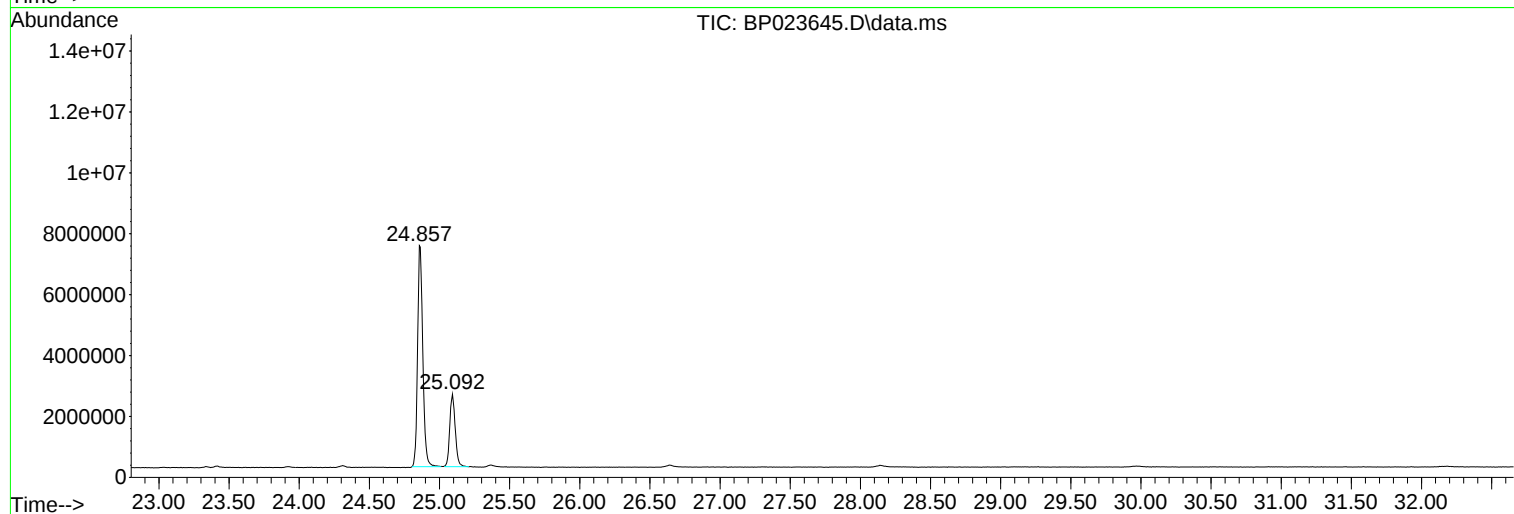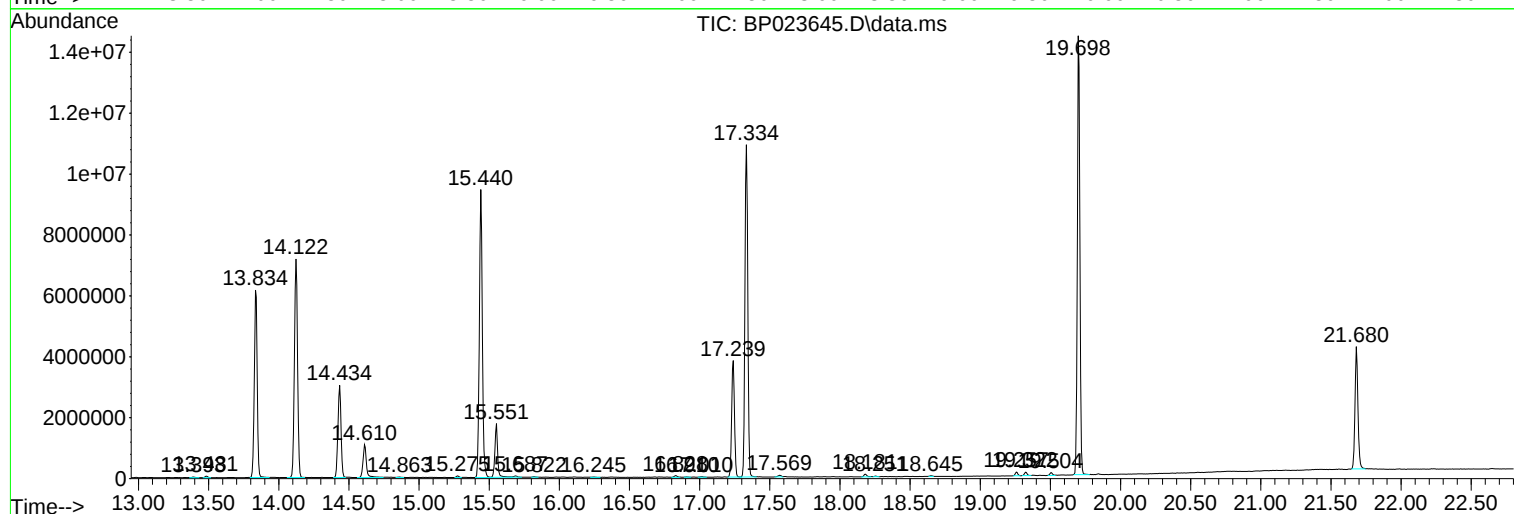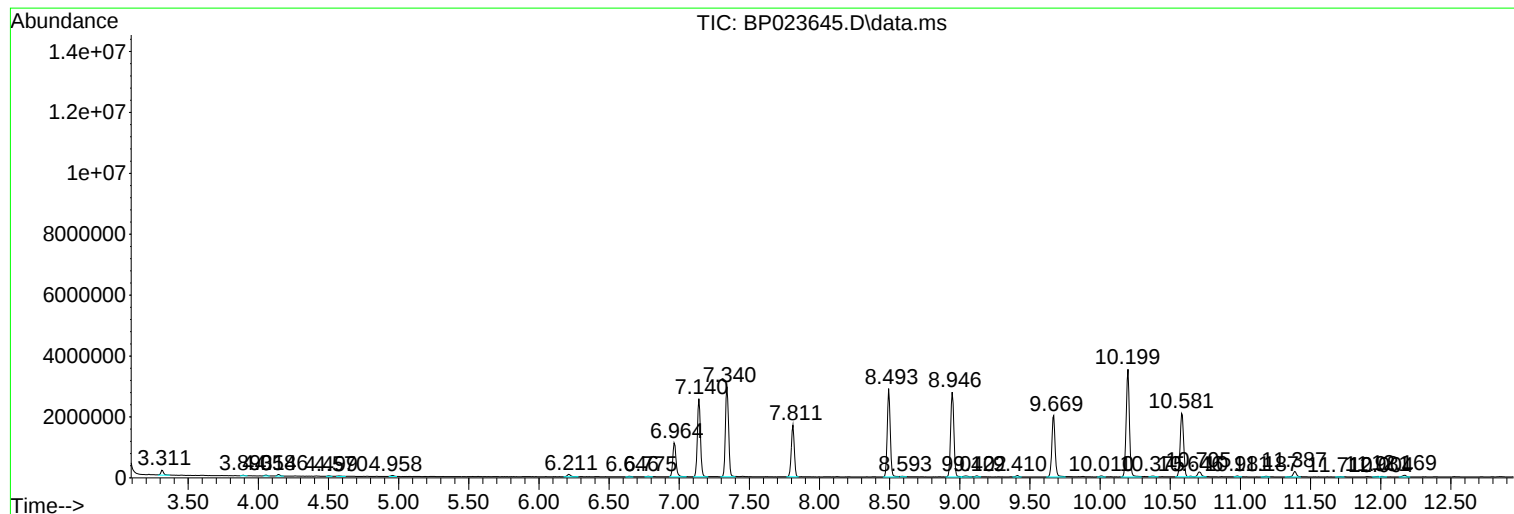

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
Data File : BP023645.D
Acq On : 18 Jan 2025 02:50
Operator : RC/JU
Sample : Q1088-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011725\
Data File : BP023645.D
Acq On : 18 Jan 2025 02:50
Operator : RC/JU
Sample : Q1088-08
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
