

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011822\
 Data File : BP008835.D
 Acq On : 18 Jan 2022 11:56
 Operator : CG/JU
 Sample : PB142032BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB142032BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	8	11	21	rVB	189957	258183	1.18%	0.302%
2	5.440	410	417	438	rBV	4878209	7586682	34.72%	8.864%
3	7.034	680	688	708	rBV	4408537	7620334	34.87%	8.903%
4	7.852	820	827	842	rBV	1047964	1703541	7.80%	1.990%
5	9.010	1015	1024	1047	rBV	2853048	5012346	22.94%	5.856%
6	10.651	1295	1303	1321	rBV	1290793	2356769	10.78%	2.753%
7	13.116	1713	1722	1739	rBV	8747199	13085953	59.88%	15.289%
8	14.492	1947	1956	1972	rBV	2191202	3357485	15.36%	3.923%
9	15.986	2202	2210	2240	rBV	6359734	10110754	46.27%	11.813%
10	17.245	2417	2424	2437	rBV	2768044	4196349	19.20%	4.903%
11	19.810	2854	2860	2875	rBV	17875968	21853072	100.00%	25.531%
12	21.339	3115	3120	3127	rBV	3426334	4424277	20.25%	5.169%
13	23.757	3525	3531	3541	rVB2	1944891	4026954	18.43%	4.705%


Sum of corrected areas: 85592699

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011822\
Data File : BP008835.D
Acq On : 18 Jan 2022 11:56
Operator : CG/JU
Sample : PB142032BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142032BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

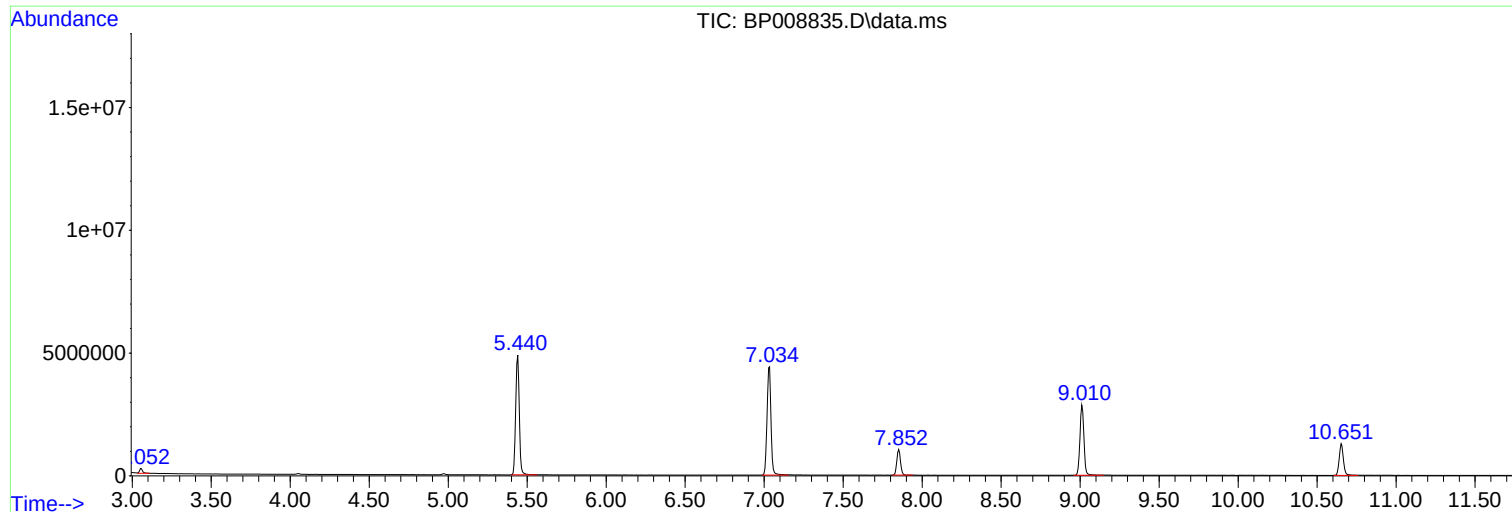

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011822\
Data File : BP008835.D
Acq On : 18 Jan 2022 11:56
Operator : CG/JU
Sample : PB142032BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142032BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.052	3.03 ng	258183	1,4-Dichlorobenzene-d4	7.852

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

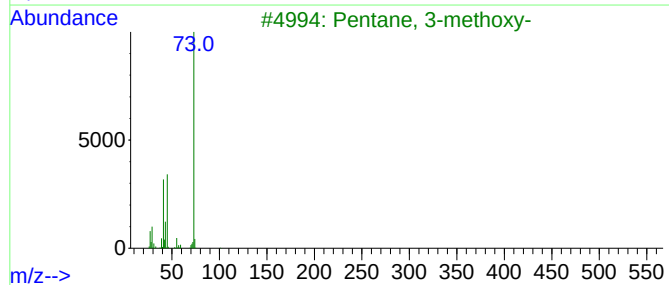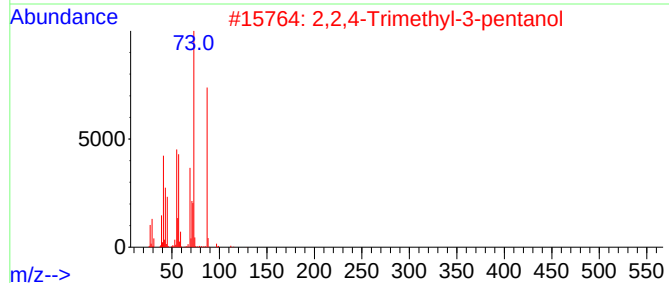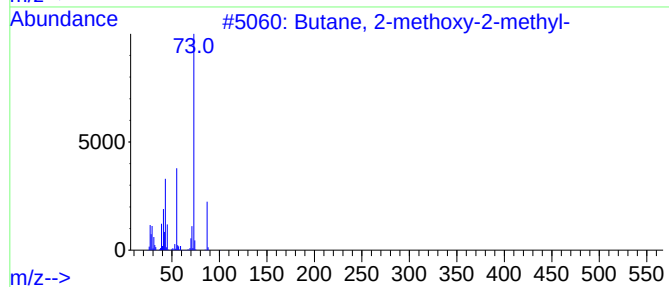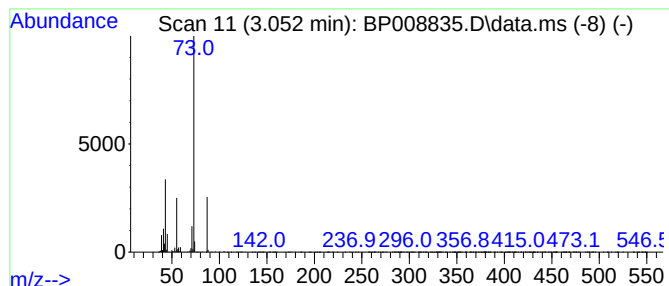

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011822\
Data File : BP008835.D
Acq On : 18 Jan 2022 11:56
Operator : CG/JU
Sample : PB142032BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB142032BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.052	3.0	ng	258183	1	7.852	1703540	20.0