

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013498.D
 Acq On : 17 Jan 2023 17:22
 Operator : CG/JU
 Sample : PB150265BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK265

Quant Time: Jan 18 01:15:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	364560	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	1494899	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164	939712	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	2016108	20.000	ng/ul	0.00
79) Chrysene-d12	21.398	240	1835273	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264	2184696	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	51972	5.541	ng/uL	0.00
4) Pyridine-d5	3.723	84	547937	20.946	ng/ul	0.00
7) Phenol-d5	7.064	99	862990	28.528	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	554116	29.035	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	702926	31.159	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	676214	29.341	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128	338994	31.848	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143	393292	33.754	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	682009	29.371	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131	710964	21.734	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	2092561	30.564	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	2311618	30.502	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	308762	24.638	ng/ul	0.00
60) Fluorene-d10	15.545	176	1780253	29.438	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	345161	27.000	ng/ul	0.00
73) Anthracene-d10	17.404	188	2808799	31.520	ng/ul	0.00
81) Pyrene-d10	19.645	212	3225246	32.300	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	3330790	31.038	ng/ul	0.00
Target Compounds						
78) Di-n-butylphthalate	18.257	149	294021	3.269	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013498.D
Acq On : 17 Jan 2023 17:22
Operator : CG/JU
Sample : PB150265BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK265

Quant Time: Jan 18 01:15:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

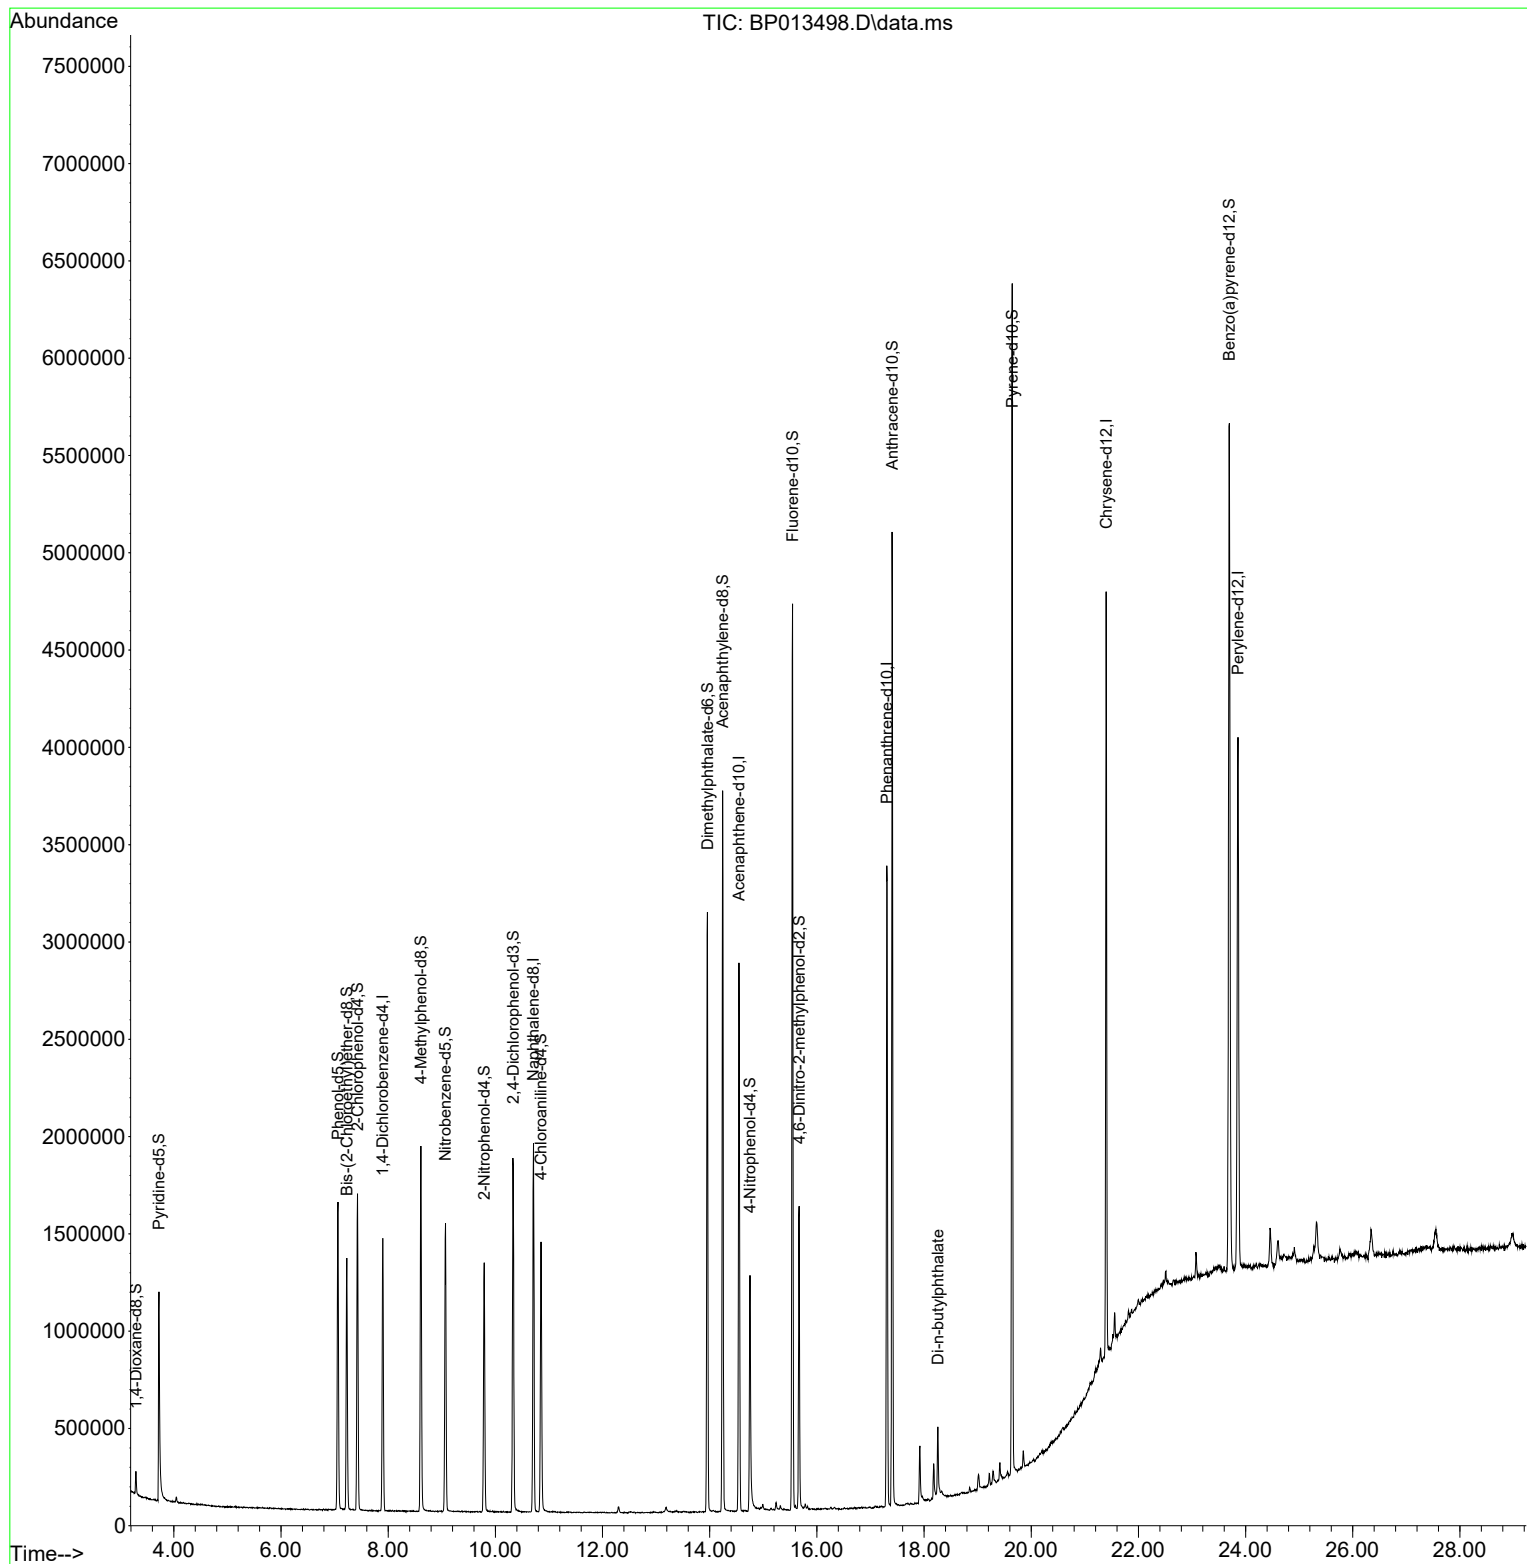

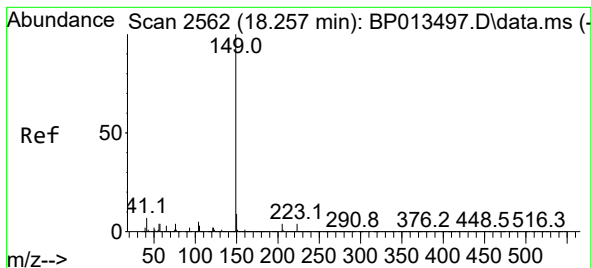

#78

Di-n-butylphthalate

Concen: 3.269 ng/ul

RT: 18.257 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP013498.D


Acq: 17 Jan 2023 17:22

Instrument :

BNA_P

ClientSampleId :

SBLK265

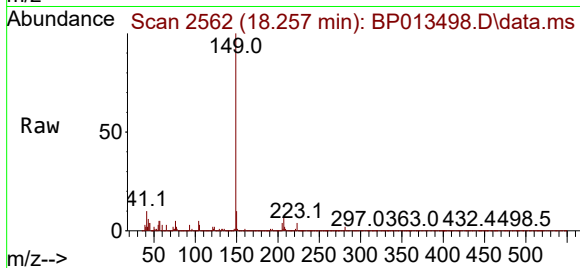

Tgt Ion:149 Resp: 294021

Ion Ratio Lower Upper

149 100

150 9.6 7.1 10.7

104 4.7 4.3 6.5

