

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013499.D
 Acq On : 17 Jan 2023 17:56
 Operator : CG/JU
 Sample : 01145-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W6

Quant Time: Jan 18 01:15:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	457408	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	1912977	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.551	164	1163399	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	2615074	20.000	ng/ul	0.00
79) Chrysene-d12	21.398	240	2358740	20.000	ng/ul	0.00
88) Perylene-d12	23.856	264	2893760	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	32763	2.784	ng/uL	0.00
4) Pyridine-d5	3.740	84	39304	1.197	ng/ul	0.02
7) Phenol-d5	7.063	99	569725	15.010	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	369088	15.414	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	468030	16.535	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	429289	14.846	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128	223544	16.412	ng/ul	0.00
24) 2-Nitrophenol-d4	9.792	143	257804	17.290	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	459470	15.463	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	526702	12.582	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1382761	16.314	ng/ul	0.00
49) Acenaphthylene-d8	14.239	160	1562587	16.654	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	162974	10.504	ng/ul	0.00
60) Fluorene-d10	15.545	176	1220708	16.305	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	187153	11.287	ng/ul	0.00
73) Anthracene-d10	17.410	188	1780852	15.407	ng/ul	0.00
81) Pyrene-d10	19.645	212	2210748	17.226	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.698	264	2418391	17.014	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.734	105	54874	1.202	ng/ul	97
78) Di-n-butylphthalate	18.257	149	207793	1.781	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.292	149	196542	2.988	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013499.D
Acq On : 17 Jan 2023 17:56
Operator : CG/JU
Sample : 01145-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W6

Quant Time: Jan 18 01:15:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration




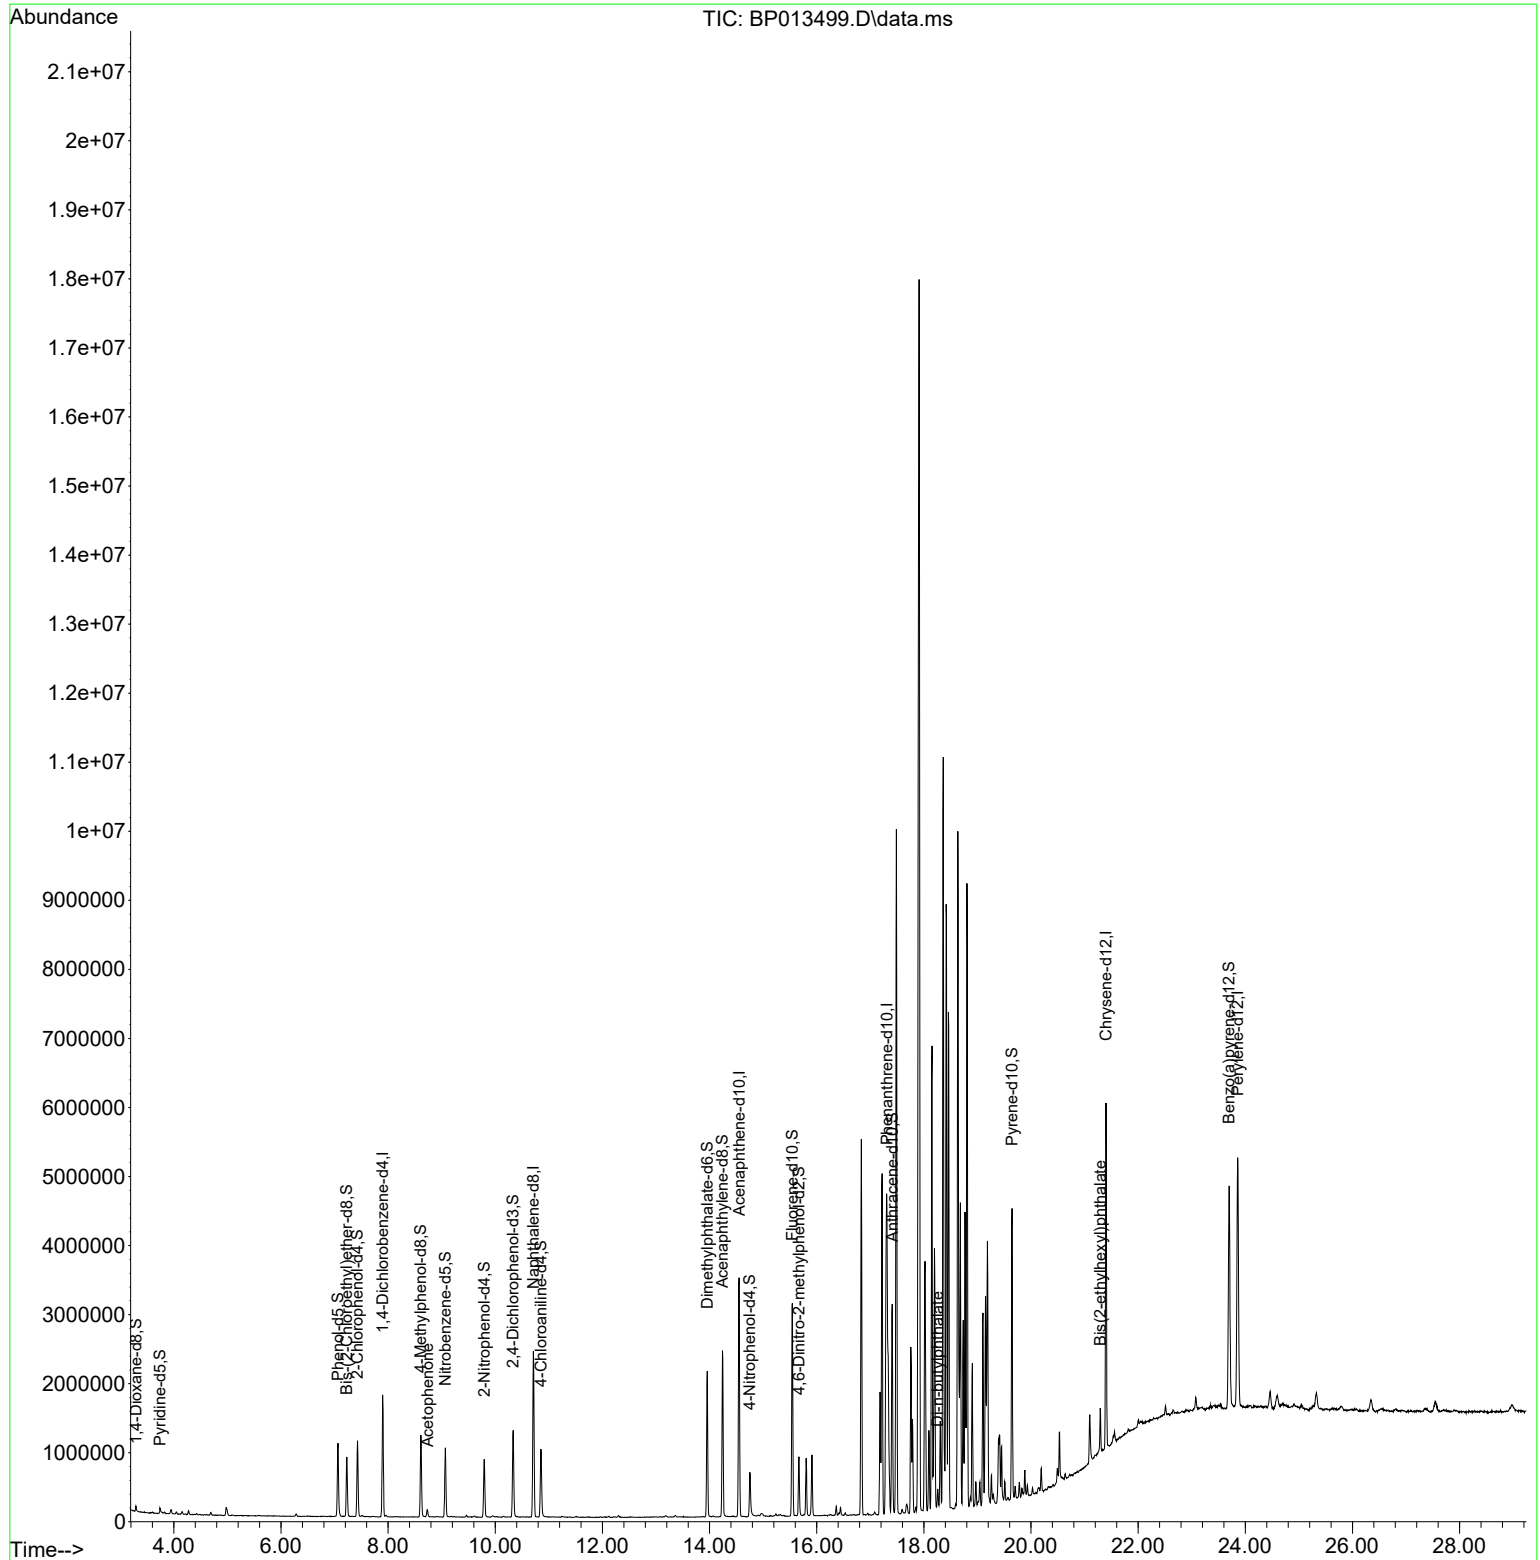


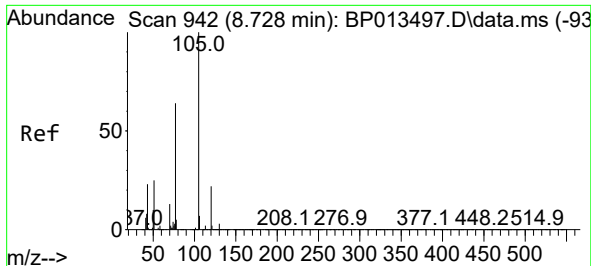

#16
Acetophenone
Concen: 1.202 ng/ul
RT: 8.734 min Scan# 942
Delta R.T. 0.005 min
Lab File: BP013499.D
Acq: 17 Jan 2023 17:56




Instrument :
BNA_P
ClientSampleId :
A43W6


Tgt Ion:105 Resp: 54874
Ion Ratio Lower Upper
105 100
77 74.1 62.5 93.7
51 30.8 24.7 37.1

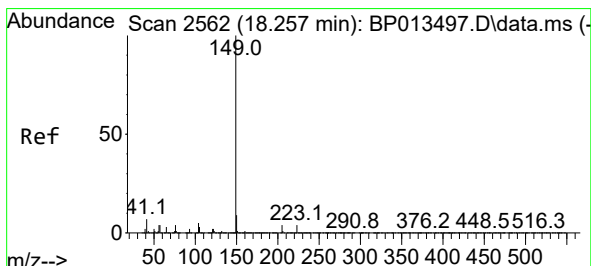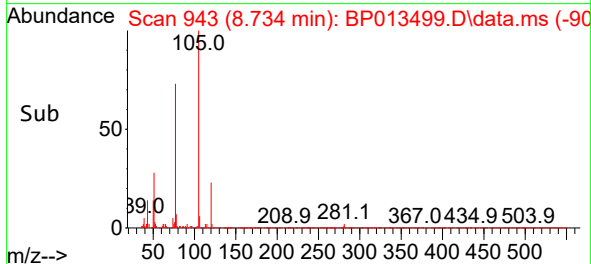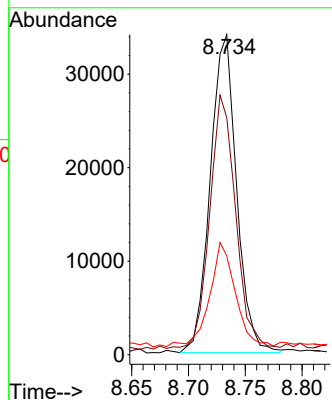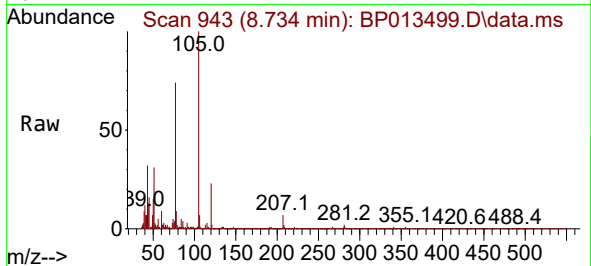

#78
Di-n-butylphthalate
Concen: 1.781 ng/ul
RT: 18.257 min Scan# 2562
Delta R.T. -0.000 min
Lab File: BP013499.D
Acq: 17 Jan 2023 17:56

Tgt Ion:149 Resp: 207793
Ion Ratio Lower Upper
149 100
150 8.8 7.1 10.7
104 5.4 4.3 6.5

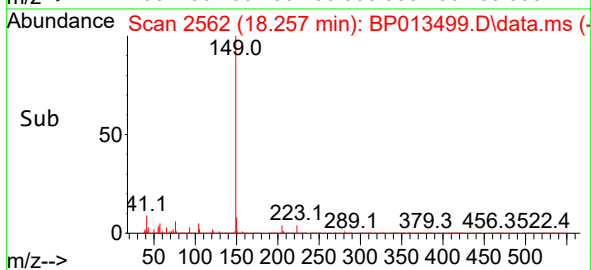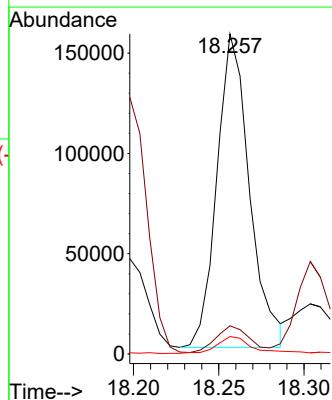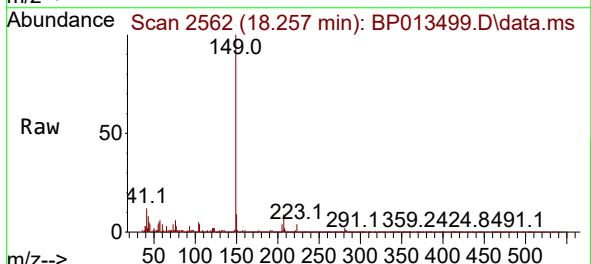

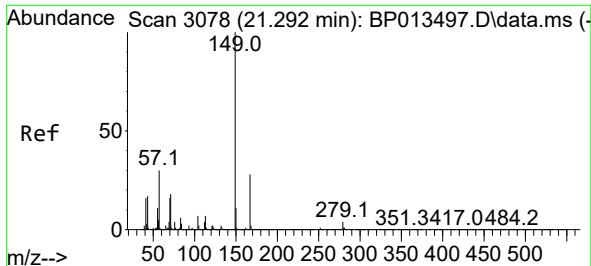

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.988 ng/ul
 RT: 21.292 min Scan# 3078
 Delta R.T. -0.000 min
 Lab File: BP013499.D
 Acq: 17 Jan 2023 17:56

Instrument :
 BNA_P
 ClientSampleId :
 A43W6

Tgt Ion:149 Resp: 196542
 Ion Ratio Lower Upper
 149 100
 167 29.1 22.2 33.4
 279 4.8 3.5 5.3

