

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013500.D
 Acq On : 17 Jan 2023 18:31
 Operator : CG/JU
 Sample : 01145-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43W0

Quant Time: Jan 18 01:16:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	406885	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	1692594	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.546	164	1062107	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.310	188	2284780	20.000	ng/ul	0.00
79) Chrysene-d12	21.398	240	2204708	20.000	ng/ul	0.00
88) Perylene-d12	23.857	264	2651867	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	32862	3.139	ng/uL	0.00
4) Pyridine-d5	3.746	84	33284	1.140	ng/ul	0.02
7) Phenol-d5	7.064	99	571580	16.929	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	372476	17.487	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	471362	18.721	ng/ul	0.00
15) 4-Methylphenol-d8	8.611	113	421190	16.374	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128	224878	18.660	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143	256130	19.415	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	446904	16.998	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131	533963	14.416	ng/ul	0.00
46) Dimethylphthalate-d6	13.957	166	1347559	17.414	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	1510625	17.636	ng/ul	0.00
54) 4-Nitrophenol-d4	14.757	143	160526	11.333	ng/ul	0.00
60) Fluorene-d10	15.540	176	1183538	17.316	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	177116	12.226	ng/ul	0.00
73) Anthracene-d10	17.404	188	1758118	17.409	ng/ul	0.00
81) Pyrene-d10	19.645	212	2294307	19.127	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.692	264	2449589	18.805	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.734	105	45950	1.132	ng/ul	98
78) Di-n-butylphthalate	18.257	149	202231	1.984	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.292	149	3264170	53.086	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013500.D
Acq On : 17 Jan 2023 18:31
Operator : CG/JU
Sample : 01145-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43W0

Quant Time: Jan 18 01:16:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration




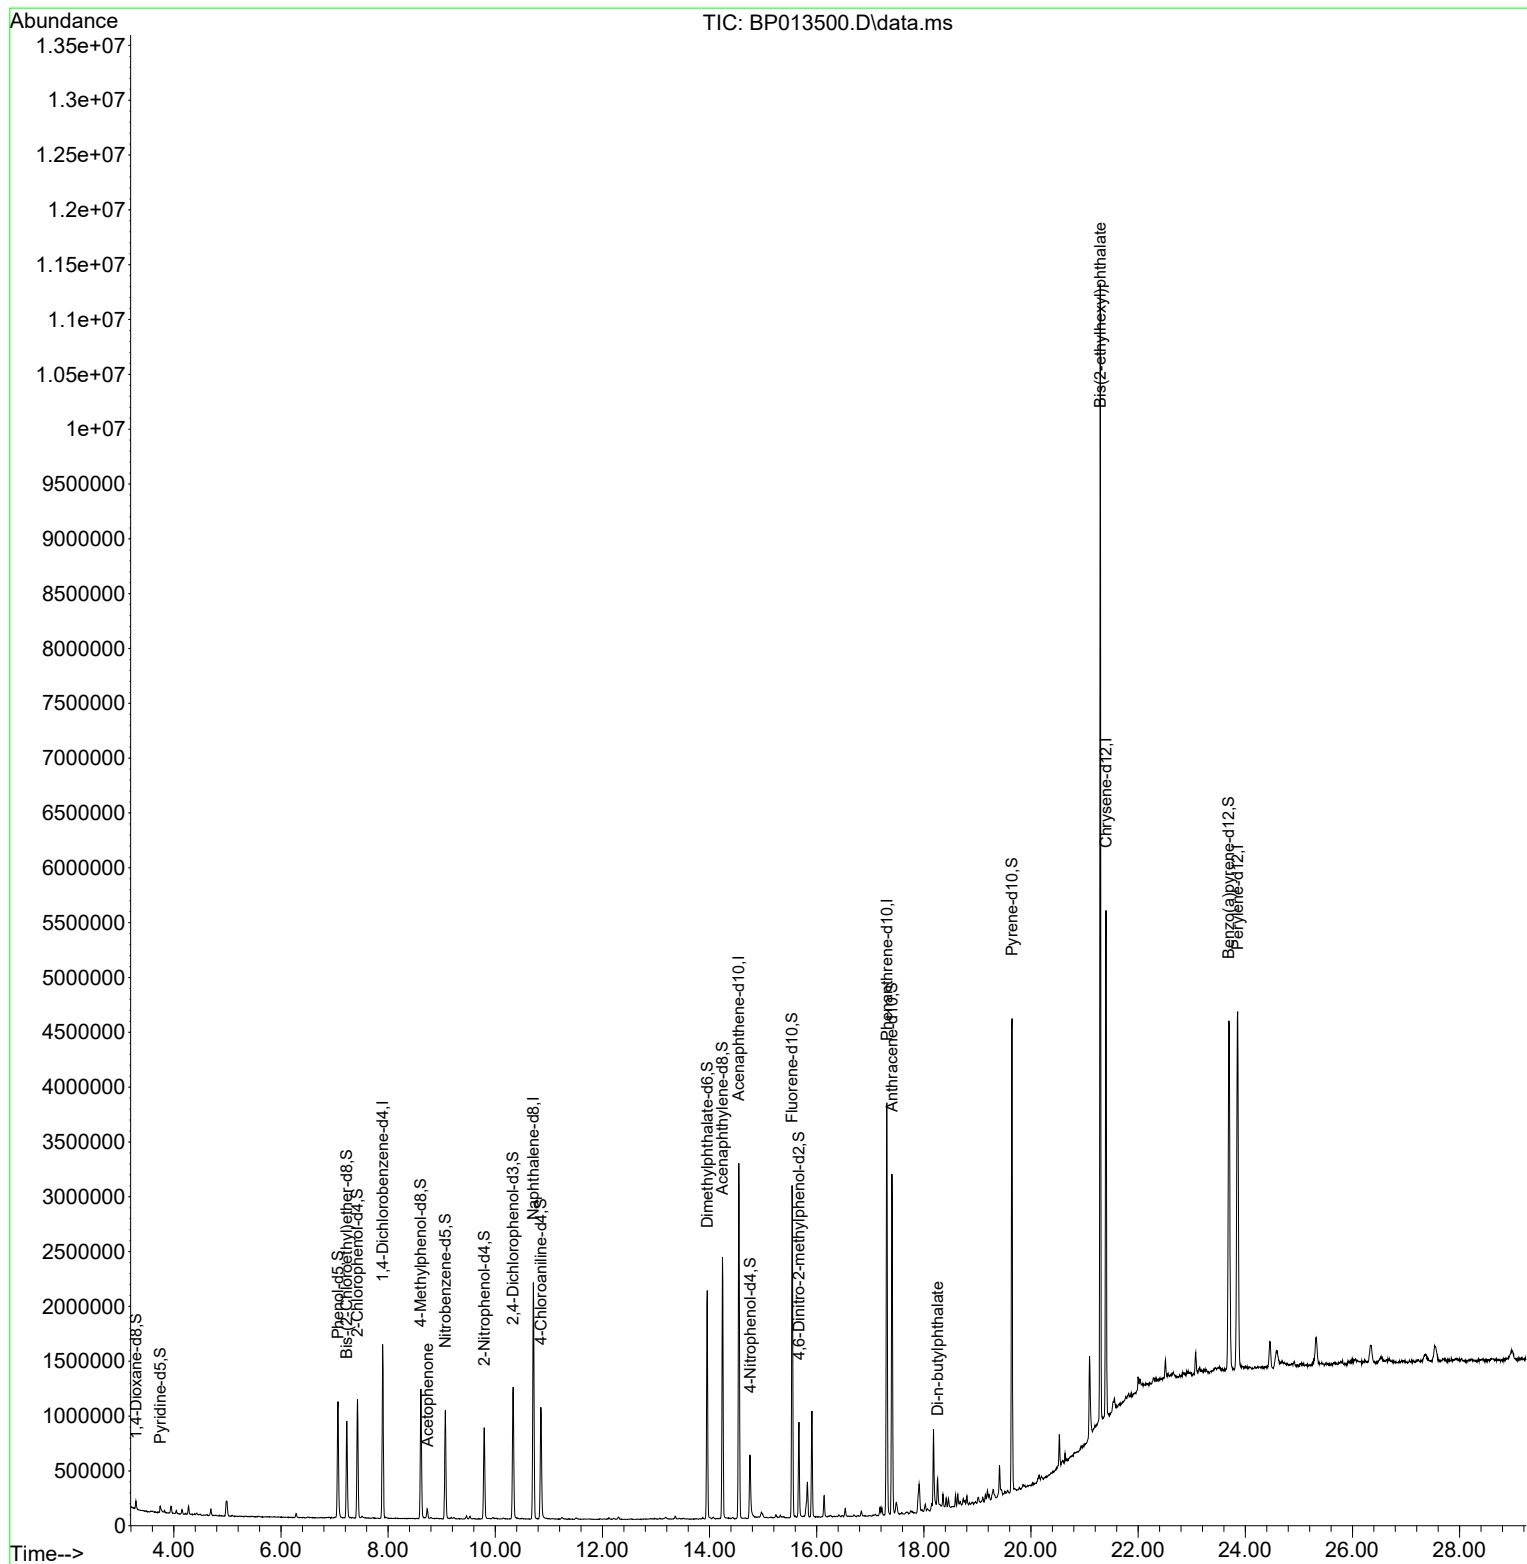


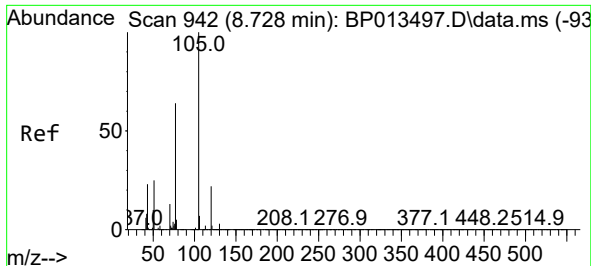

#16
Acetophenone
Concen: 1.132 ng/ul
RT: 8.734 min Scan# 942
Delta R.T. 0.006 min
Lab File: BP013500.D
Acq: 17 Jan 2023 18:31




Instrument :
BNA_P
ClientSampleId :
A43W0


Tgt Ion:105 Resp: 45950
Ion Ratio Lower Upper
105 100
77 77.3 62.5 93.7
51 33.2 24.7 37.1

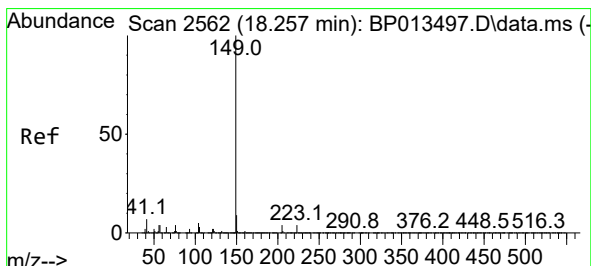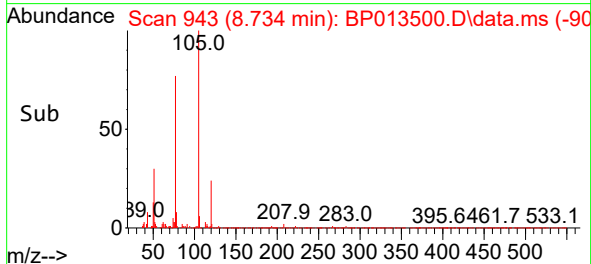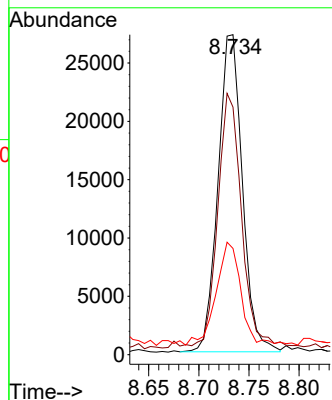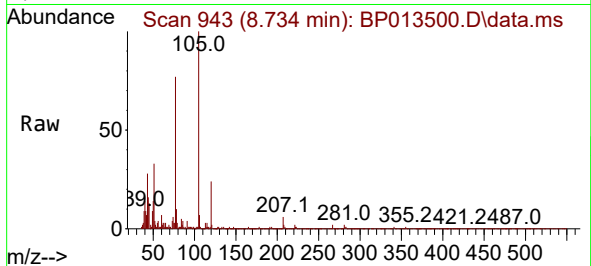

#78
Di-n-butylphthalate
Concen: 1.984 ng/ul
RT: 18.257 min Scan# 2562
Delta R.T. 0.000 min
Lab File: BP013500.D
Acq: 17 Jan 2023 18:31

Tgt Ion:149 Resp: 202231
Ion Ratio Lower Upper
149 100
150 9.2 7.1 10.7
104 5.1 4.3 6.5

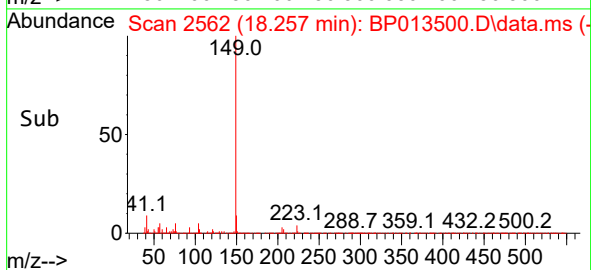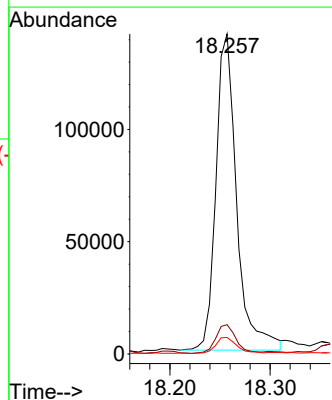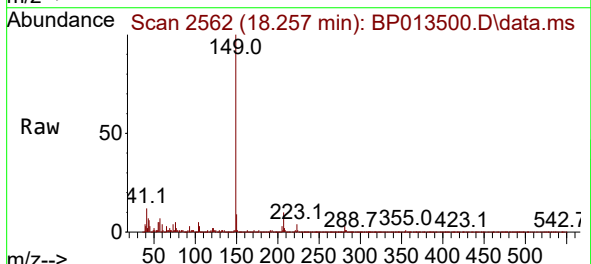

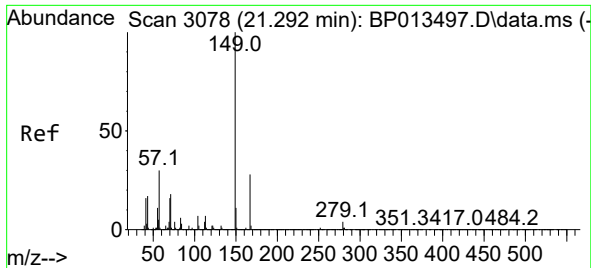

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 53.086 ng/ul
 RT: 21.292 min Scan# 3078
 Delta R.T. 0.000 min
 Lab File: BP013500.D
 Acq: 17 Jan 2023 18:31

Instrument :
 BNA_P
 ClientSampleId :
 A43W0

Tgt Ion:149 Resp: 3264170
 Ion Ratio Lower Upper
 149 100
 167 28.0 22.2 33.4
 279 4.6 3.5 5.3

