

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP011823\  
 Data File : BP013524.D  
 Acq On : 18 Jan 2023 16:29  
 Operator : CG/JU  
 Sample : 01145-02DL 30X  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A43S7DL

Quant Time: Jan 19 01:46:49 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP010523.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Jan 18 01:06:35 2023  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| -----                         |        |      |          |        |       |          |
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.899  | 152  | 434218   | 20.000 | ng/ul | 0.00     |
| 20) Naphthalene-d8            | 10.710 | 136  | 1822765  | 20.000 | ng/ul | 0.00     |
| 38) Acenaphthene-d10          | 14.546 | 164  | 1095015  | 20.000 | ng/ul | 0.00     |
| 64) Phenanthrene-d10          | 17.304 | 188  | 2170399  | 20.000 | ng/ul | 0.00     |
| 79) Chrysene-d12              | 21.392 | 240  | 1864103  | 20.000 | ng/ul | 0.00     |
| 88) Perylene-d12              | 23.845 | 264  | 2373784  | 20.000 | ng/ul | -0.01    |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 3.293  | 96   | 1505     | 0.135  | ng/uL | 0.00     |
| 4) Pyridine-d5                | 3.711  | 84   | 655      | 0.021  | ng/ul | -0.01    |
| 7) Phenol-d5                  | 7.064  | 99   | 19612    | 0.544  | ng/ul | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.228  | 67   | 13761    | 0.605  | ng/ul | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.428  | 132  | 15584    | 0.580  | ng/ul | 0.00     |
| 15) 4-Methylphenol-d8         | 8.616  | 113  | 13308    | 0.485  | ng/ul | 0.00     |
| 21) Nitrobenzene-d5           | 9.069  | 128  | 6353     | 0.490  | ng/ul | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.793  | 143  | 7386     | 0.520  | ng/ul | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.463 | 165  | 163      | 0.006  | ng/ul | 0.13     |
| 31) 4-Chloroaniline-d4        | 10.863 | 131  | 13818    | 0.346  | ng/ul | 0.01     |
| 46) Dimethylphthalate-d6      | 13.957 | 166  | 50576    | 0.634  | ng/ul | 0.00     |
| 49) Acenaphthylene-d8         | 14.240 | 160  | 53543    | 0.606  | ng/ul | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.746 | 143  | 38       | 0.003  | ng/ul | 0.00     |
| 60) Fluorene-d10              | 15.540 | 176  | 45674    | 0.648  | ng/ul | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.675 | 200  | 4122     | 0.300  | ng/ul | 0.00     |
| 73) Anthracene-d10            | 17.404 | 188  | 65499    | 0.683  | ng/ul | 0.00     |
| 81) Pyrene-d10                | 19.639 | 212  | 75378    | 0.743  | ng/ul | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.680 | 264  | 82308    | 0.706  | ng/ul | -0.02    |


|                               |        |     |         |               |        |
|-------------------------------|--------|-----|---------|---------------|--------|
| Target Compounds              |        |     |         |               | Qvalue |
| 86) Bis(2-ethylhexyl)phtha... | 21.286 | 149 | 3264963 | 62.801 ng/ul# | 78     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP011823\  
Data File : BP013524.D  
Acq On : 18 Jan 2023 16:29  
Operator : CG/JU  
Sample : 01145-02DL 30X  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
A43S7DL

Quant Time: Jan 19 01:46:49 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP010523.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Jan 18 01:06:35 2023  
Response via : Initial Calibration

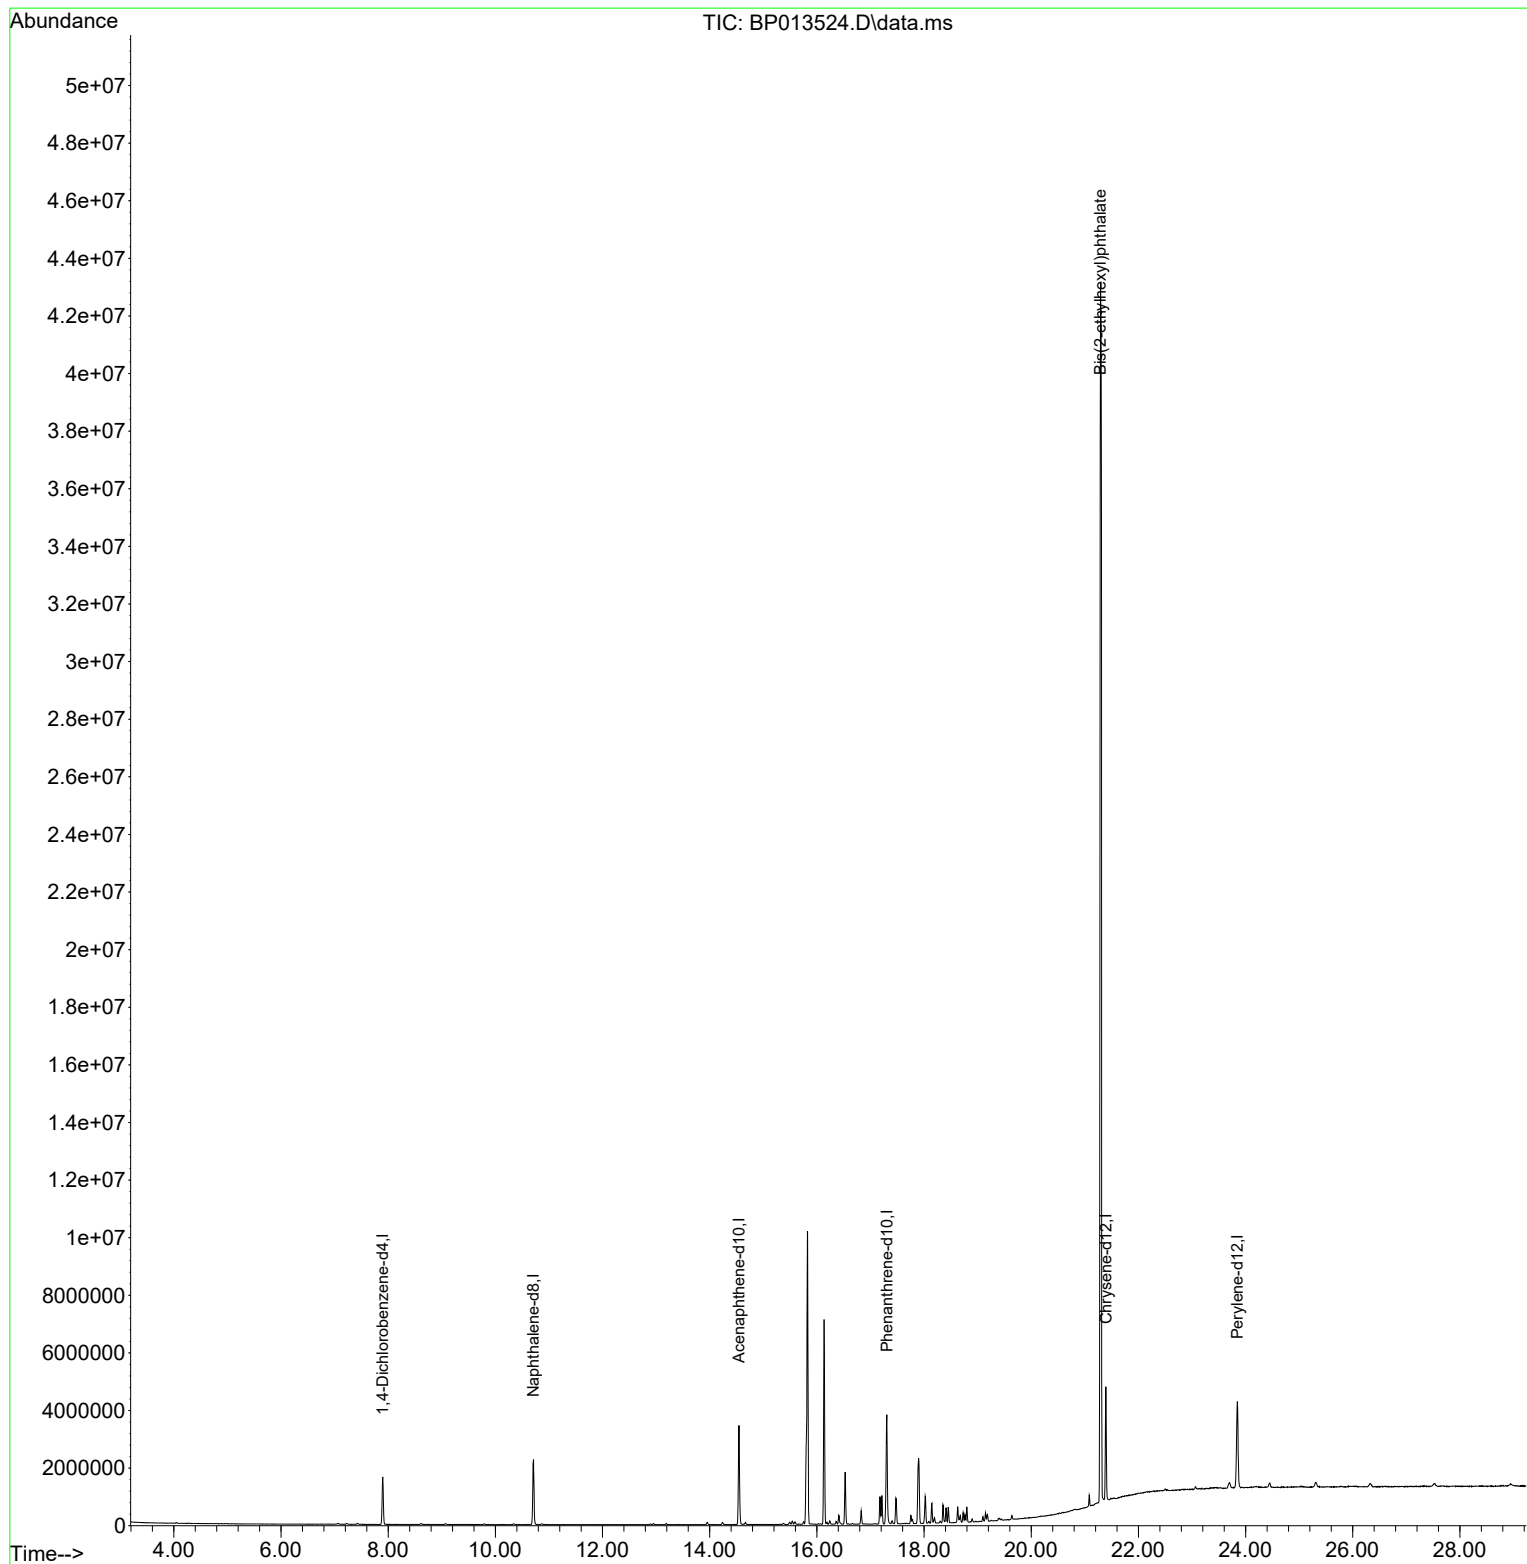

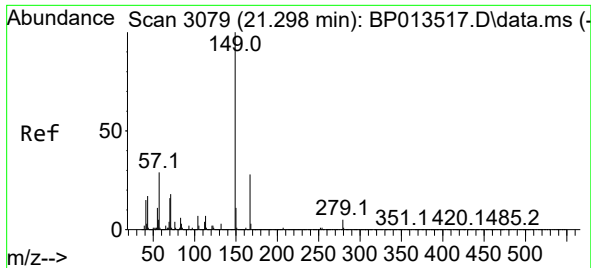

#86  
 Bis(2-ethylhexyl)phthalate  
 Concen: 62.801 ng/ul  
 RT: 21.286 min Scan# 3077  
 Delta R.T. -0.006 min  
 Lab File: BP013524.D  
 Acq: 18 Jan 2023 16:29

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A43S7DL

Tgt Ion:149 Resp: 3264963  
 Ion Ratio Lower Upper  
 149 100  
 167 40.3 22.2 33.4#  
 279 7.2 3.5 5.3#

