

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013529.D
 Acq On : 18 Jan 2023 19:21
 Operator : CG/JU
 Sample : 01146-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43Y5

Quant Time: Jan 19 01:48:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	432289	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	1617120	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164	942686	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	2144814	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240	2209877	20.000	ng/ul	0.00
88) Perylene-d12	23.845	264	2712725	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	17300	1.556	ng/uL	0.00
4) Pyridine-d5	3.728	84	644	0.021	ng/ul	0.00
7) Phenol-d5	7.058	99	324833	9.056	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	213004	9.412	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	261677	9.782	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	251306	9.196	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	118487	10.290	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	125283	9.940	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	244126	9.719	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131	134399	3.798	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	717252	10.443	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160	789123	10.380	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	66916	5.323	ng/ul	0.00
60) Fluorene-d10	15.540	176	636365	10.490	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	76920	5.656	ng/ul	0.00
73) Anthracene-d10	17.404	188	996078	10.507	ng/ul	0.00
81) Pyrene-d10	19.639	212	1330547	11.066	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.686	264	1452871	10.903	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.728	105	100909	2.340	ng/ul	97
61) Fluorene	15.592	166	146619	2.133	ng/ul#	73
86) Bis(2-ethylhexyl)phtha...	21.286	149	3597578	58.371	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013529.D
Acq On : 18 Jan 2023 19:21
Operator : CG/JU
Sample : 01146-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43Y5

Quant Time: Jan 19 01:48:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration




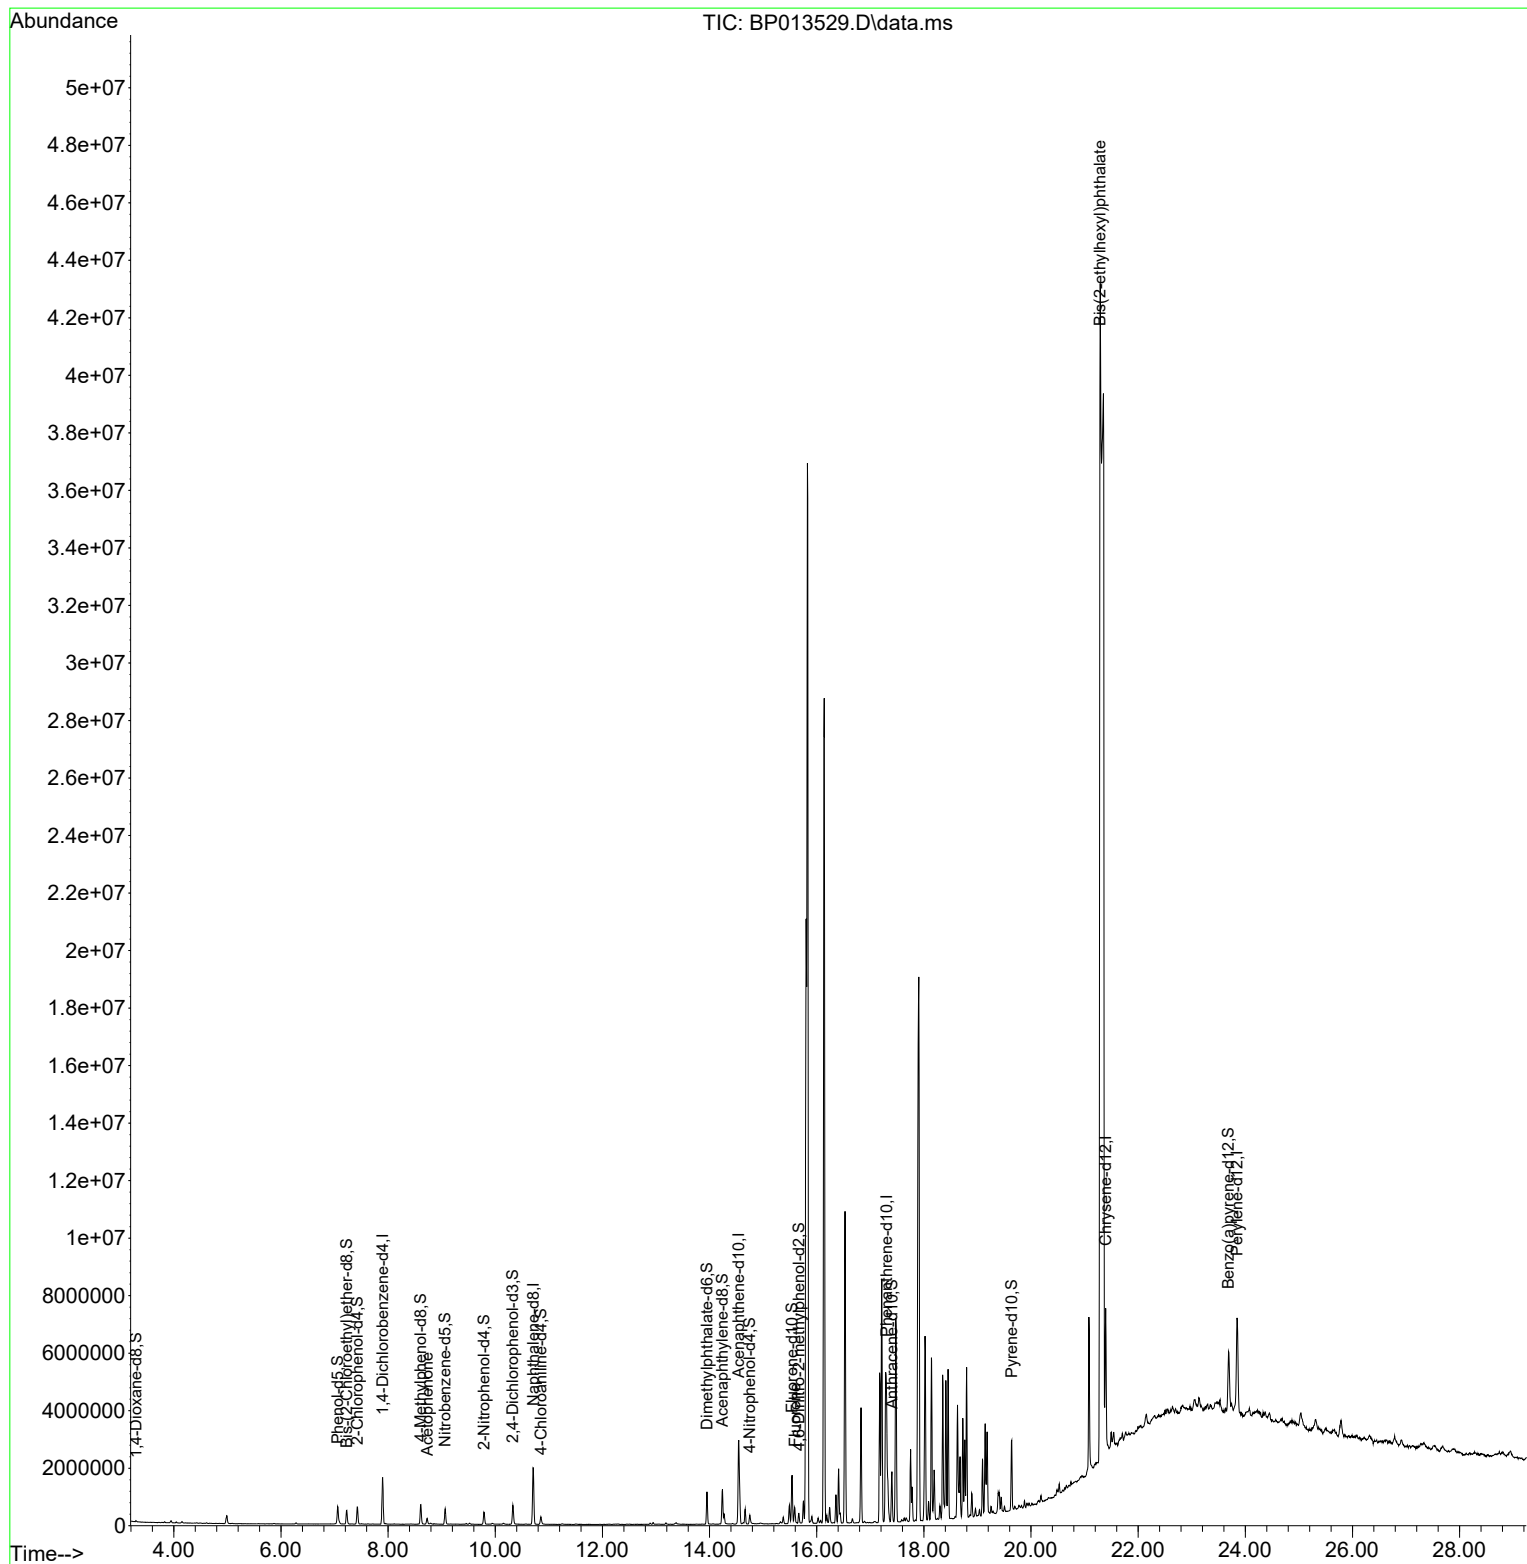


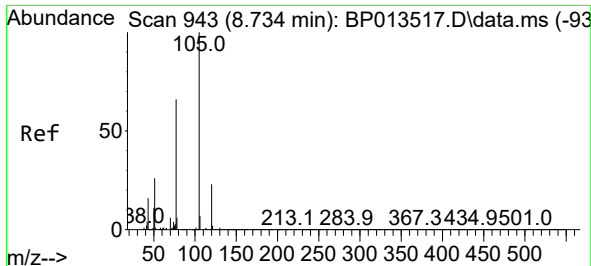

#16
Acetophenone
Concen: 2.340 ng/ul
RT: 8.728 min Scan# 943
Delta R.T. 0.000 min
Lab File: BP013529.D
Acq: 18 Jan 2023 19:21




Instrument :
BNA_P
ClientSampleId :
A43Y5


Tgt Ion:105 Resp: 100909
Ion Ratio Lower Upper
105 100
77 80.3 62.5 93.7
51 32.3 24.7 37.1

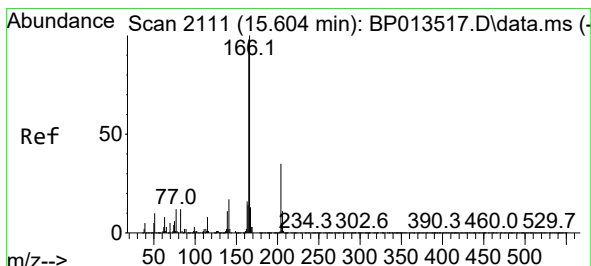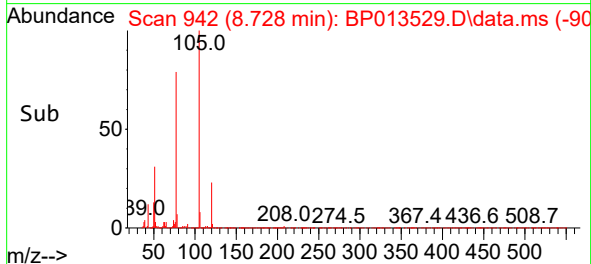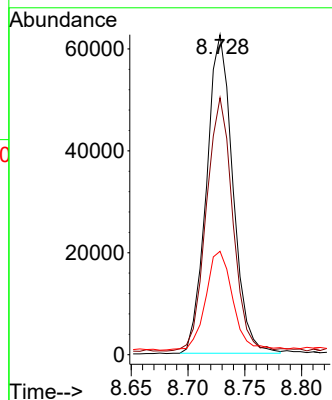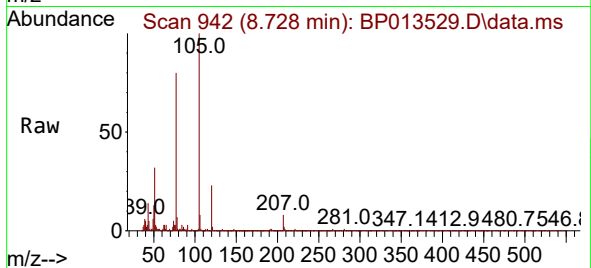

#61
Fluorene
Concen: 2.133 ng/ul
RT: 15.592 min Scan# 2109
Delta R.T. -0.006 min
Lab File: BP013529.D
Acq: 18 Jan 2023 19:21

Tgt Ion:166 Resp: 146619
Ion Ratio Lower Upper
166 100
165 105.7 78.0 117.0
167 78.1 10.8 16.2#

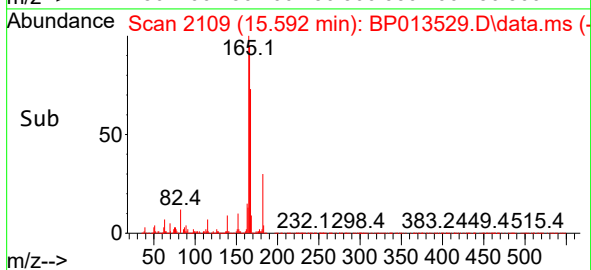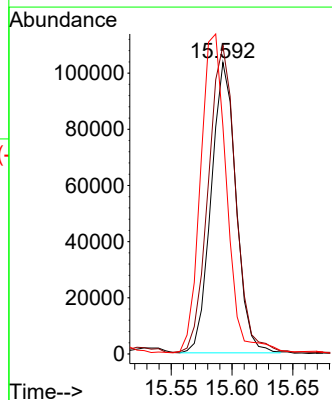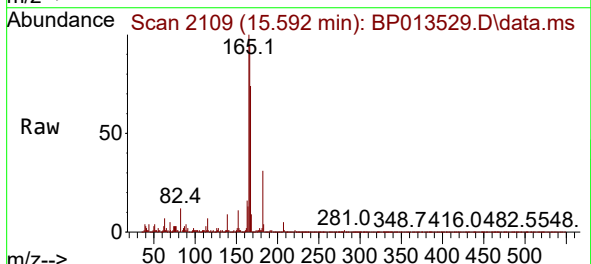

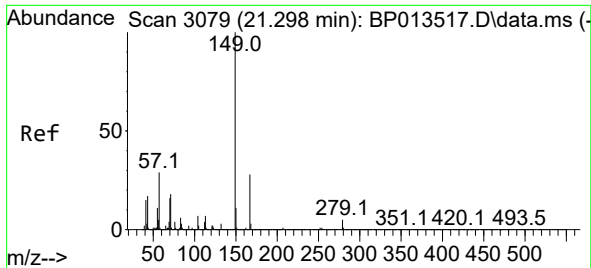

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 58.371 ng/ul
 RT: 21.286 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BP013529.D
 Acq: 18 Jan 2023 19:21

Instrument :
 BNA_P
 ClientSampleId :
 A43Y5

Tgt Ion:149 Resp: 3597578
 Ion Ratio Lower Upper
 149 100
 167 42.9 22.2 33.4#
 279 8.5 3.5 5.3#

