

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013524.D
 Acq On : 18 Jan 2023 16:29
 Operator : CG/JU
 Sample : 01145-02DL 30X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :

BNA_P

ClientSampleId :

A43S7DL

Quant Time: Jan 19 01:46:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration




Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Supervised By :mohammad

Supervised By :mohammad

01/20/2023

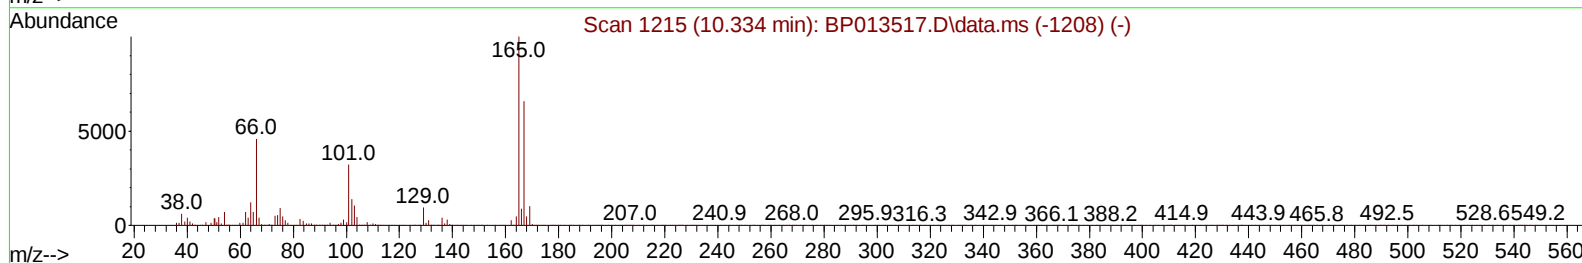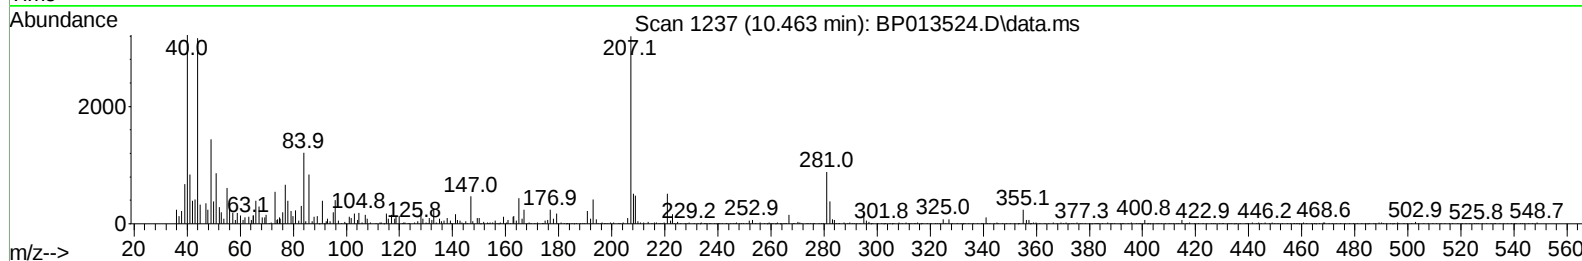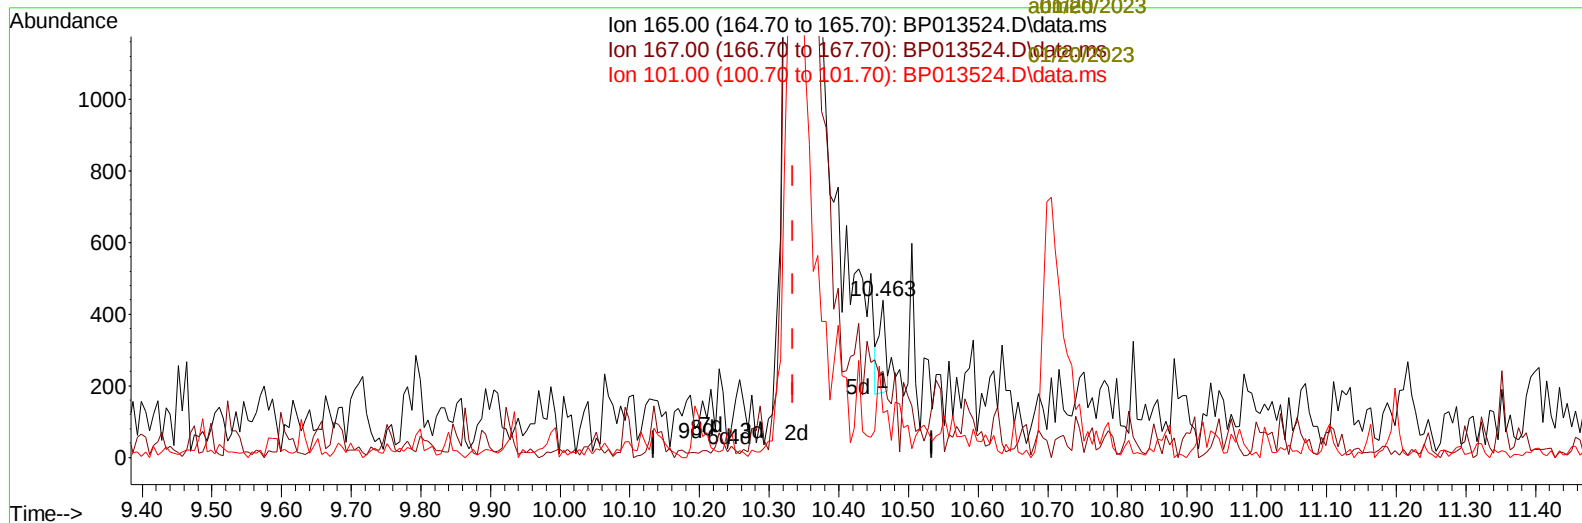

TIC: BP013524.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.463min (+ 0.130) 0.01 ng/ul

response 163

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	55.02
101.00	32.50	28.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013524.D
 Acq On : 18 Jan 2023 16:29
 Operator : CG/JU
 Sample : 01145-02DL 30X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43S7DL




Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Supervised By :mohammad
 Supervised By :mohammad
 01/20/2023

Quant Time: Jan 19 01:46:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Ion 165.00 (164.70 to 165.70): BP013524.D\data.ms
 Ion 167.00 (166.70 to 167.70): BP013524.D\data.ms
 Ion 101.00 (100.70 to 101.70): BP013524.D\data.ms

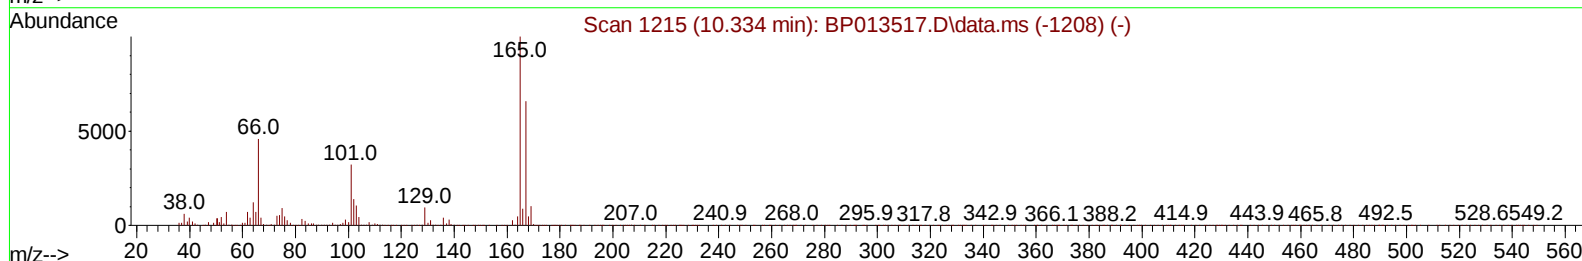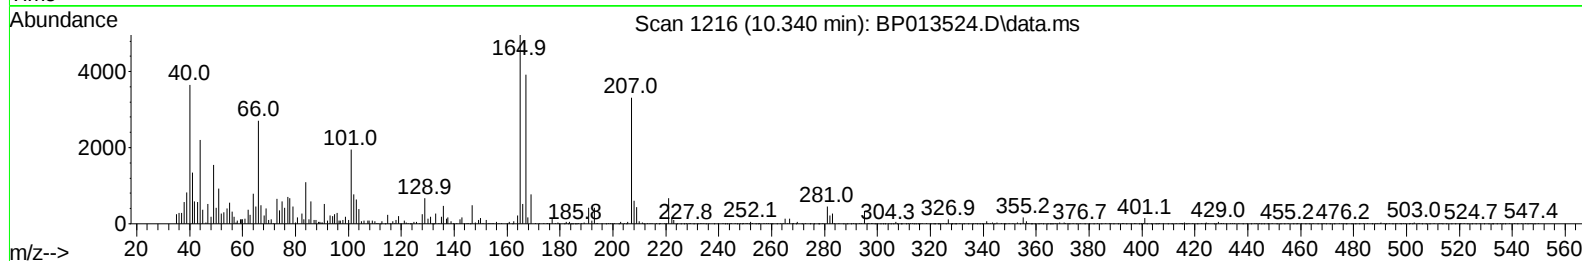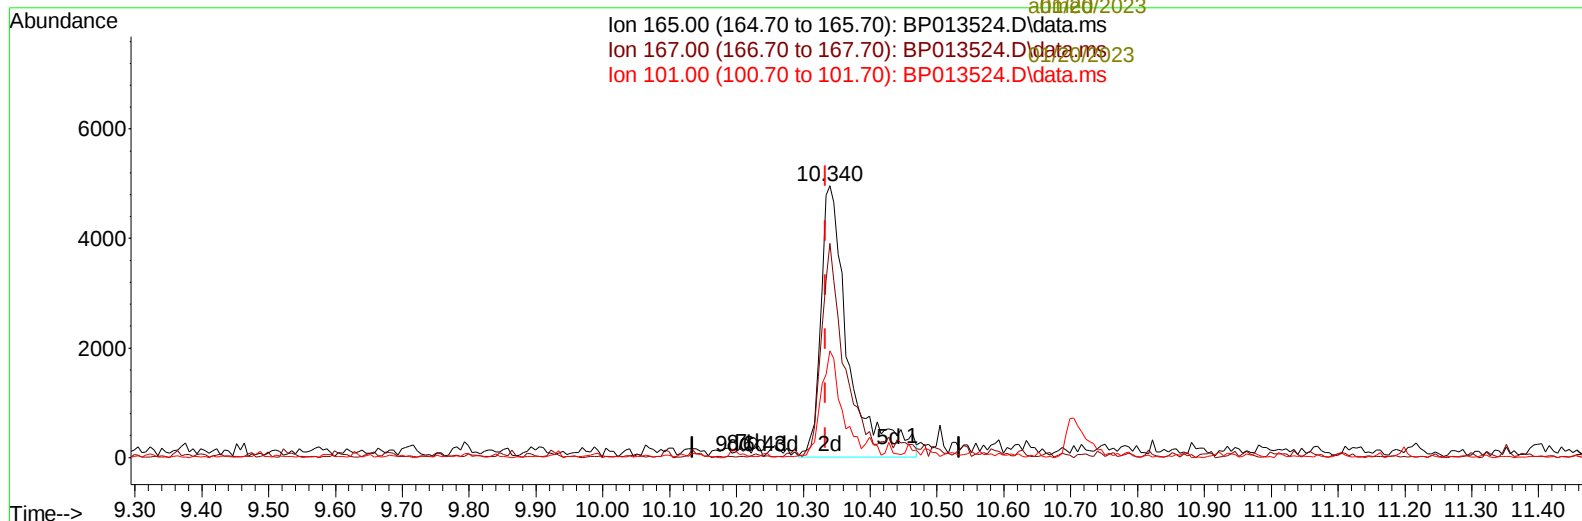

TIC: BP013524.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.340min (+ 0.006) 0.51 ng/ul m

response 14354

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.10	78.97#
101.00	32.50	39.25#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013524.D
 Acq On : 18 Jan 2023 16:29
 Operator : CG/JU
 Sample : 01145-02DL 30X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43S7DL


Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023


Supervised By :mohammad
 Supervised By :mohammad
 01/20/2023

Quant Time: Jan 19 01:46:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration


Ion 149.00 (148.70 to 149.70): BP013524.D\data.ms
 Ion 167.00 (166.70 to 167.70): BP013524.D\data.ms
 Ion 279.00 (278.70 to 279.70): BP013524.D\data.ms

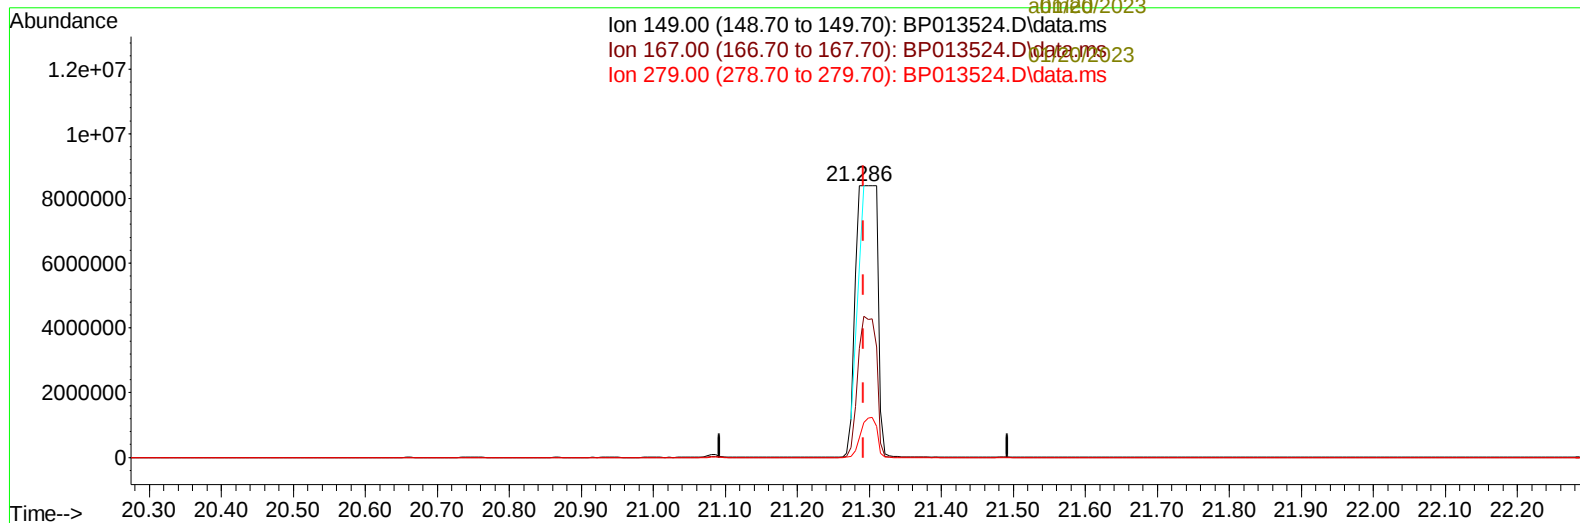

Scan 3077 (21.286 min): BP013524.D\data.ms

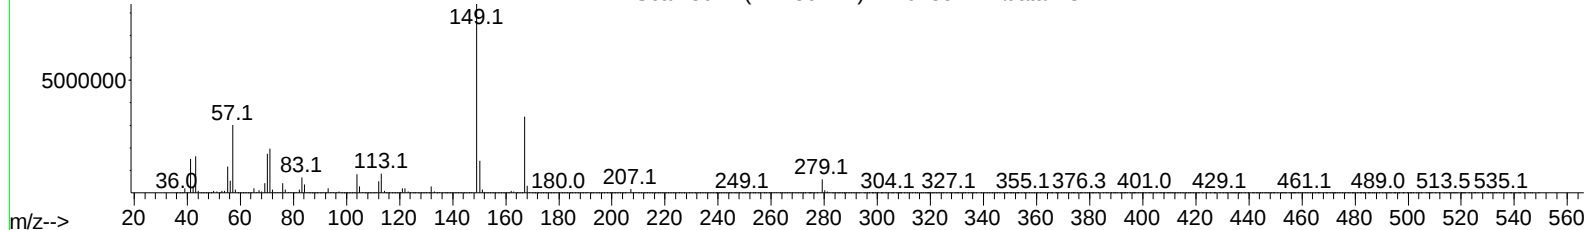

Scan 3079 (21.298 min): BP013517.D\data.ms (-3074) (-)

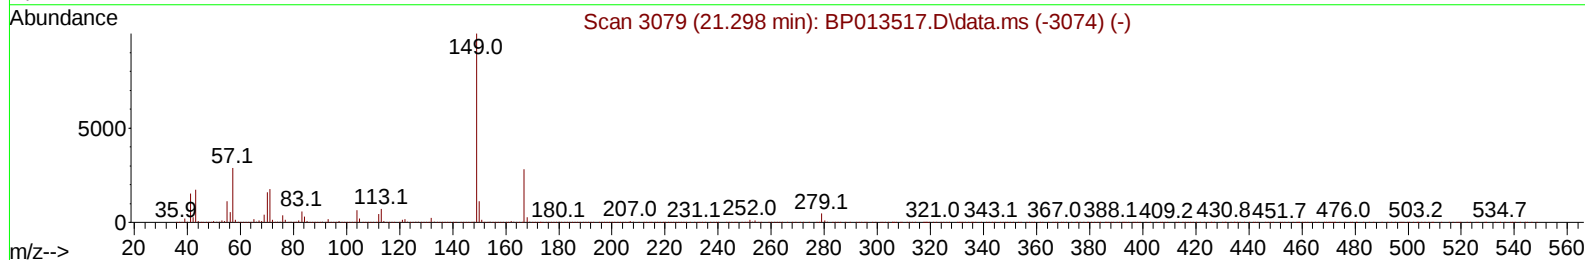

TIC: BP013524.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.286min (-0.006) 62.80 ng/u1

response 3264963

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	27.80	40.26#
279.00	4.40	7.21#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013524.D
 Acq On : 18 Jan 2023 16:29
 Operator : CG/JU
 Sample : 01145-02DL 30X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43S7DL


Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023


Supervised By :mohammad
 Supervised By :mohammad
 01/20/2023

Quant Time: Jan 19 01:46:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration


Ion 149.00 (148.70 to 149.70): BP013524.D\data.ms
 Ion 167.00 (166.70 to 167.70): BP013524.D\data.ms
 Ion 279.00 (278.70 to 279.70): BP013524.D\data.ms

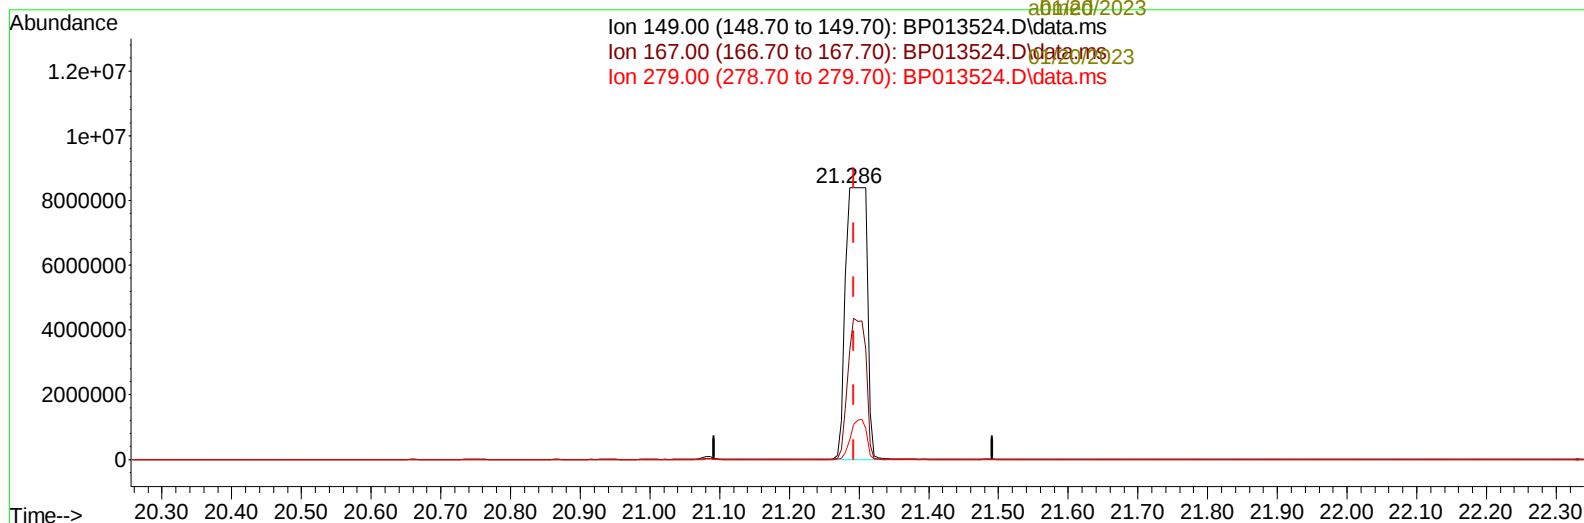

Scan 3077 (21.286 min): BP013524.D\data.ms

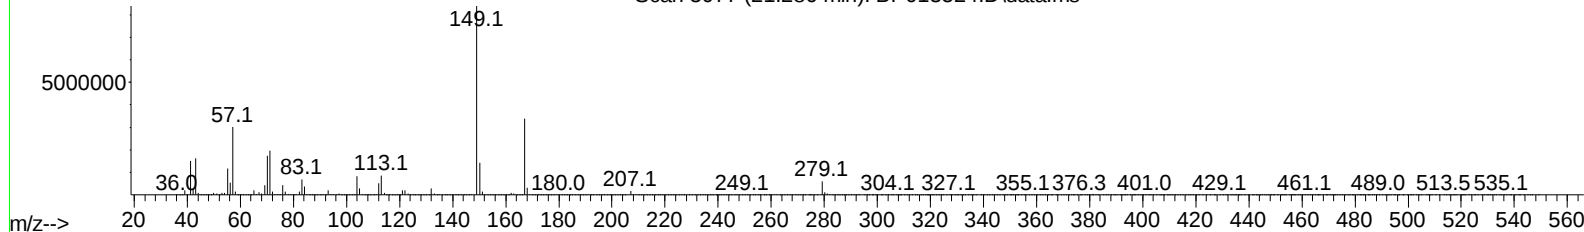

Scan 3079 (21.298 min): BP013517.D\data.ms (-3074) (-)

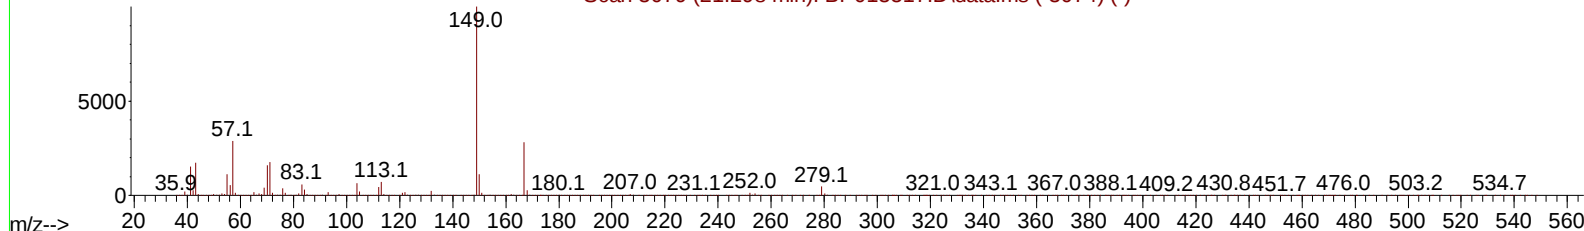

TIC: BP013524.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.286min (-0.006) 343.32 ng/ul m

response 17848938

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	27.80	40.26#
279.00	4.40	7.21#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013524.D
 Acq On : 18 Jan 2023 16:29
 Operator : CG/JU
 Sample : 01145-02DL 30X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43S7DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Supervised By :mohammad
 Supervised By :mohammad
 01/20/2023

Quant Time: Jan 19 01:46:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----01/20/2023							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.899	152		434218	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136		1822765	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.546	164		1095015	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188		2170399	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240		1864103	20.000	ng/ul	0.00
88) Perylene-d12	23.845	264		2373784	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	0.000	96		0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	7.064	99		19612	0.544	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67		13761	0.605	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132		15584	0.580	ng/ul	0.00
15) 4-Methylphenol-d8	8.616	113		13308	0.485	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128		6353	0.490	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143		7386	0.520	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.340	165		14354m	0.507	ng/ul	0.00
31) 4-Chloroaniline-d4	10.863	131		13818	0.346	ng/ul	0.01
46) Dimethylphthalate-d6	13.957	166		50576	0.634	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160		53543	0.606	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143		0d	0.000	ng/ul	
60) Fluorene-d10	15.540	176		45674	0.648	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.675	200		4122	0.300	ng/ul	0.00
73) Anthracene-d10	17.404	188		65499	0.683	ng/ul	0.00
81) Pyrene-d10	19.639	212		75378	0.743	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.680	264		82308	0.706	ng/ul	-0.02

Target Compounds Qvalue
 86) Bis(2-ethylhexyl)phtha... 21.286 149 17848938m 343.321 ng/ul

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013524.D
Acq On : 18 Jan 2023 16:29
Operator : CG/JU
Sample : 01145-02DL 30X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A43S7DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
Supervised By :mohammad ahmed 01/20/2023

Supervised By :mohammad
Supervised By :mohammad
01/20/2023

Quant Time: Jan 19 01:46:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

