




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013532.D
 Acq On : 18 Jan 2023 21:03
 Operator : CG/JU
 Sample : 01146-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4411

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:49:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

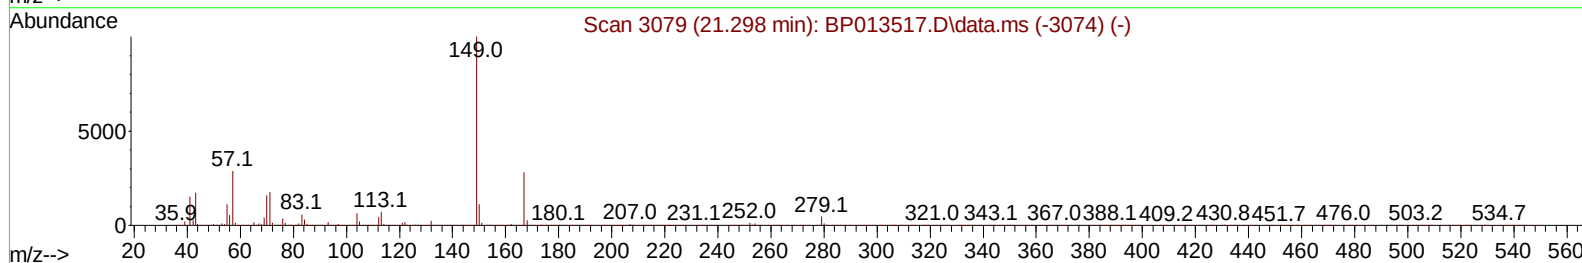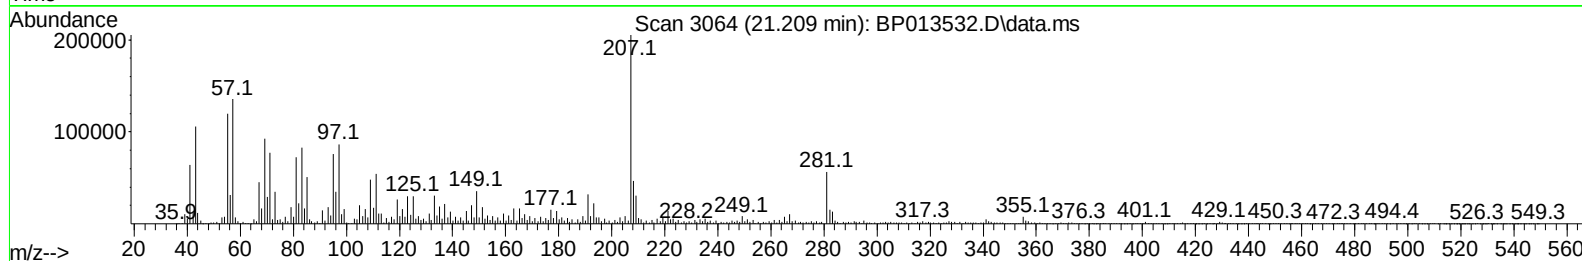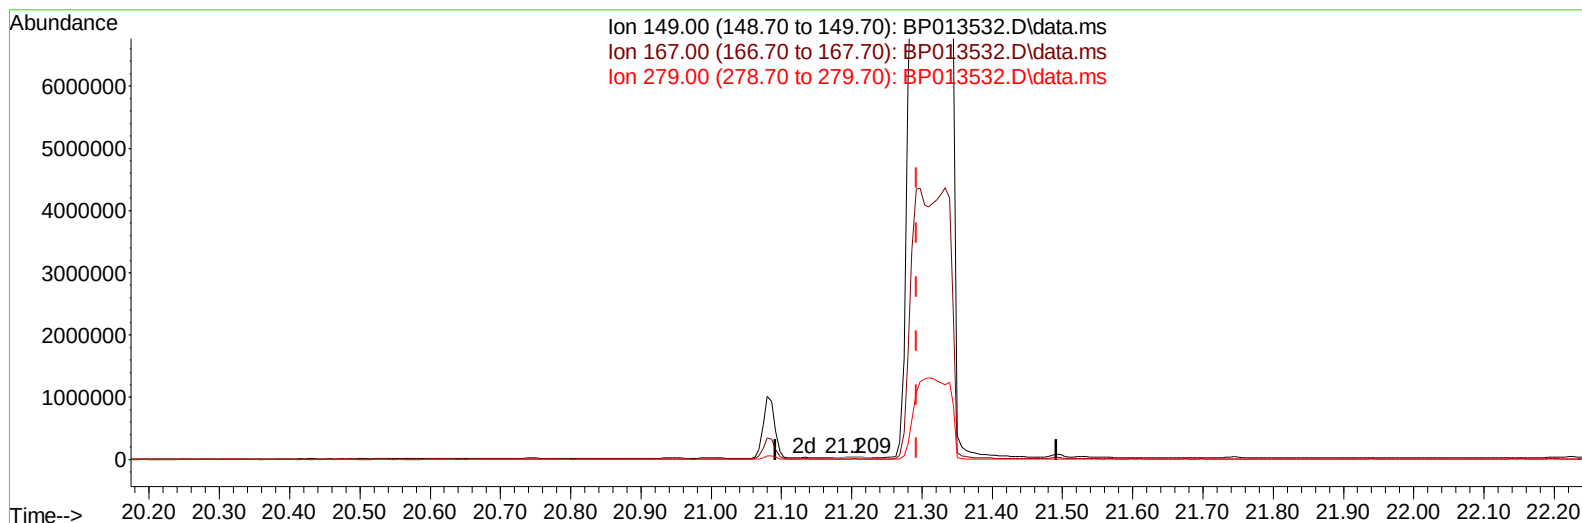

TIC: BP013532.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.209min (-0.083) 0.28 ng/ul

response 18712

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	27.80	30.15
279.00	4.40	6.45#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013532.D
 Acq On : 18 Jan 2023 21:03
 Operator : CG/JU
 Sample : 01146-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4411

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:49:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

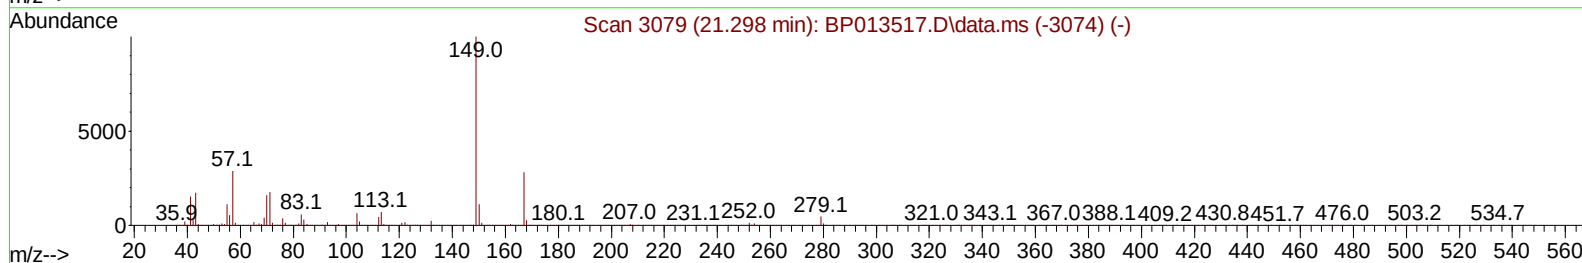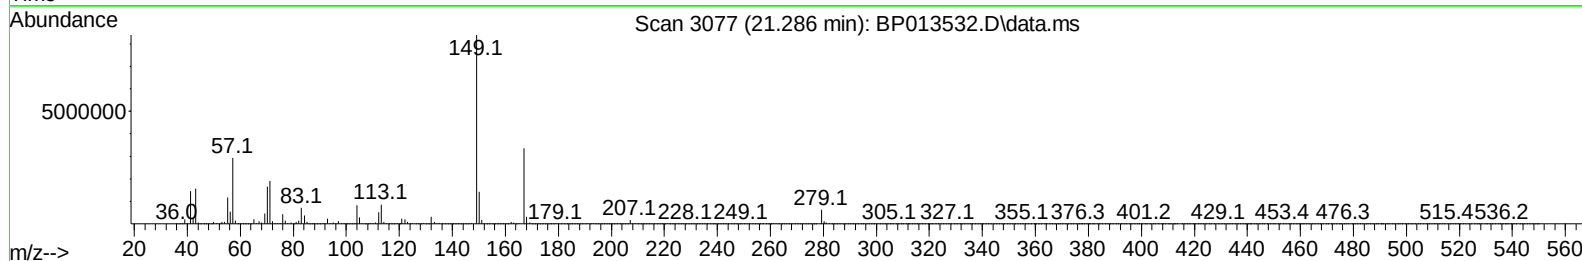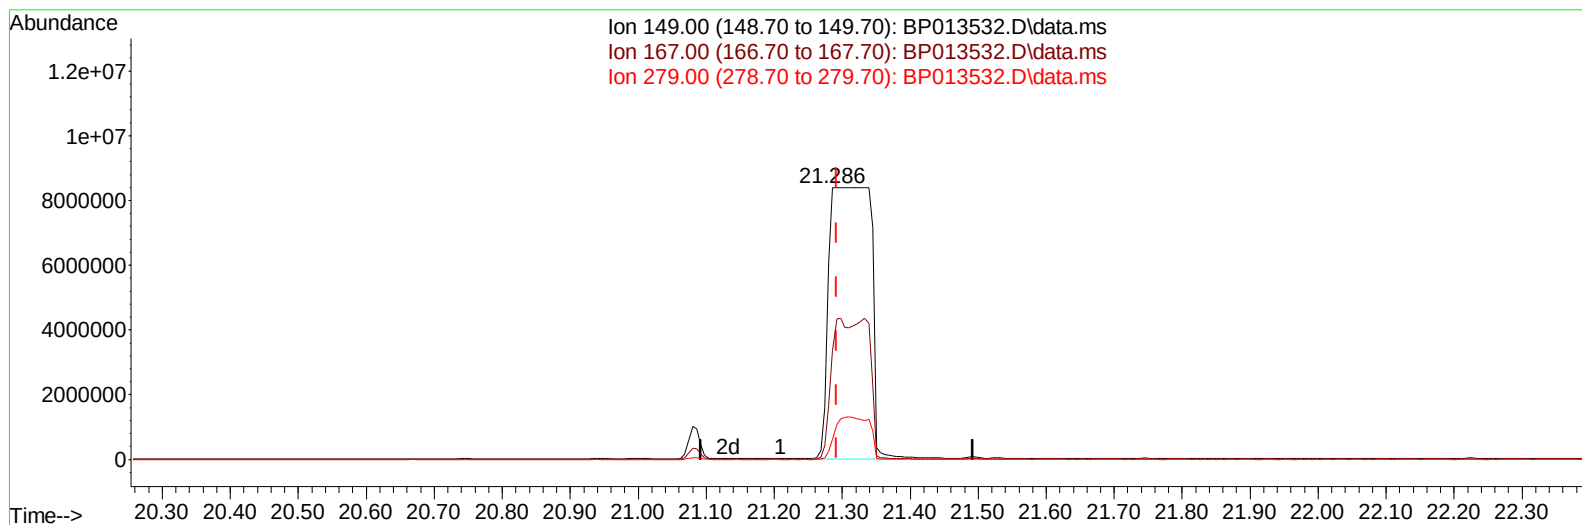

TIC: BP013532.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.286min (-0.006) 523.22 ng/ul m

response 35302192

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	27.80	40.11#
279.00	4.40	7.54#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013532.D
 Acq On : 18 Jan 2023 21:03
 Operator : CG/JU
 Sample : 01146-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4411

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 19 01:49:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	459073	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	1768167	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164	1047183	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188	2379556	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240	2419216	20.000	ng/ul	0.00
88) Perylene-d12	23.845	264	2981570	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	39453	3.341	ng/uL	0.00
4) Pyridine-d5	3.728	84	124429	3.777	ng/ul	0.00
7) Phenol-d5	7.057	99	785967	20.633	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	478323	19.904	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132	641660	22.587	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	624012	21.501	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	297053	23.595	ng/ul	0.00
24) 2-Nitrophenol-d4	9.792	143	342779	24.872	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	626706	22.818	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	472130	12.202	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	1804720	23.655	ng/ul	0.00
49) Acenaphthylene-d8	14.239	160	2115853	25.054	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143	241188	17.271	ng/ul	0.00
60) Fluorene-d10	15.539	176	1609538	23.884	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	258059	17.103	ng/ul	0.00
73) Anthracene-d10	17.404	188	2614202	24.855	ng/ul	0.00
81) Pyrene-d10	19.639	212	3331736	25.312	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.686	264	3698287	25.252	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.286	149	35302192m	523.221	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013532.D
Acq On : 18 Jan 2023 21:03
Operator : CG/JU
Sample : 01146-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4411

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 19 01:49:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

