




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013533.D
 Acq On : 18 Jan 2023 21:38
 Operator : CG/JU
 Sample : 01146-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4412

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:49:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

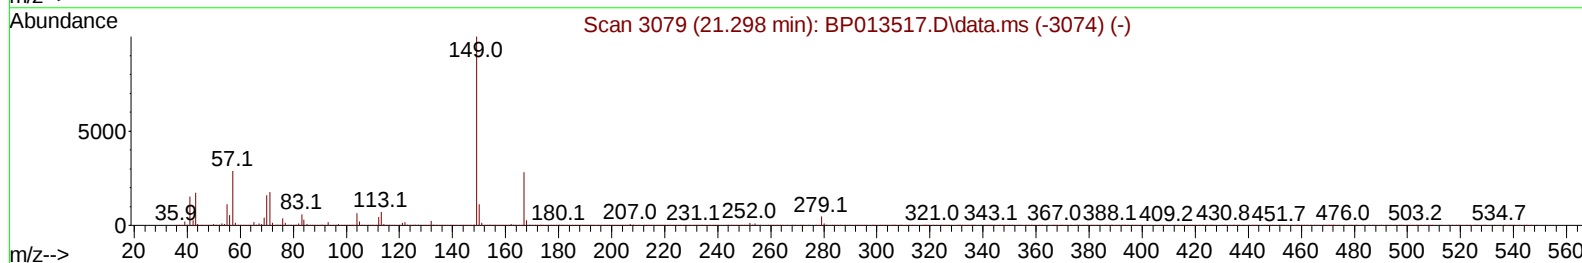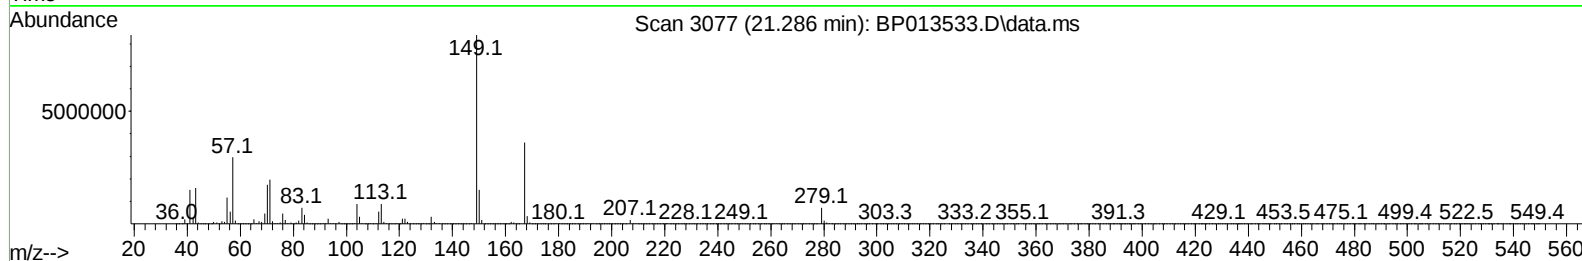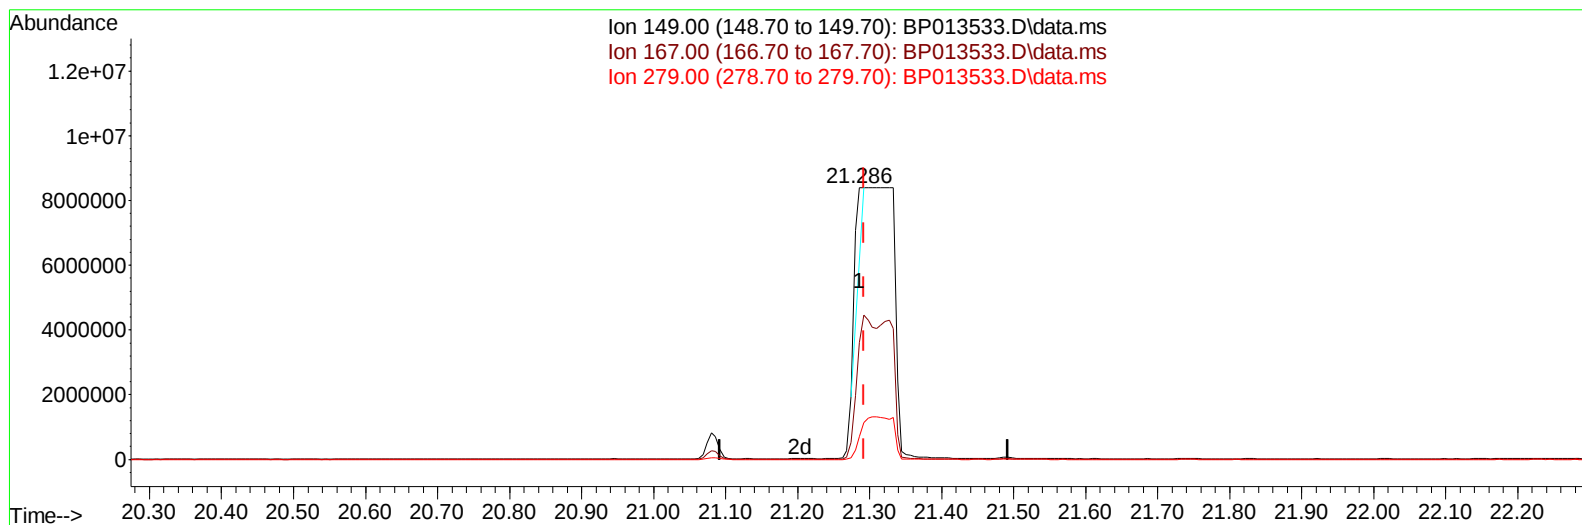

TIC: BP013533.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.286min (-0.006) 61.09 ng/u1

response 3623791

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	27.80	43.00#
279.00	4.40	8.46#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013533.D
 Acq On : 18 Jan 2023 21:38
 Operator : CG/JU
 Sample : 01146-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4412

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:49:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

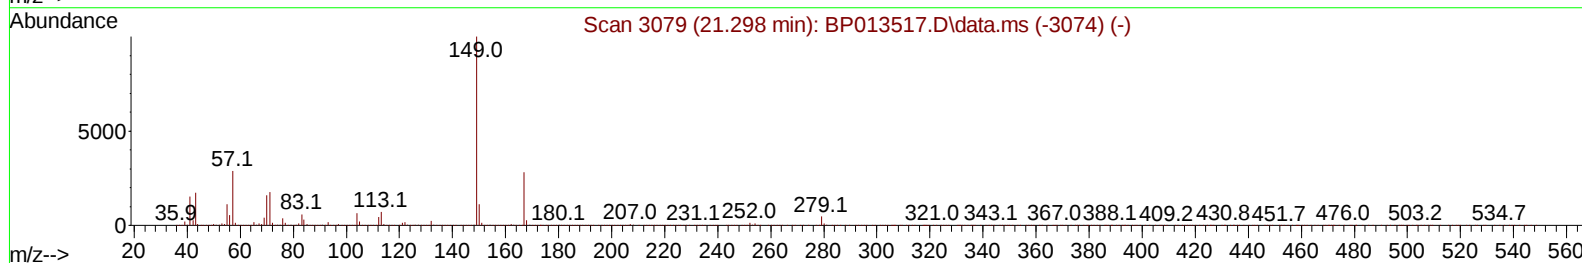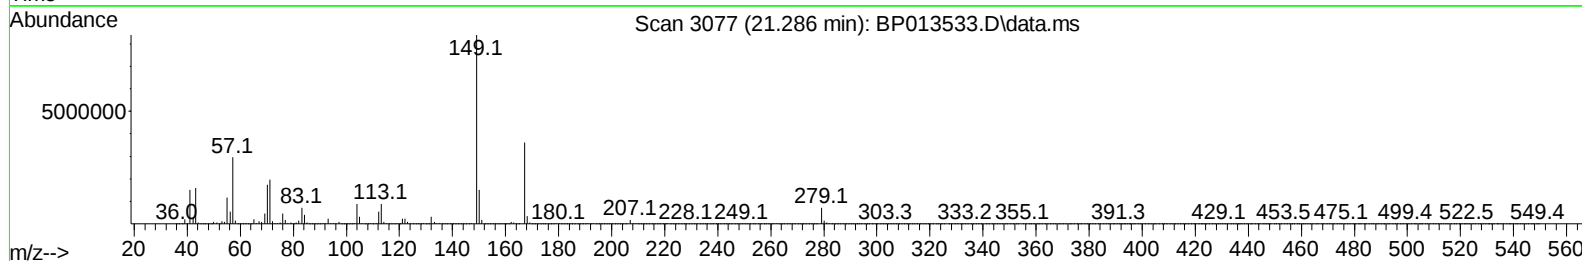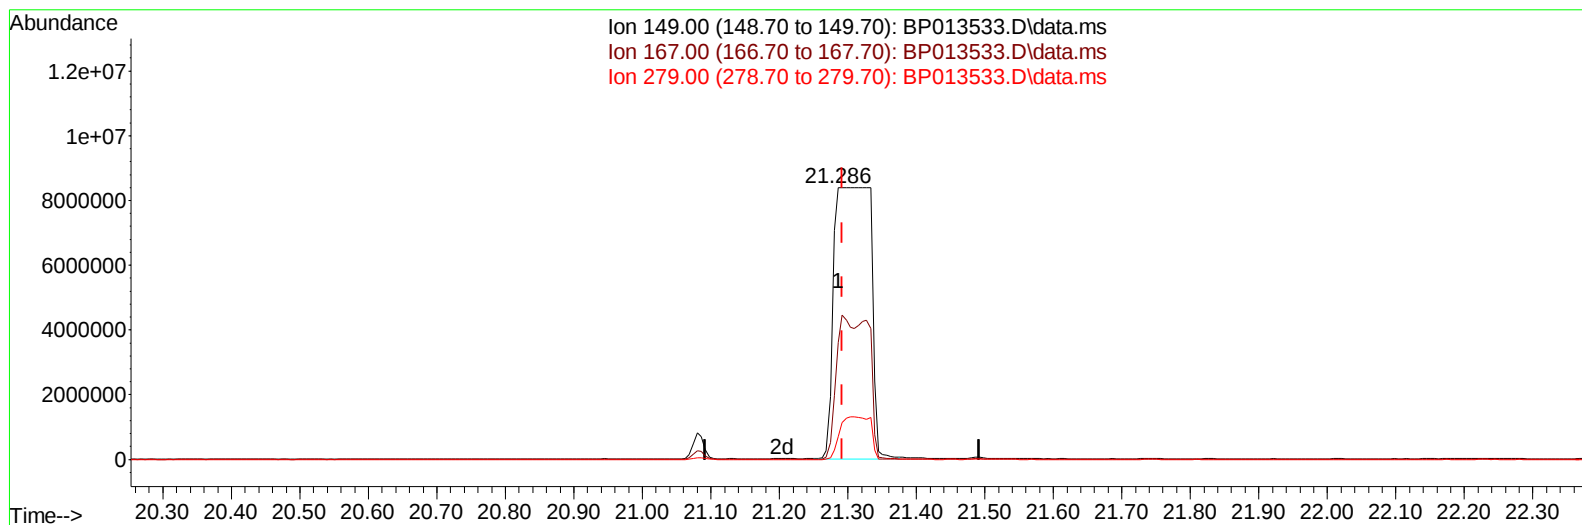

TIC: BP013533.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.286min (-0.006) 523.22 ng/ul m

response 31037446

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	27.80	43.00#
279.00	4.40	8.46#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013533.D
 Acq On : 18 Jan 2023 21:38
 Operator : CG/JU
 Sample : 01146-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4412

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:49:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.898	152		444813	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136		1712155	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164		970722	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.304	188		2122275	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240		2126955	20.000	ng/ul	0.00
88) Perylene-d12	23.845	264		2719181	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.293	96		41987	3.669	ng/uL	0.00
4) Pyridine-d5	3.728	84		226752	7.104	ng/ul	0.00
7) Phenol-d5	7.057	99		778309	21.087	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67		473592	20.338	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132		627325	22.790	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113		617412	21.956	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128		290569	23.835	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143		336055	25.182	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165		614837	23.118	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131		517993	13.825	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166		1719261	24.310	ng/ul	0.00
49) Acenaphthylene-d8	14.239	160		2006261	25.627	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143		231887	17.913	ng/ul	0.00
60) Fluorene-d10	15.539	176		1534258	24.560	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200		233624	17.361	ng/ul	0.00
73) Anthracene-d10	17.404	188		2370135	25.266	ng/ul	0.00
81) Pyrene-d10	19.639	212		3032732	26.207	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.686	264		3498781	26.195	ng/ul	-0.01
Target Compounds							
86) Bis(2-ethylhexyl)phtha...	21.286	149		31037446m	523.222	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013533.D
Acq On : 18 Jan 2023 21:38
Operator : CG/JU
Sample : 01146-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4412

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 19 01:49:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

