




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013536.D
 Acq On : 18 Jan 2023 23:21
 Operator : CG/JU
 Sample : 01146-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4462

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:50:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

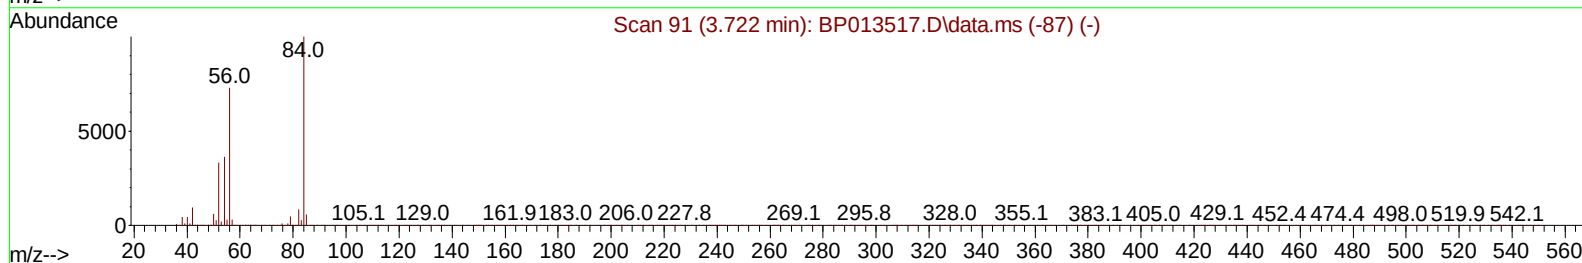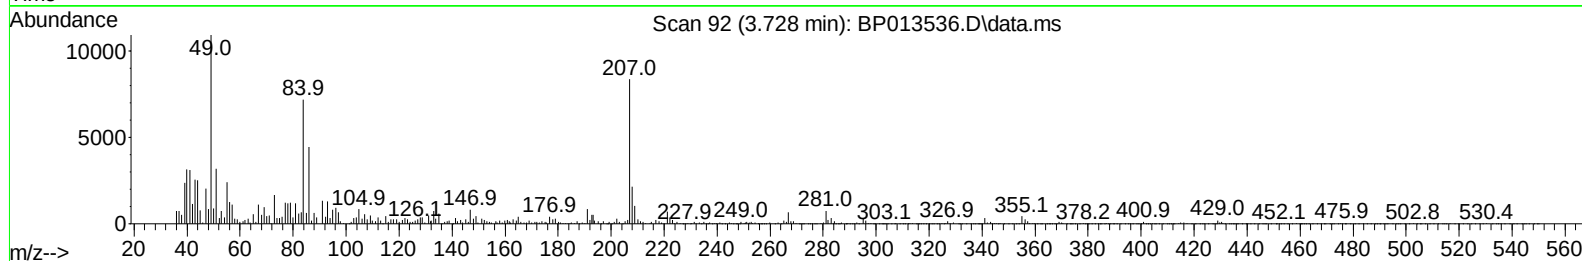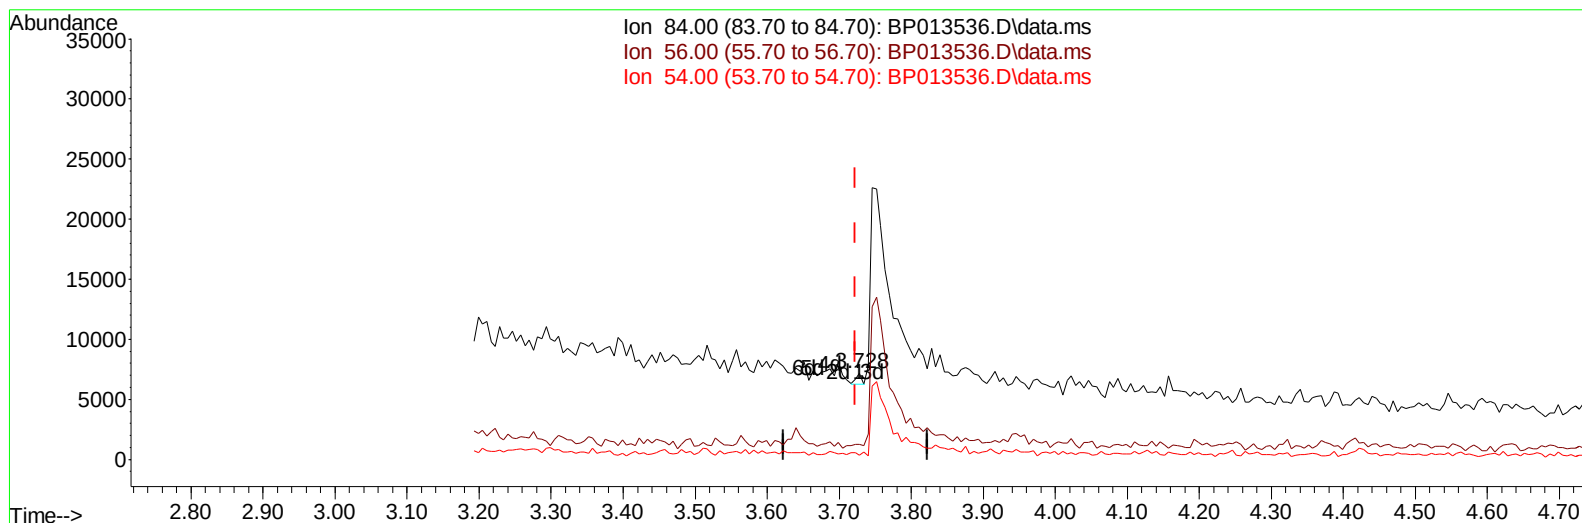

TIC: BP013536.D\data.ms

(4) Pyridine-d5 (S)

3.728min (+ 0.006) 0.01 ng/u1

response 472

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	72.30	17.33#
54.00	34.30	5.16#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013536.D
 Acq On : 18 Jan 2023 23:21
 Operator : CG/JU
 Sample : 01146-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4462

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:50:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

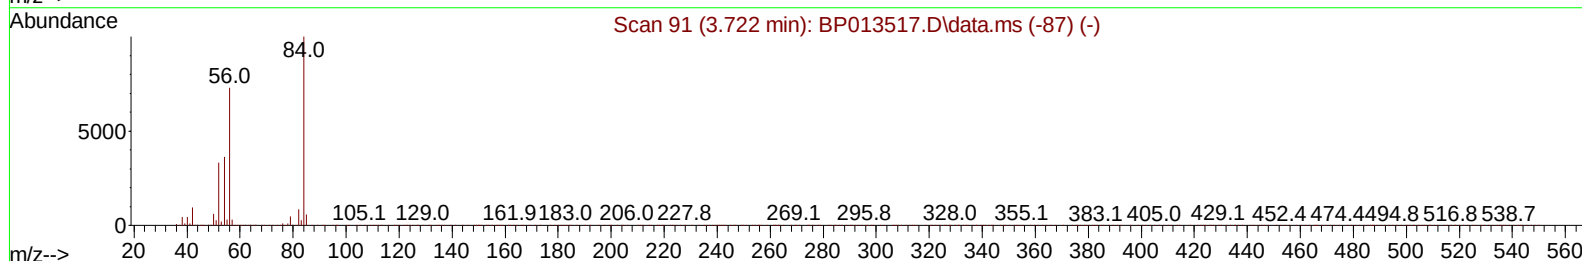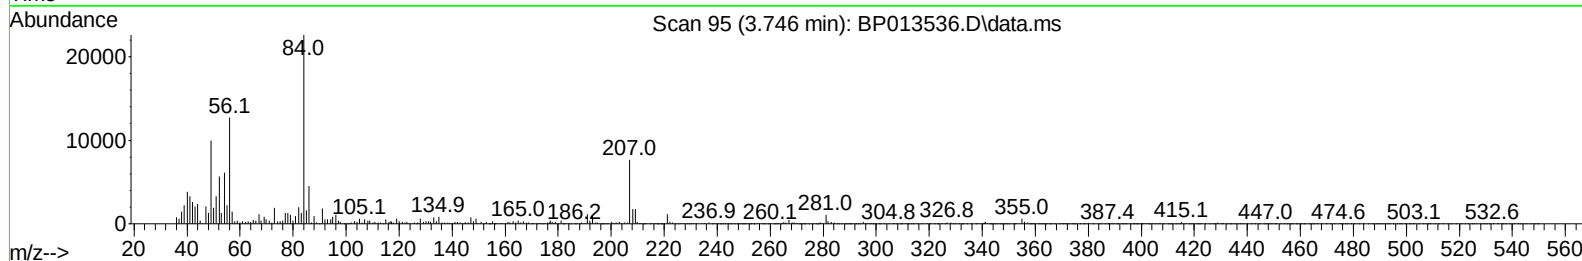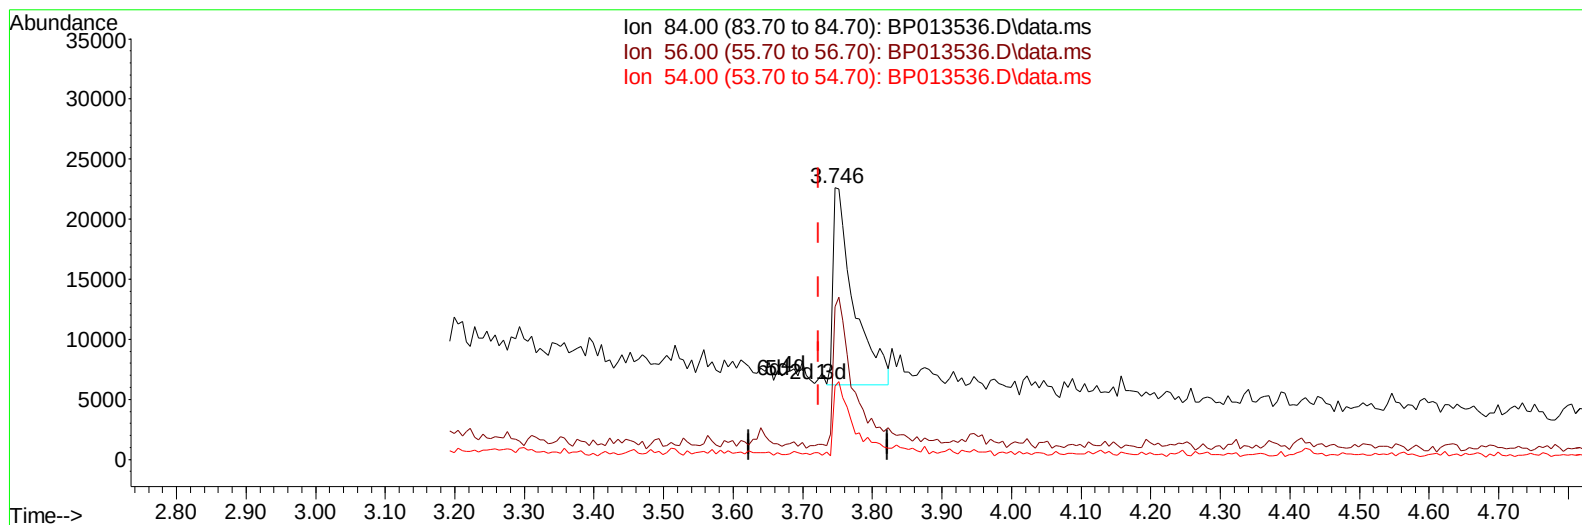

TIC: BP013536.D\data.ms

(4) Pyridine-d5 (S)

3.746min (+ 0.023) 0.92 ng/ul m

response 33824

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	72.30	56.19#
54.00	34.30	27.10#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013536.D
 Acq On : 18 Jan 2023 23:21
 Operator : CG/JU
 Sample : 01146-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4462

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 19 01:50:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

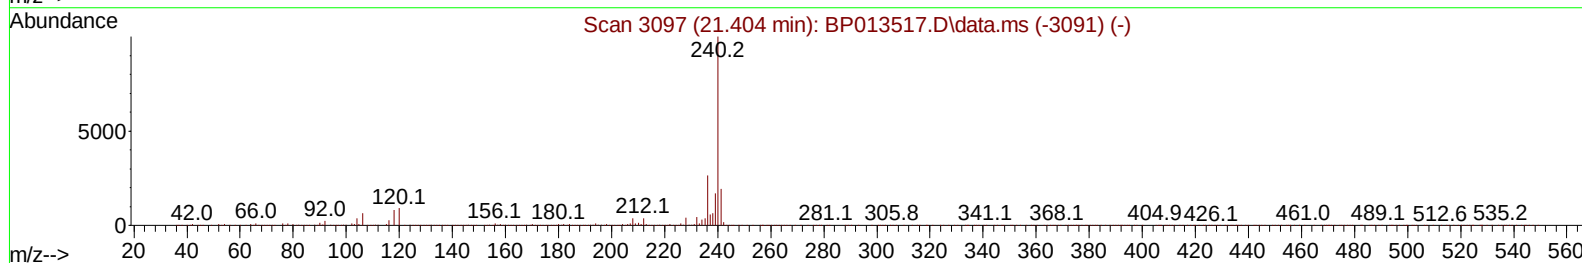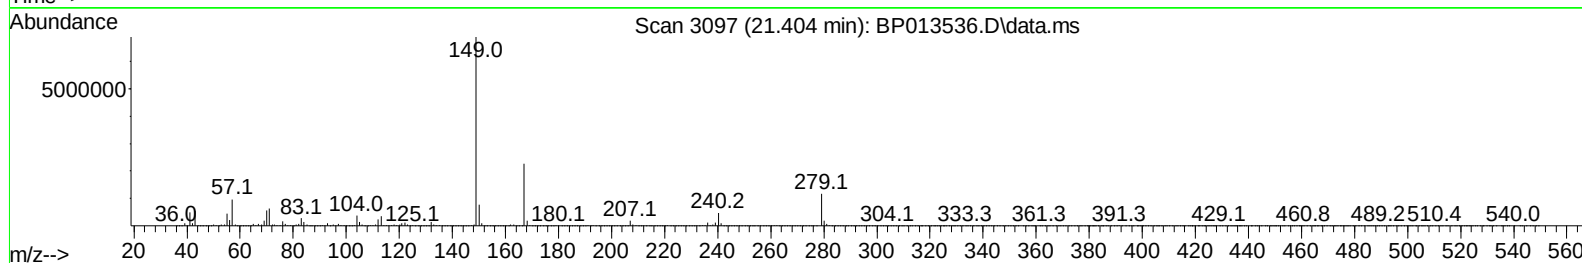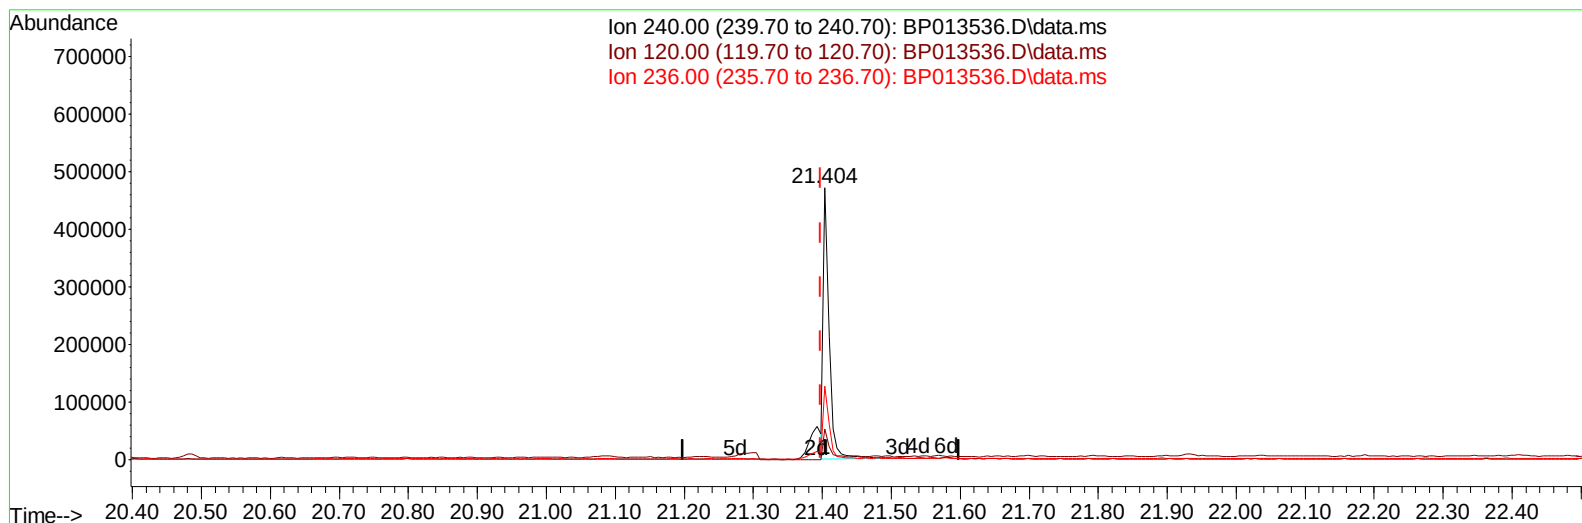

TIC: BP013536.D\data.ms

(79) Chrysene-d12 (I)

21.404min (+ 0.006) 20.00 ng/ul

response 282386

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	9.30	11.15
236.00	25.30	27.03
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013536.D
 Acq On : 18 Jan 2023 23:21
 Operator : CG/JU
 Sample : 01146-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4462

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:50:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

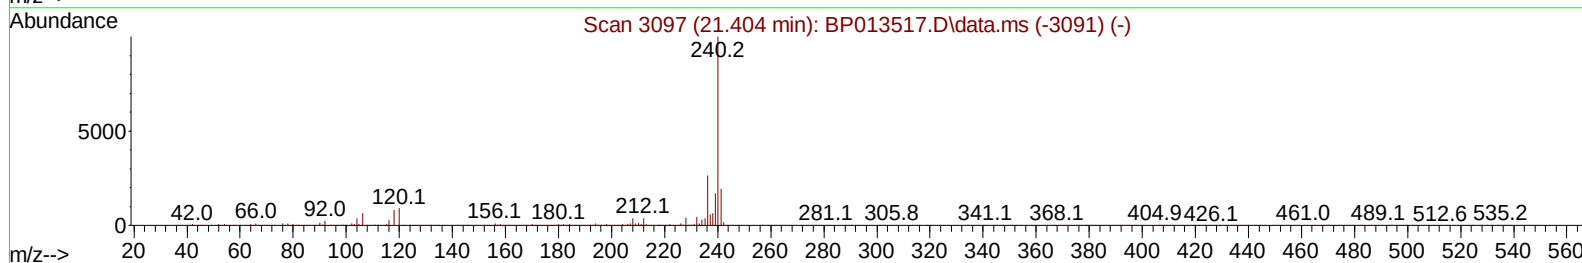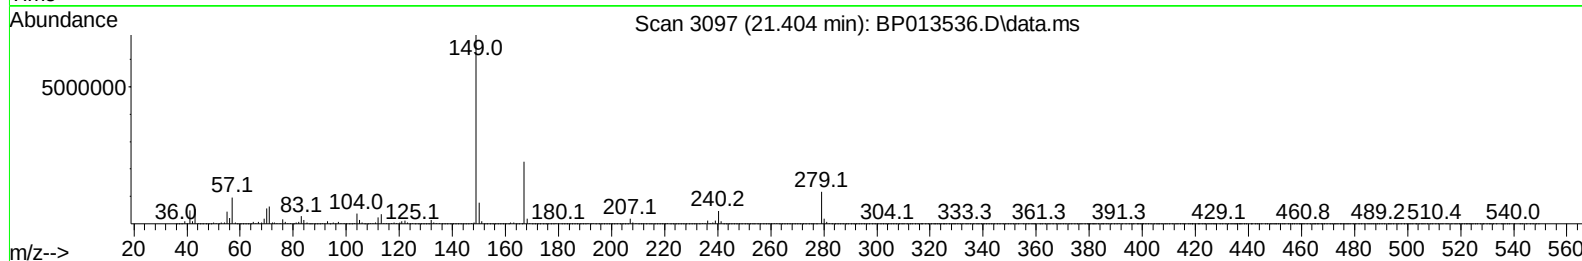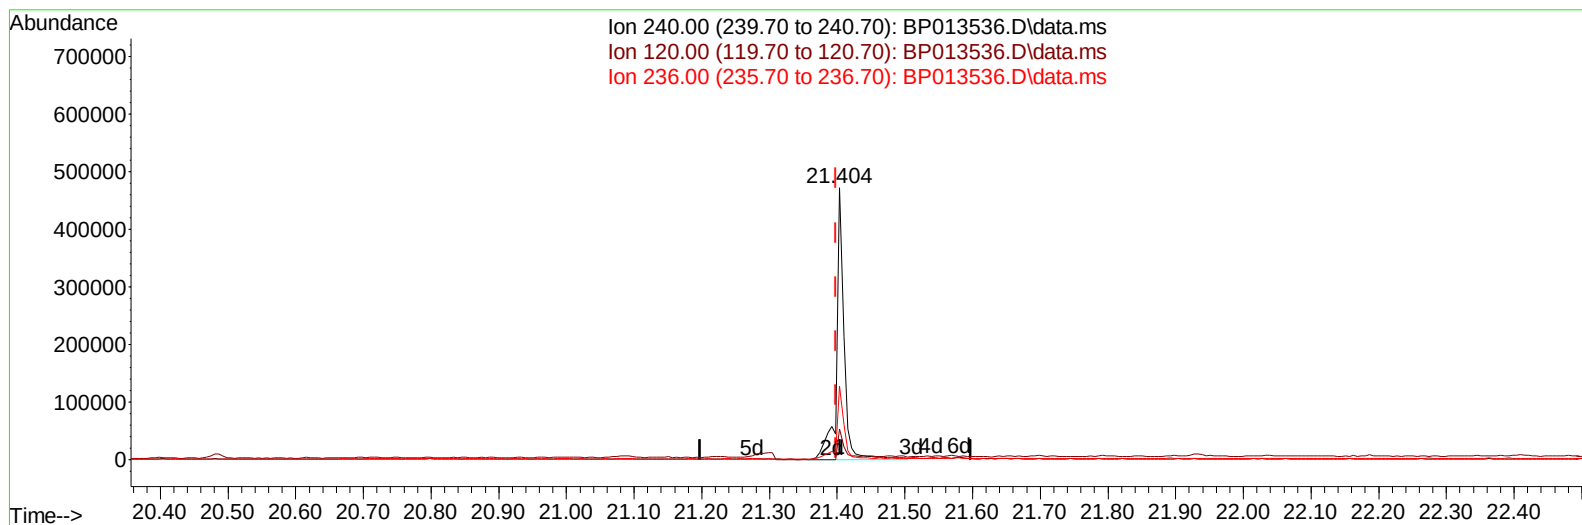

TIC: BP013536.D\data.ms

(79) Chrysene-d12 (I)

21.404min (+ 0.006) 20.00 ng/ul m

response 357273

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	9.30	11.15
236.00	25.30	27.03
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013536.D
 Acq On : 18 Jan 2023 23:21
 Operator : CG/JU
 Sample : 01146-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4462

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:50:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

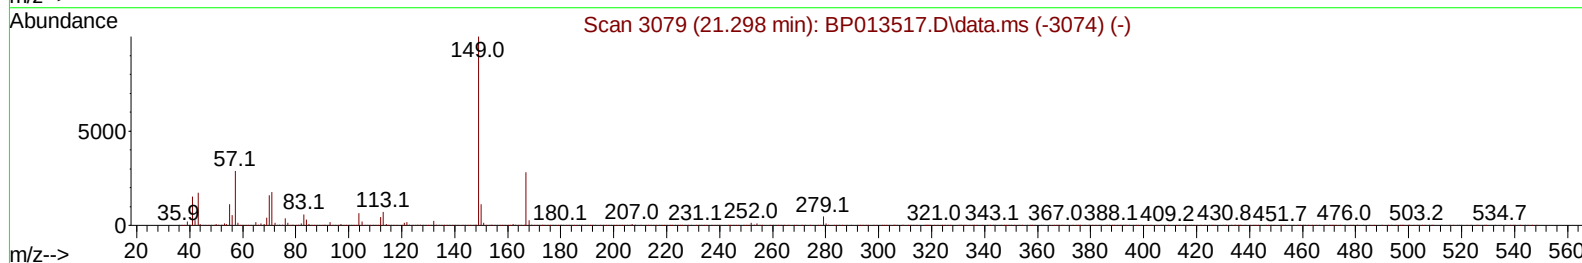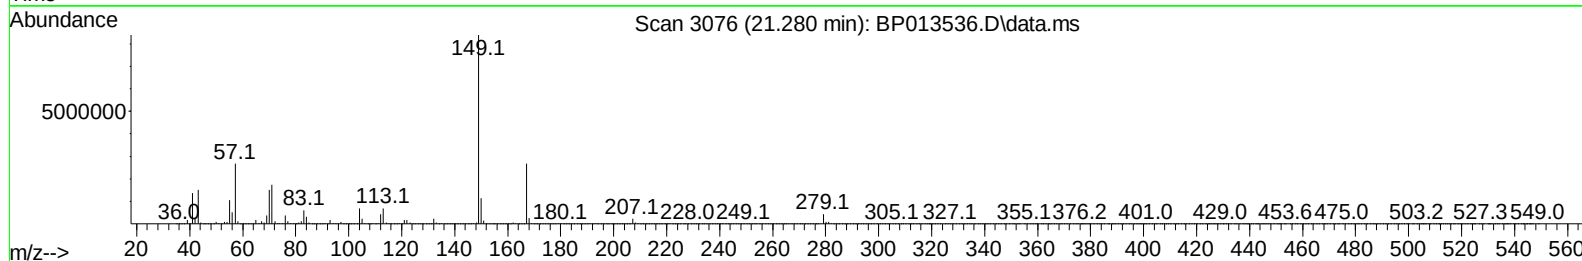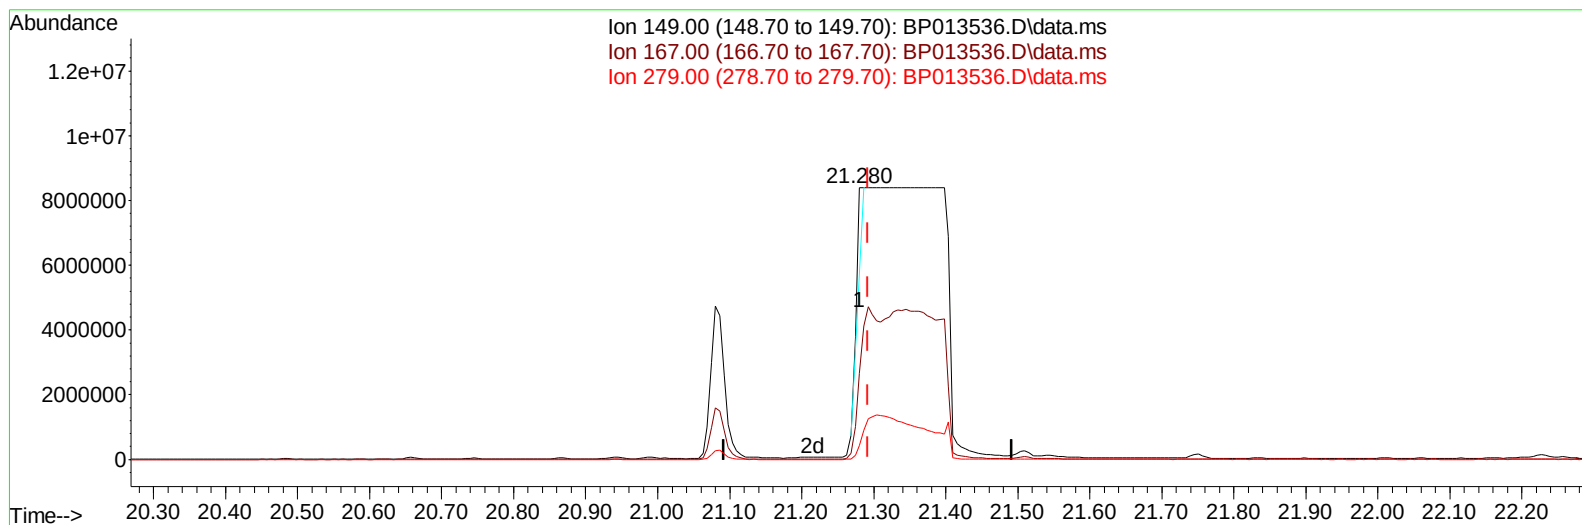

TIC: BP013536.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.280min (-0.012) 267.08 ng/ul

response 2661202

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	27.80	31.74
279.00	4.40	5.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013536.D
 Acq On : 18 Jan 2023 23:21
 Operator : CG/JU
 Sample : 01146-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4462

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:50:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

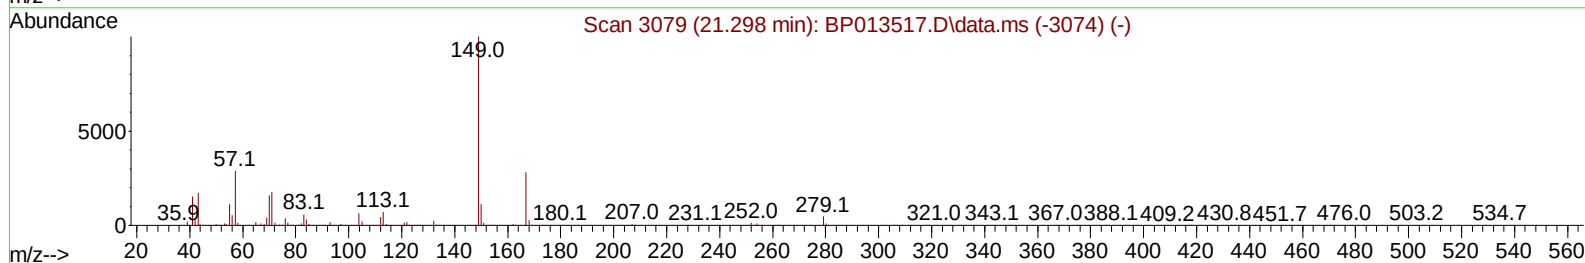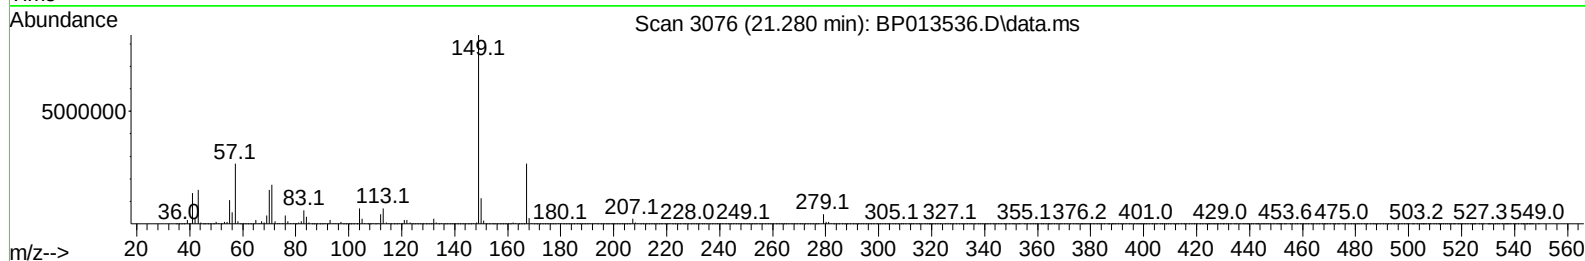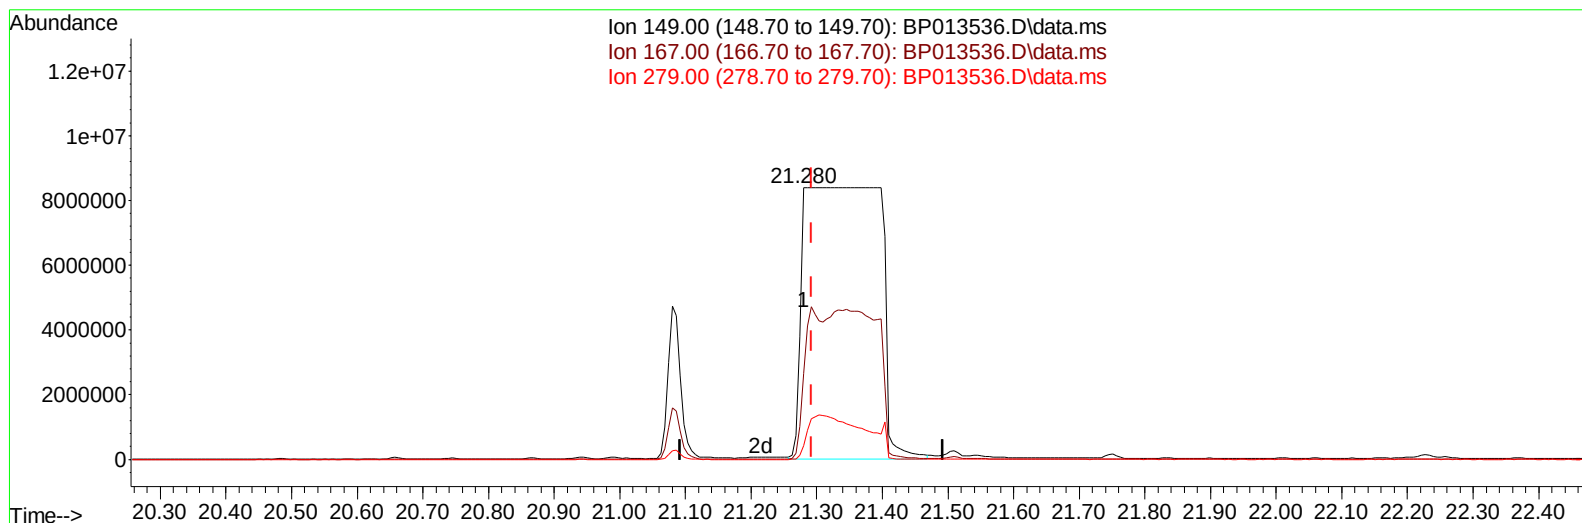

TIC: BP013536.D\data.ms

(86) Bis(2-ethylhexyl)phthalate

21.280min (-0.012) 6758.87 ng/ul m

response 67346657

Ion	Exp%	Act%
149.00	100.00	100.00
167.00	27.80	31.74
279.00	4.40	5.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013536.D
 Acq On : 18 Jan 2023 23:21
 Operator : CG/JU
 Sample : 01146-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4462

Manual IntegrationsAPPROVED

Quant Time: Jan 19 01:50:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.893	152		512469	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136		1879006	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164		1084422	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188		3686159	20.000	ng/ul	0.01
79) Chrysene-d12	21.404	240		357273m	20.000	ng/ul	0.00
88) Perylene-d12	23.851	264		3075693	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.293	96		38577	2.926	ng/uL	0.00
4) Pyridine-d5	3.746	84		33824m	0.920	ng/ul	0.02
7) Phenol-d5	7.058	99		728202	17.124	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67		446399	16.640	ng/ul	0.00
11) 2-Chlorophenol-d4	7.428	132		581531	18.338	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113		564827	17.434	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128		269853	20.170	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143		307316	20.983	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165		555902	19.046	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131		691236	16.811	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166		1553960	19.668	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160		1840691	21.047	ng/ul	0.00
54) 4-Nitrophenol-d4	14.751	143		122358	8.461	ng/ul	0.00
60) Fluorene-d10	15.539	176		1414778	20.273	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200		120565	5.158	ng/ul	0.01
73) Anthracene-d10	17.422	188		2233483	13.708	ng/ul	0.01
81) Pyrene-d10	19.639	212		2884199	148.375	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.692	264		3105199	20.553	ng/ul	0.00
Target Compounds							
86) Bis(2-ethylhexyl)phtha...	21.280	149		67346657m	6758.874	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013536.D
Acq On : 18 Jan 2023 23:21
Operator : CG/JU
Sample : 01146-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4462

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 19 01:50:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

