

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013501.D
 Acq On : 17 Jan 2023 19:05
 Operator : CG/JU
 Sample : 01145-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43S7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/18/2023
 Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 18 01:16:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	463609	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	1803553	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	1119828	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.310	188	2820104	20.000	ng/u1	0.00
79) Chrysene-d12	21.398	240	75167	20.000	ng/u1	# 0.00
88) Perylene-d12	23.868	264	3030868	20.000	ng/u1	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	28655	2.403	ng/uL	0.00
4) Pyridine-d5	3.746	84	36079	1.085	ng/u1	0.02
7) Phenol-d5	7.063	99	611488	15.895	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	374940	15.449	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	487433	16.990	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	488494	16.667	ng/u1	0.00
21) Nitrobenzene-d5	9.069	128	228273	17.776	ng/u1	0.00
24) 2-Nitrophenol-d4	9.793	143	264169	18.792	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	497711	17.766	ng/u1	0.00
31) 4-Chloroaniline-d4	10.851	131	586897	14.871	ng/u1	0.00
46) Dimethylphthalate-d6	13.957	166	1491341	18.279	ng/u1	0.00
49) Acenaphthylene-d8	14.240	160	1700045	18.824	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	198206	13.272	ng/u1	0.00
60) Fluorene-d10	15.545	176	1354972	18.802	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.681	200	216059	12.083	ng/u1	0.01
73) Anthracene-d10	17.410	188	2124492	17.044	ng/u1	0.00
81) Pyrene-d10	19.645	212	2750346	672.507	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.710	264	2842164	19.091	ng/u1	0.01

Target Compounds Qvalue
 86) Bis(2-ethylhexyl)phtha... 21.292 149 78200791m 37302.885 ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013501.D
Acq On : 17 Jan 2023 19:05
Operator : CG/JU
Sample : 01145-02
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A43S7

Quant Time: Jan 18 01:16:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/18/2023
Supervised By :mohammad ahmed 01/20/2023

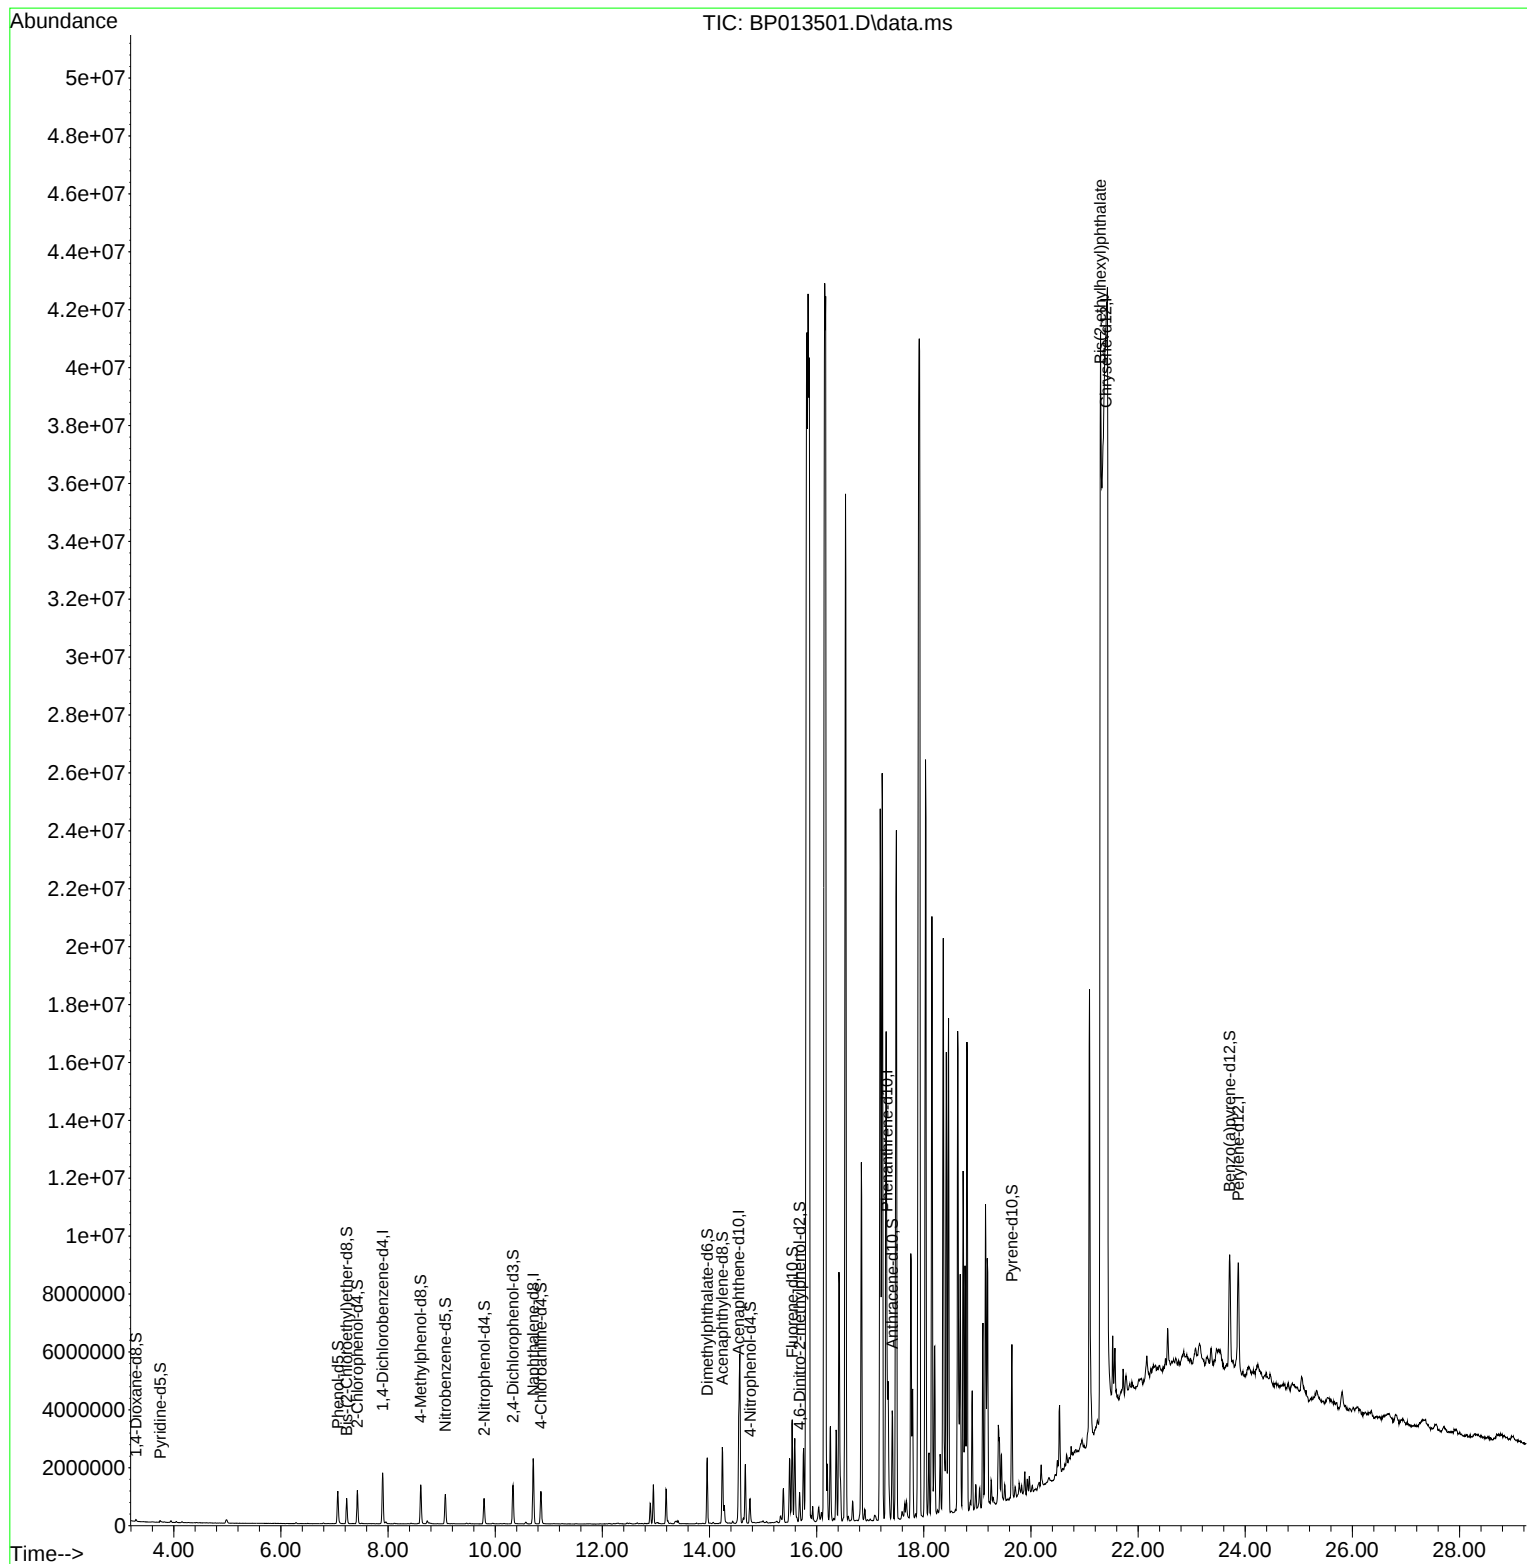

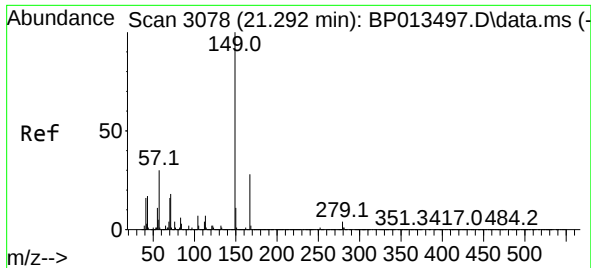

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 37302.885 ng/ul m
 RT: 21.292 min Scan# 3078
 Delta R.T. 0.000 min
 Lab File: BP013501.D
 Acq: 17 Jan 2023 19:05

Instrument :
 BNA_P
 ClientSampleId :
 A43S7

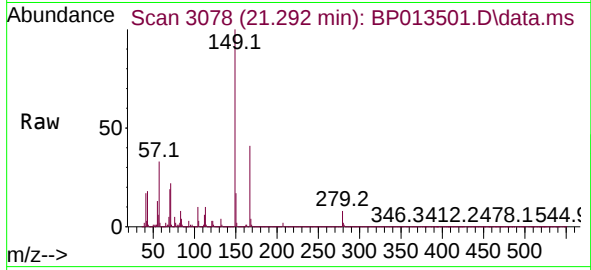

Tgt Ion:149 Resp:78200791
 Ion Ratio Lower Upper
 149 100
 167 40.8 22.2 33.4
 279 8.5 3.5 5.3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/18/2023
 Supervised By :mohammad ahmed 01/20/2023

