

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013504.D
 Acq On : 17 Jan 2023 20:48
 Operator : CG/JU
 Sample : 01145-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43T9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/18/2023
 Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 18 01:17:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	373563	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	1565290	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	1018768	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.310	188	2200314	20.000	ng/u1	0.00
79) Chrysene-d12	21.398	240	1993002	20.000	ng/u1	0.00
88) Perylene-d12	23.857	264	2517056	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	21363	2.223	ng/uL	0.00
4) Pyridine-d5	3.752	84	17836m	0.665	ng/u1	0.03
7) Phenol-d5	7.063	99	385496	12.436	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	246324	12.596	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	318078	13.760	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	313238	13.264	ng/u1	0.00
21) Nitrobenzene-d5	9.069	128	152702	13.701	ng/u1	0.00
24) 2-Nitrophenol-d4	9.793	143	176826	14.493	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	322523	13.265	ng/u1	0.00
31) 4-Chloroaniline-d4	10.851	131	394101	11.506	ng/u1	0.00
46) Dimethylphthalate-d6	13.957	166	1111342	14.973	ng/u1	0.00
49) Acenaphthylene-d8	14.240	160	1209650	14.723	ng/u1	0.00
54) 4-Nitrophenol-d4	14.757	143	122919	9.047	ng/u1	0.00
60) Fluorene-d10	15.545	176	967840	14.762	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	142425	10.208	ng/u1	0.00
73) Anthracene-d10	17.404	188	1568208	16.125	ng/u1	0.00
81) Pyrene-d10	19.639	212	1934222	17.838	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.692	264	2112633	17.087	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.292	149	2593360	46.657	ng/u1	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013504.D
Acq On : 17 Jan 2023 20:48
Operator : CG/JU
Sample : 01145-06
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A43T9

Quant Time: Jan 18 01:17:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/18/2023
Supervised By :mohammad ahmed 01/20/2023

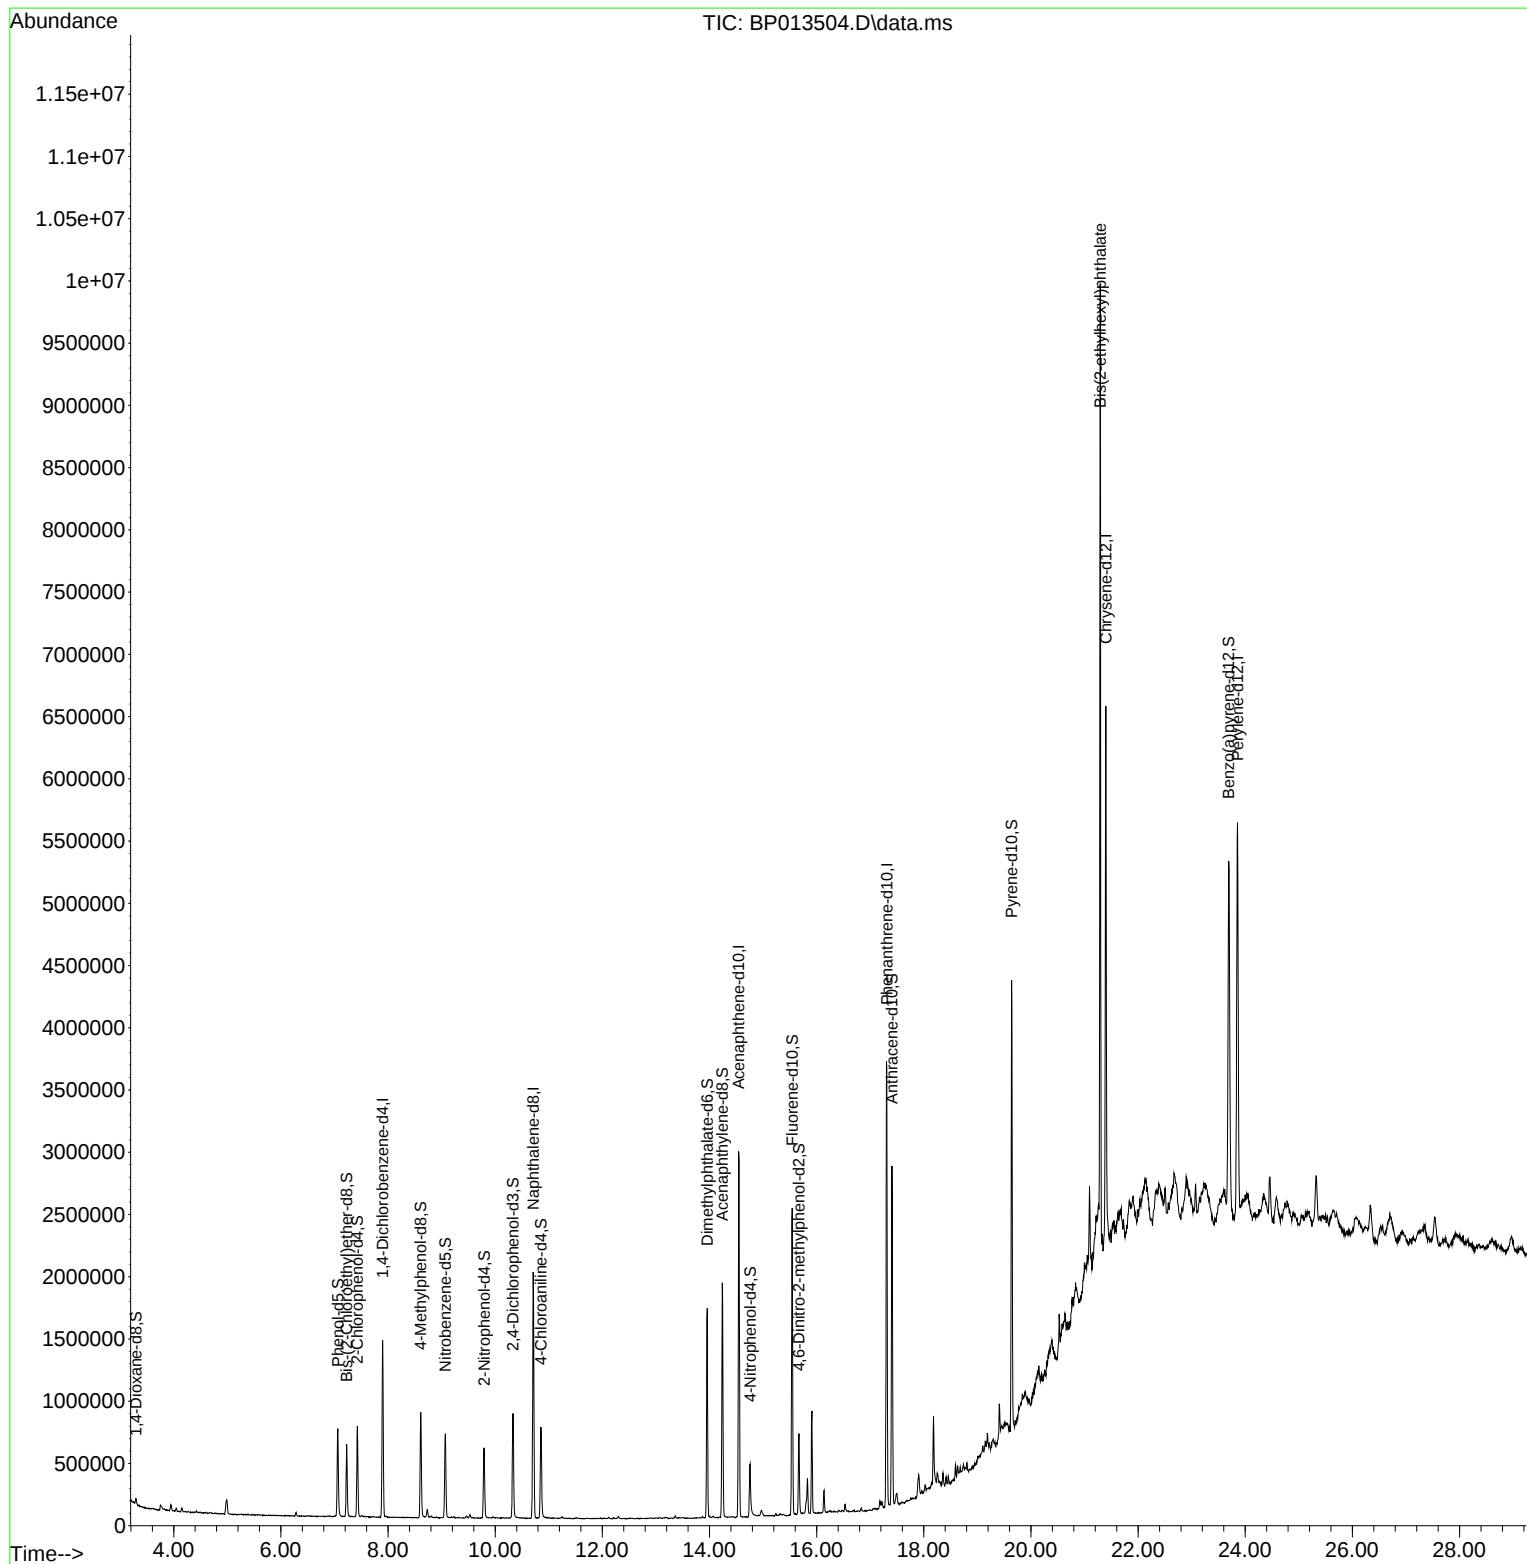

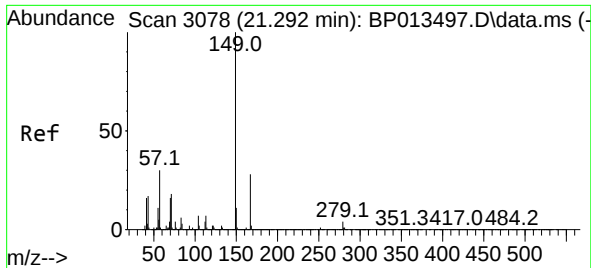

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 46.657 ng/ul
 RT: 21.292 min Scan# 3078
 Delta R.T. -0.000 min
 Lab File: BP013504.D
 Acq: 17 Jan 2023 20:48

Instrument :
 BNA_P
 ClientSampleId :
 A43T9

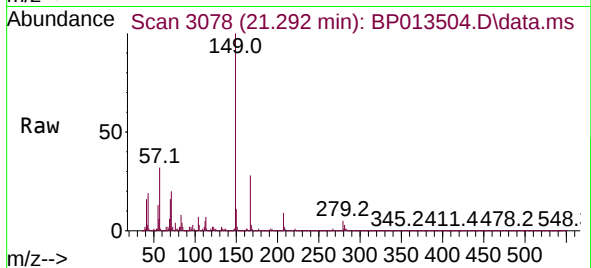

Tgt Ion:149 Resp: 2593360
 Ion Ratio Lower Upper
 149 100
 167 28.4 22.2 33.4
 279 4.7 3.5 5.3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/18/2023
 Supervised By :mohammad ahmed 01/20/2023

