

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013505.D
 Acq On : 17 Jan 2023 21:22
 Operator : CG/JU
 Sample : 01145-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43X9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/18/2023
 Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 18 01:17:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	422692	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	1692432	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	1048730	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.304	188	2390574	20.000	ng/u1	0.00
79) Chrysene-d12	21.398	240	2417469	20.000	ng/u1	0.00
88) Perylene-d12	23.857	264	2984567	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	34594	3.181	ng/uL	0.00
4) Pyridine-d5	3.746	84	38882	1.282	ng/u1	0.02
7) Phenol-d5	7.063	99	671732	19.152	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	421039	19.028	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	551740	21.094	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	535993	20.058	ng/u1	0.00
21) Nitrobenzene-d5	9.069	128	257612	21.378	ng/u1	0.00
24) 2-Nitrophenol-d4	9.793	143	299819	22.728	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	541620	20.602	ng/u1	0.00
31) 4-Chloroaniline-d4	10.852	131	654646	17.676	ng/u1	0.00
46) Dimethylphthalate-d6	13.957	166	1656254	21.677	ng/u1	0.00
49) Acenaphthylene-d8	14.240	160	1880340	22.232	ng/u1	0.00
54) 4-Nitrophenol-d4	14.751	143	210684	15.064	ng/u1	0.00
60) Fluorene-d10	15.545	176	1486008	22.018	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.669	200	241496	15.932	ng/u1	0.00
73) Anthracene-d10	17.404	188	2387992	22.600	ng/u1	0.00
81) Pyrene-d10	19.639	212	3048242	23.175	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.698	264	3341665	22.794	ng/u1	0.00

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.292	149	28014279m	415.506	ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013505.D
Acq On : 17 Jan 2023 21:22
Operator : CG/JU
Sample : 01145-11
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A43X9

Quant Time: Jan 18 01:17:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/18/2023
Supervised By :mohammad ahmed 01/20/2023

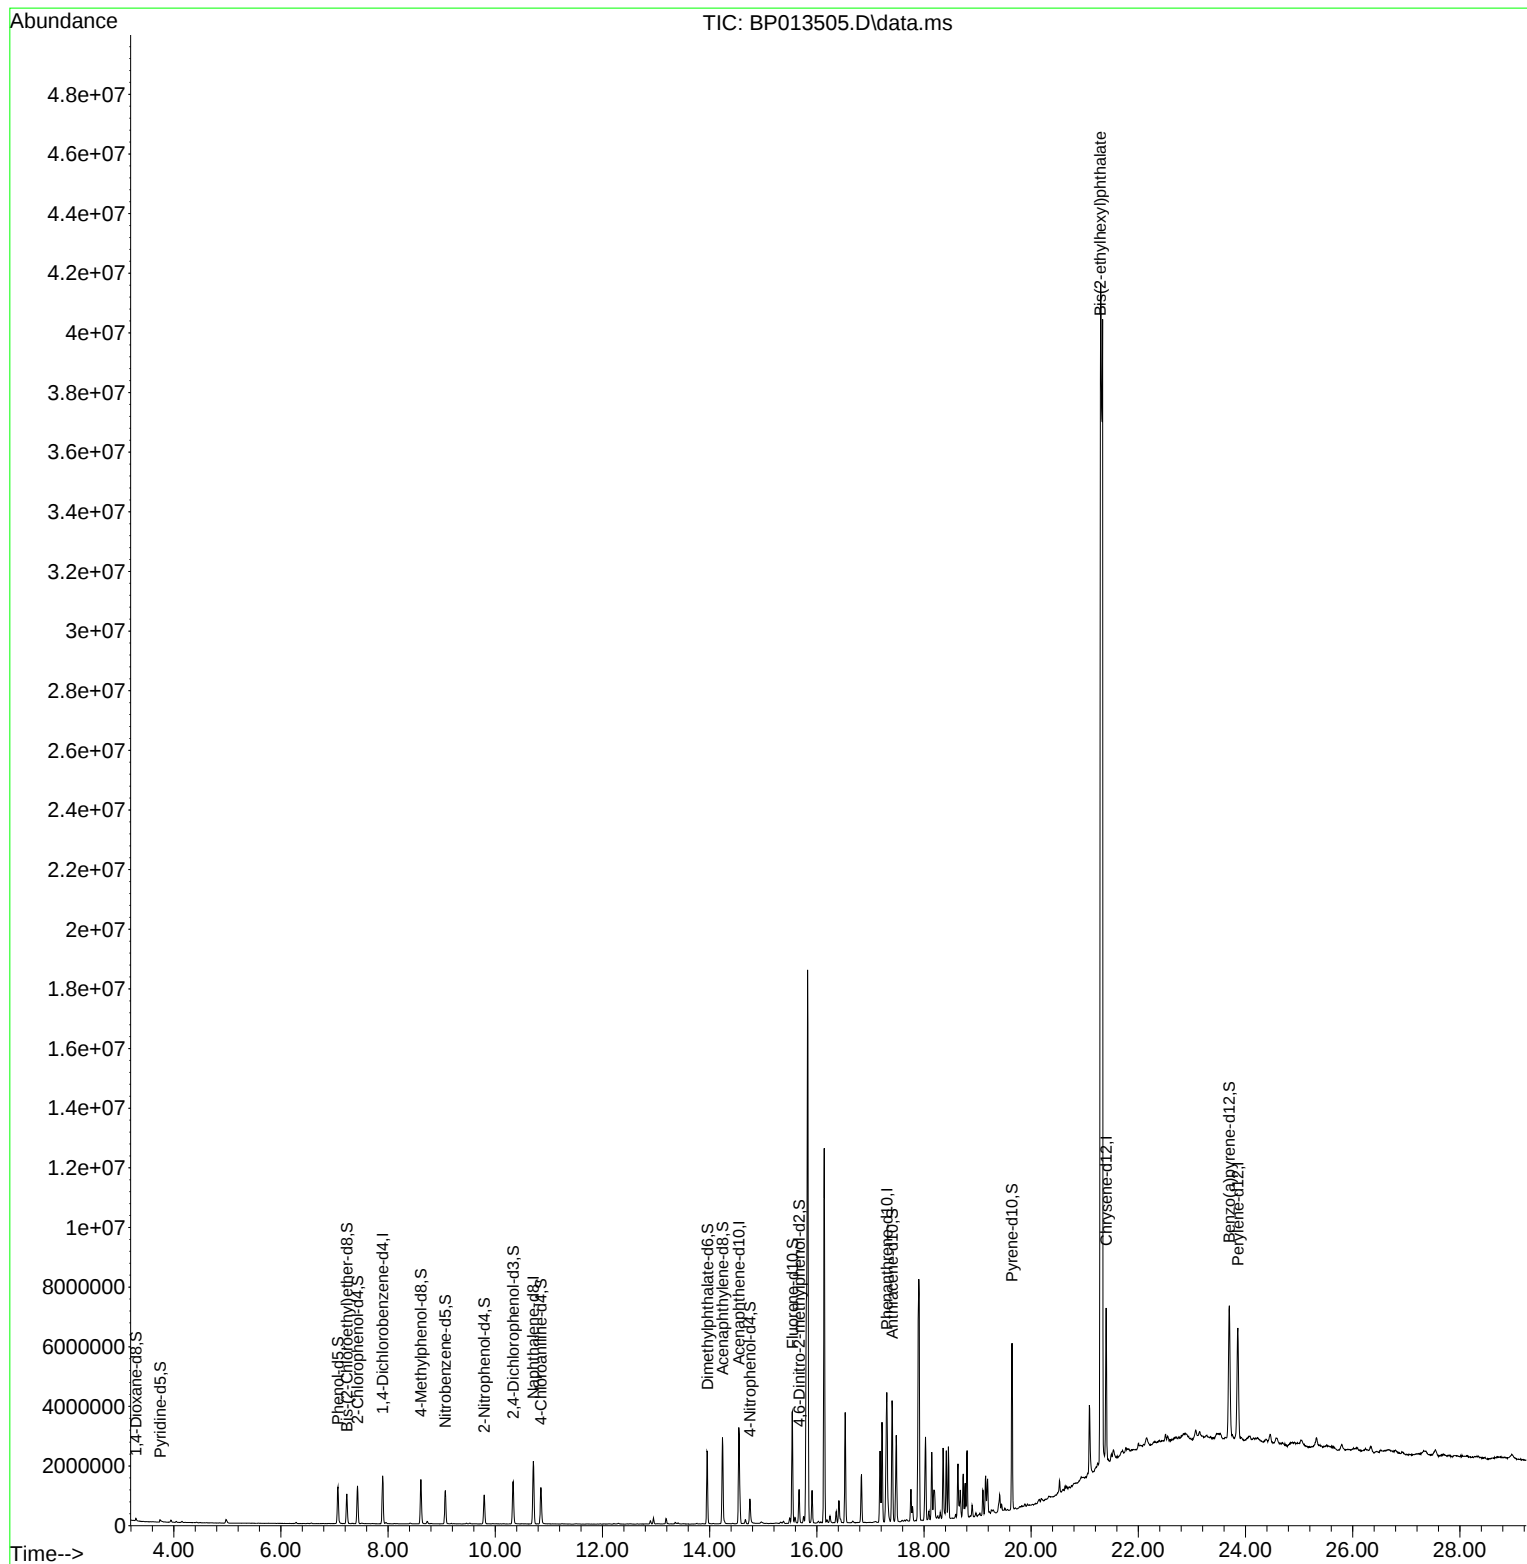

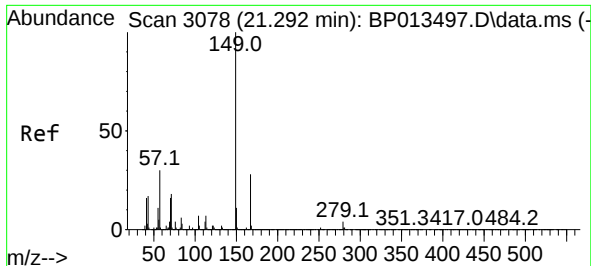

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 415.506 ng/ul m
 RT: 21.292 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: BP013505.D
 Acq: 17 Jan 2023 21:22

Instrument :
 BNA_P
 ClientSampleId :
 A43X9

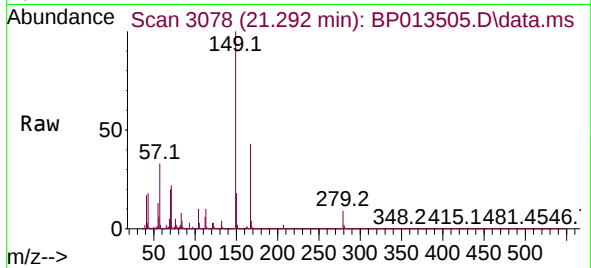

Tgt Ion:149 Resp:28014279
 Ion Ratio Lower Upper
 149 100
 167 42.6 22.2 33.4
 279 8.9 3.5 5.3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/18/2023
 Supervised By :mohammad ahmed 01/20/2023

