

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013525.D
 Acq On : 18 Jan 2023 17:04
 Operator : CG/JU
 Sample : 01145-11DL 30X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43X9DL

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 19 01:47:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	415464	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	1738554	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	1062584	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.304	188	2145155	20.000	ng/u1	0.00
79) Chrysene-d12	21.392	240	1899675	20.000	ng/u1	0.00
88) Perylene-d12	23.845	264	2309555	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	1524	0.143	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.063	99	20306	0.589	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	15744	0.724	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	16729m	0.651	ng/u1	0.00
15) 4-Methylphenol-d8	8.616	113	14091	0.536	ng/u1	0.00
21) Nitrobenzene-d5	9.069	128	6481	0.524	ng/u1	0.00
24) 2-Nitrophenol-d4	9.793	143	7406	0.547	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.340	165	12853	0.476	ng/u1	0.00
31) 4-Chloroaniline-d4	10.863	131	15341m	0.403	ng/u1	0.01
46) Dimethylphthalate-d6	13.957	166	51938	0.671	ng/u1	0.00
49) Acenaphthylene-d8	14.240	160	53015	0.619	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.540	176	46858	0.685	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.404	188	71877	0.758	ng/u1	0.00
81) Pyrene-d10	19.639	212	79751	0.772	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.686	264	82459	0.727	ng/u1	-0.01

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.292	149	4565629	86.175 ng/u1#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013525.D
Acq On : 18 Jan 2023 17:04
Operator : CG/JU
Sample : 01145-11DL 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A43X9DL

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
Supervised By :mohammad ahmed 01/20/2023


Quant Time: Jan 19 01:47:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

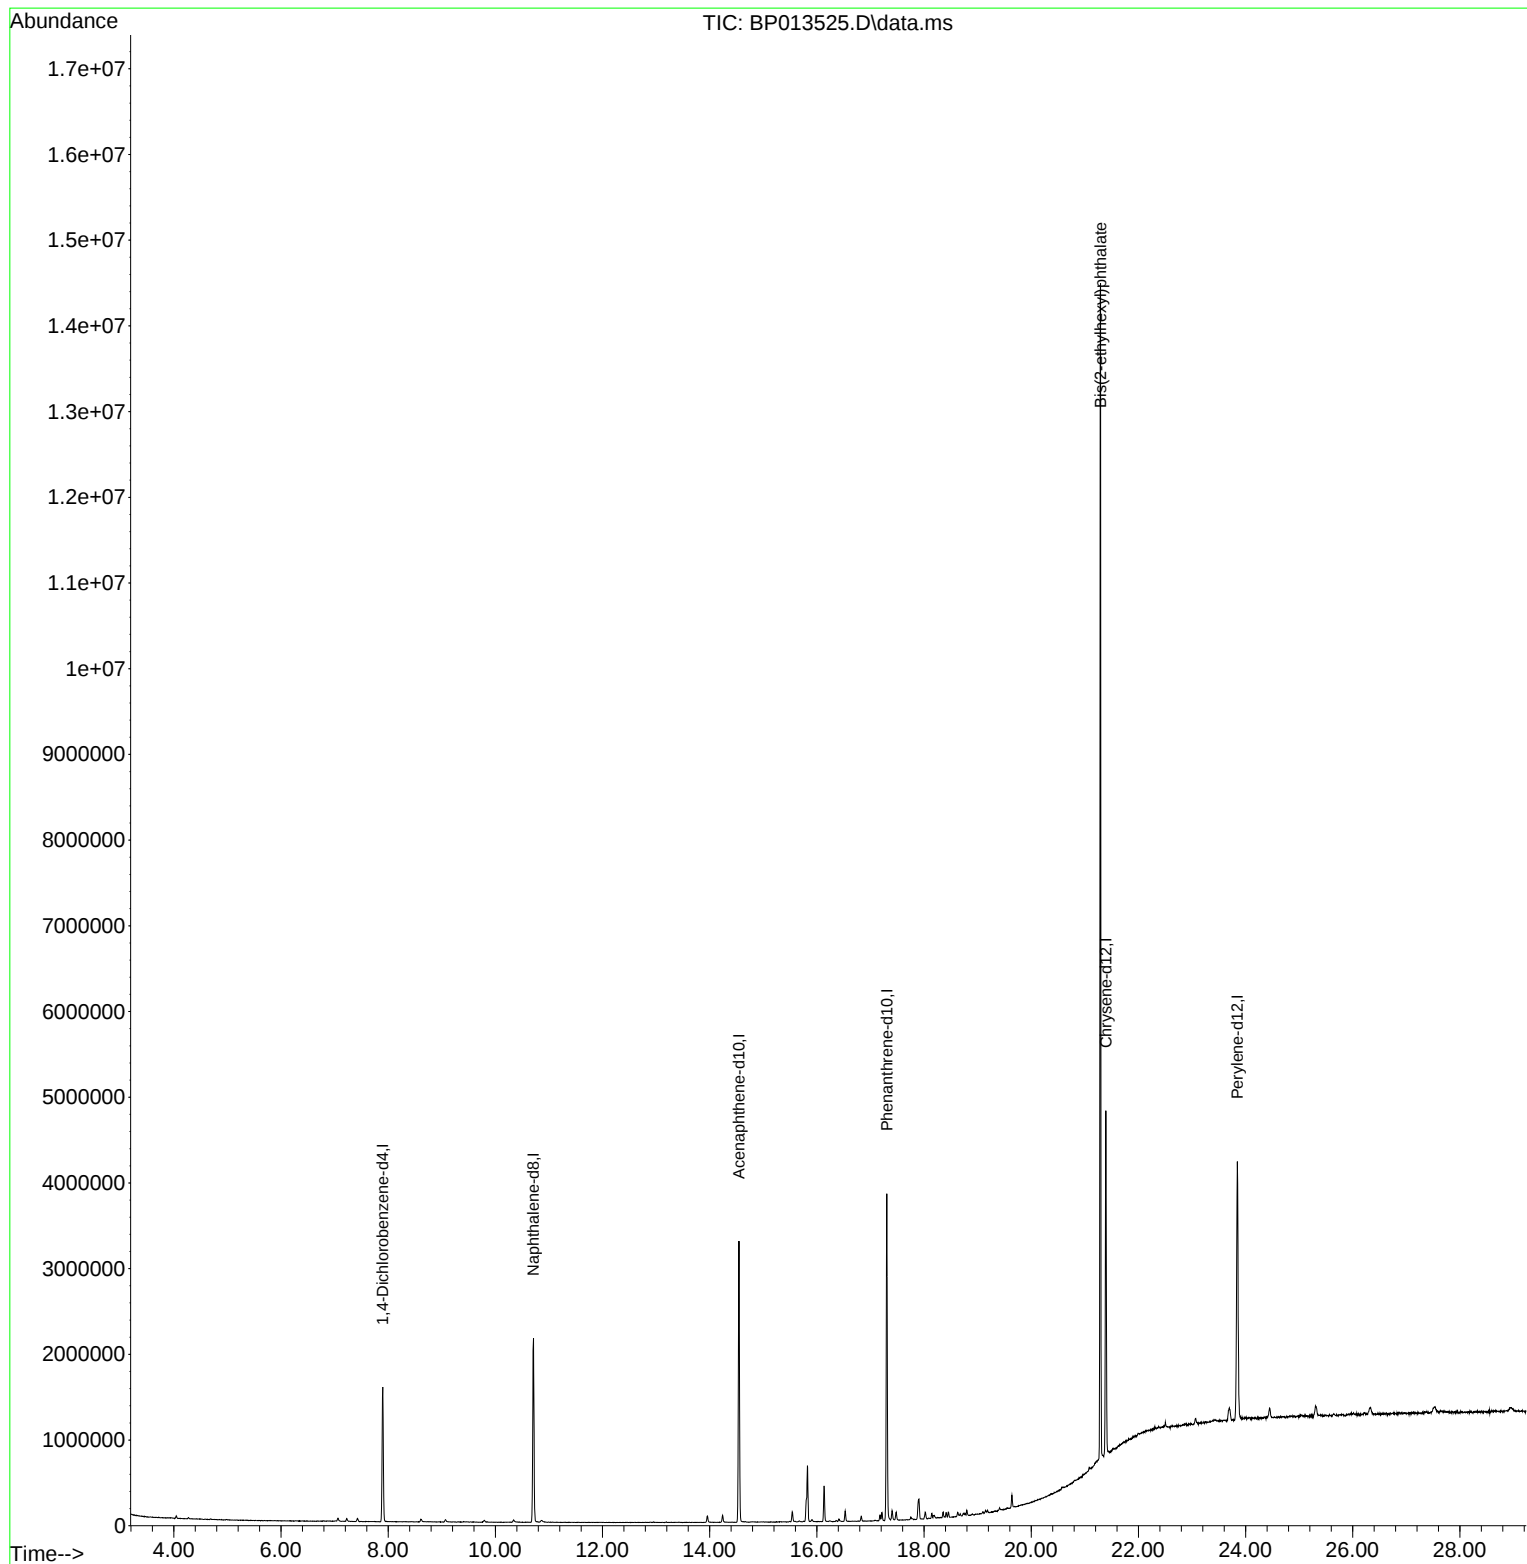

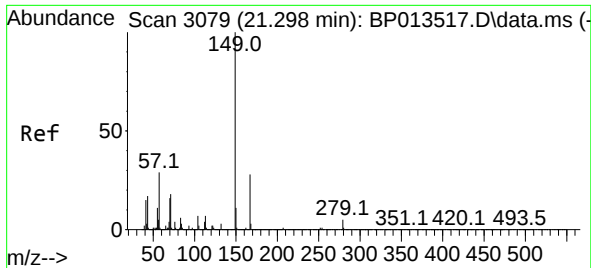

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 86.175 ng/ul
 RT: 21.292 min Scan# 3078
 Delta R.T. 0.000 min
 Lab File: BP013525.D
 Acq: 18 Jan 2023 17:04

Instrument :
 BNA_P
 ClientSampleId :
 A43X9DL

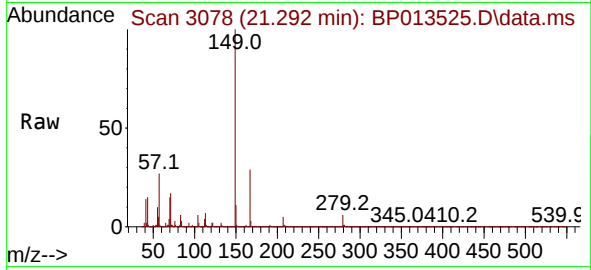

Tgt Ion:149 Resp: 4565629
 Ion Ratio Lower Upper
 149 100
 167 29.2 22.2 33.4
 279 5.6 3.5 5.3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

