

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013530.D
 Acq On : 18 Jan 2023 19:55
 Operator : CG/JU
 Sample : 01146-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A43Z9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 19 01:48:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	411828	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	1608902	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	935878	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.304	188	1871186	20.000	ng/u1	0.00
79) Chrysene-d12	21.392	240	1772400	20.000	ng/u1	0.00
88) Perylene-d12	23.839	264	2295141	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	40506	3.823	ng/uL	0.00
4) Pyridine-d5	3.758	84	21565m	0.730	ng/u1	0.04
7) Phenol-d5	7.058	99	751991	22.005	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	495021	22.961	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	623749	24.476	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	593770	22.806	ng/u1	0.00
21) Nitrobenzene-d5	9.069	128	297186	25.942	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	334297	26.658	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	596371	23.863	ng/u1	0.00
31) 4-Chloroaniline-d4	10.851	131	310911	8.831	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	1710159	25.081	ng/u1	0.00
49) Acenaphthylene-d8	14.240	160	1965908	26.047	ng/u1	0.00
54) 4-Nitrophenol-d4	14.751	143	164874	13.210	ng/u1	0.00
60) Fluorene-d10	15.539	176	1494933	24.822	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	199675	16.829	ng/u1	0.00
73) Anthracene-d10	17.404	188	2149048	25.984	ng/u1	0.00
81) Pyrene-d10	19.639	212	2624784	27.219	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.680	264	3033831	26.910	ng/u1	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.286	149	2323609	47.007	ng/u1	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013530.D
Acq On : 18 Jan 2023 19:55
Operator : CG/JU
Sample : 01146-04
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A43Z9

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 19 01:48:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

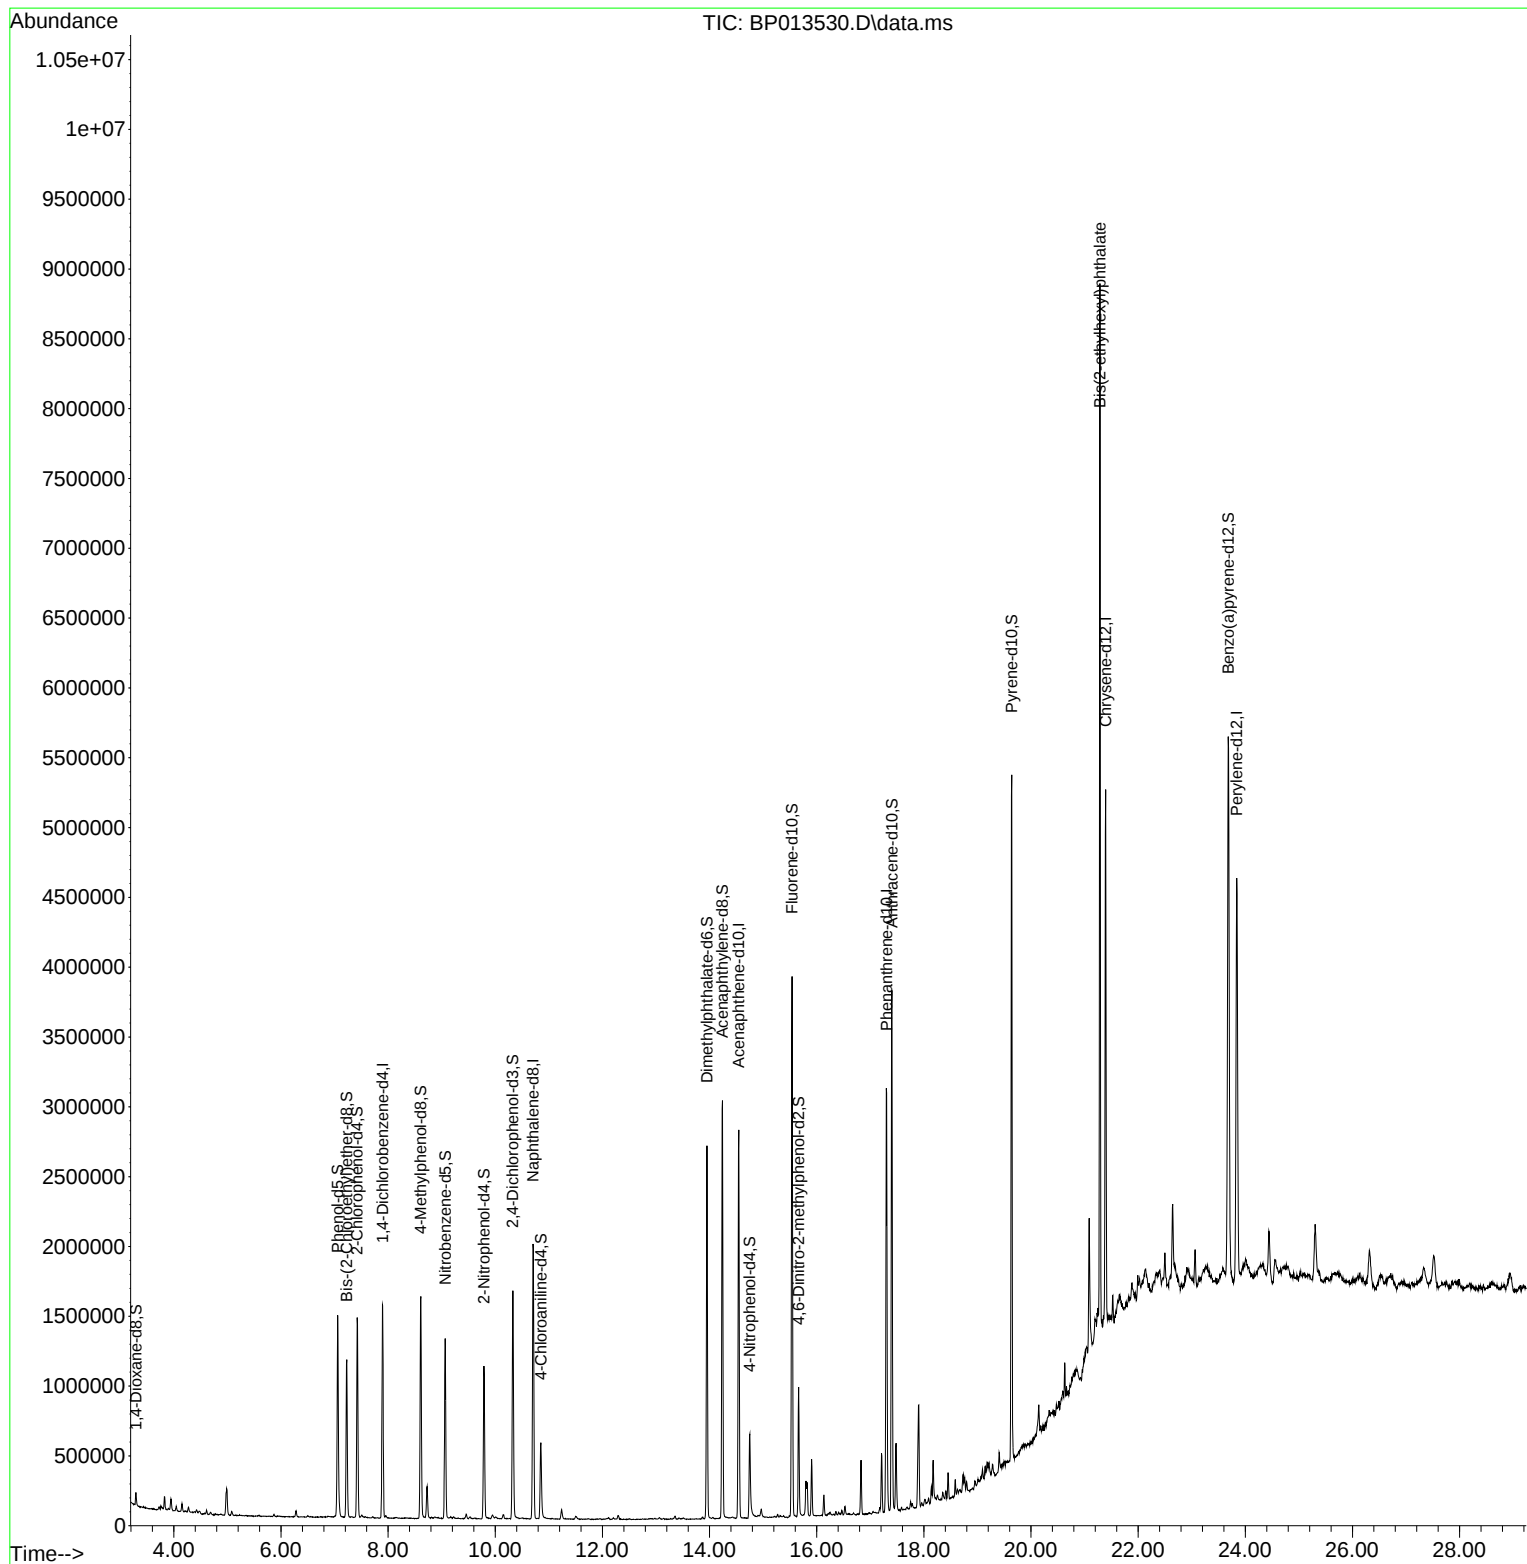

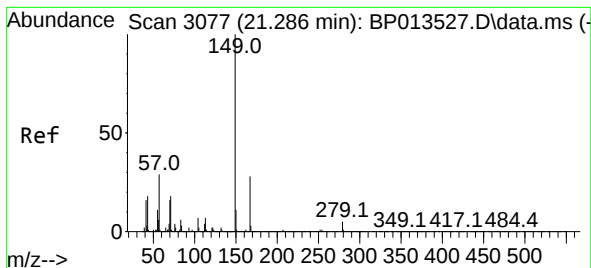

#86

Bis(2-ethylhexyl)phthalate

Concen: 47.007 ng/ul

RT: 21.286 min Scan# 3077

Delta R.T. -0.006 min

Lab File: BP013530.D

Acq: 18 Jan 2023 19:55

Instrument :

BNA_P

ClientSampleId :

A43Z9

Tgt Ion:149 Resp: 2323609

Ion Ratio Lower Upper

149 100

167 28.3 22.2 33.4

279 4.8 3.5 5.3

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023

Supervised By :mohammad ahmed 01/20/2023

