

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013531.D
 Acq On : 18 Jan 2023 20:29
 Operator : CG/JU
 Sample : 01146-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4405

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 19 01:49:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	452167	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	1736567	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	1097389	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.322	188	2181878	20.000	ng/u1	0.01
79) Chrysene-d12	21.404	240	34355m	20.000	ng/u1	0.00
88) Perylene-d12	23.880	264	2677912	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	33364	2.868	ng/uL	0.00
4) Pyridine-d5	3.752	84	22878m	0.705	ng/u1	0.03
7) Phenol-d5	7.057	99	683902	18.228	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	416753	17.606	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	554090	19.803	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	536036	18.752	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	245871	19.885	ng/u1	0.00
24) 2-Nitrophenol-d4	9.793	143	287008	21.204	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	537111	19.912	ng/u1	0.00
31) 4-Chloroaniline-d4	10.851	131	299538	7.882	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	1543682	19.308	ng/u1	0.00
49) Acenaphthylene-d8	14.239	160	1818658	20.550	ng/u1	0.00
54) 4-Nitrophenol-d4	14.857	143	185733m	12.691	ng/u1	0.11
60) Fluorene-d10	15.545	176	1812970	25.672	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	149398m	10.799	ng/u1	0.08
73) Anthracene-d10	17.416	188	2012217	20.865	ng/u1	0.00
81) Pyrene-d10	19.651	212	2754380	1473.570	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.721	264	2701351	20.536	ng/u1	0.02

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.280	149	144188631m	150487.199	ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013531.D
Acq On : 18 Jan 2023 20:29
Operator : CG/JU
Sample : 01146-08
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A4405

Quant Time: Jan 19 01:49:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/19/2023
Supervised By :mohammad ahmed 01/20/2023

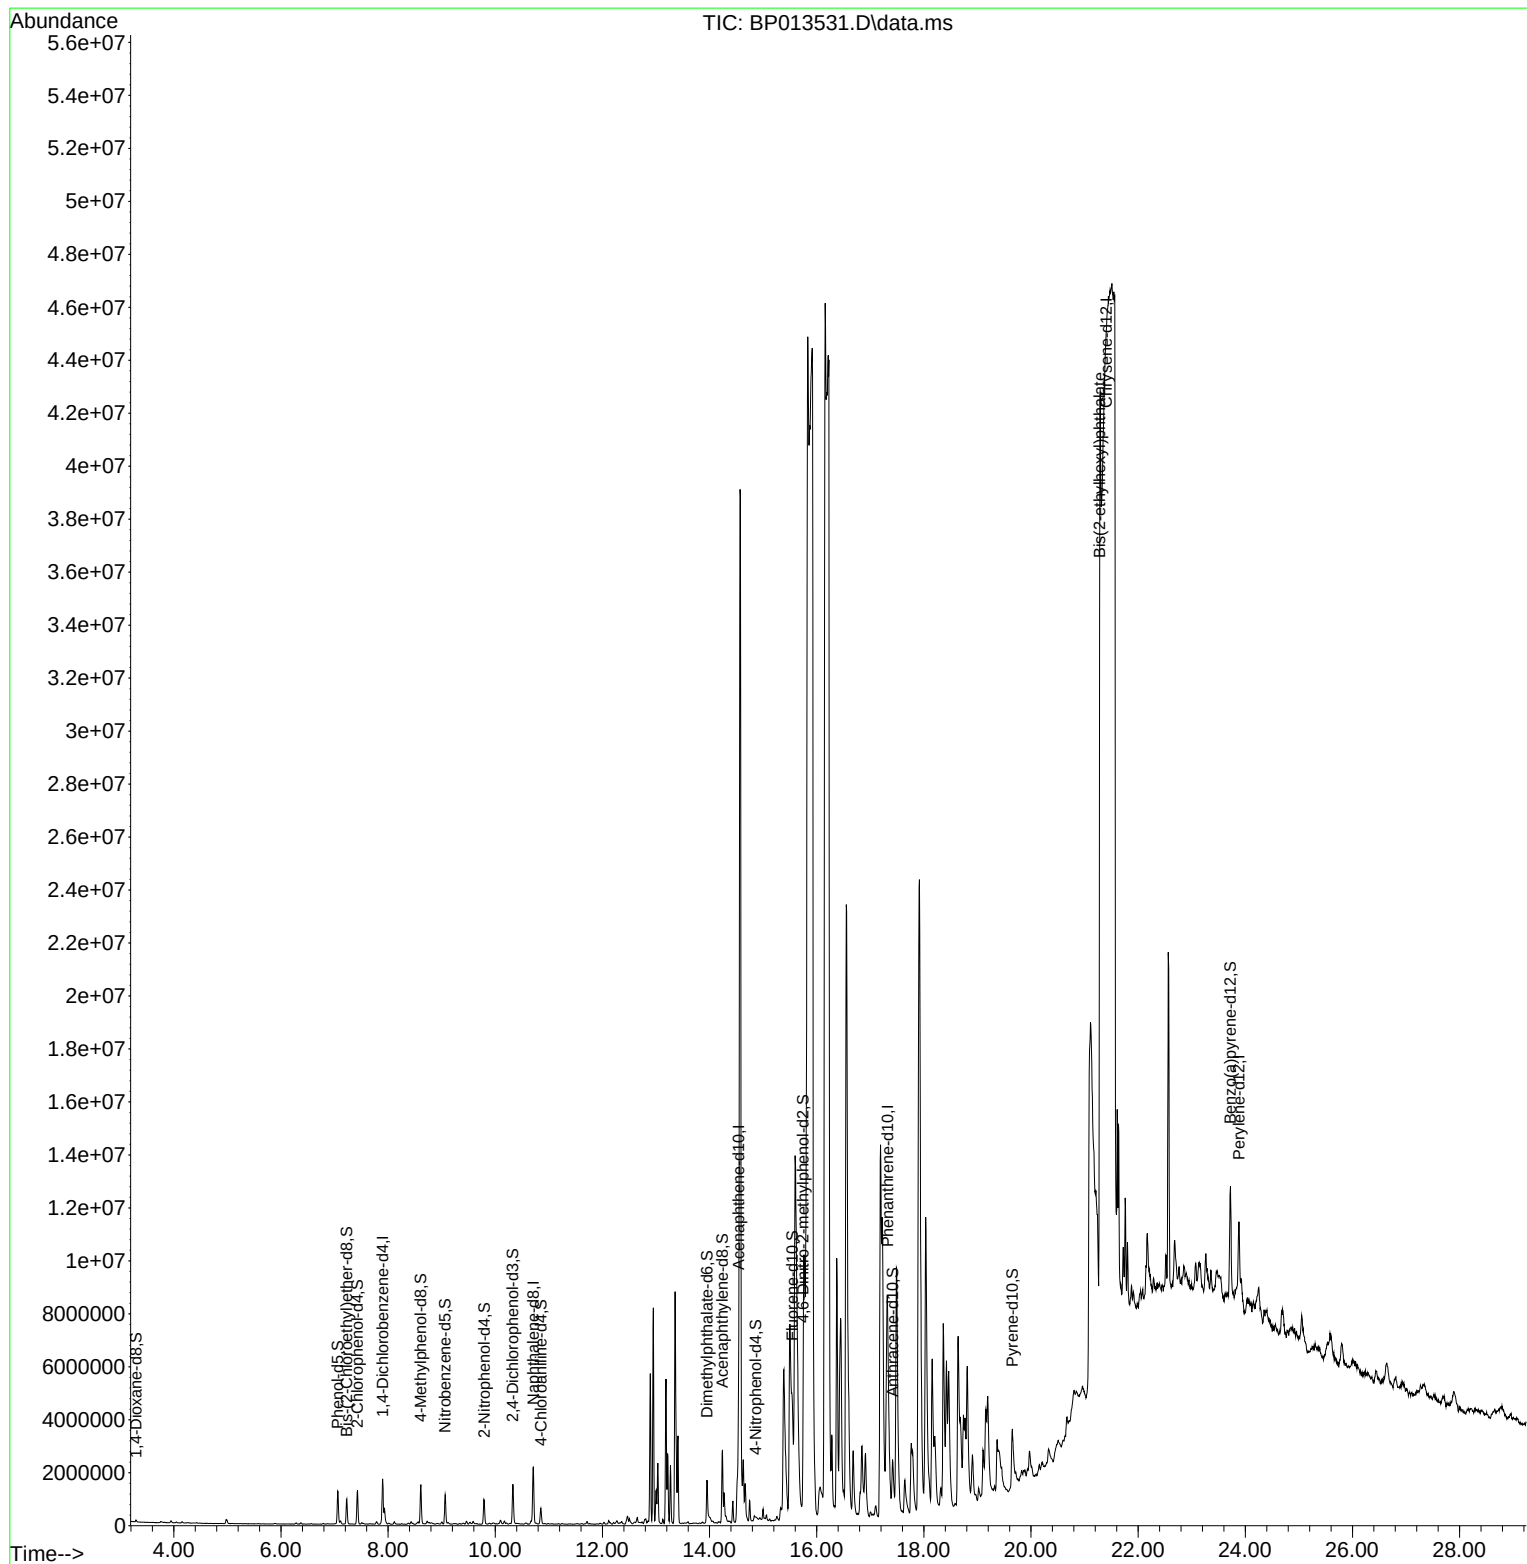

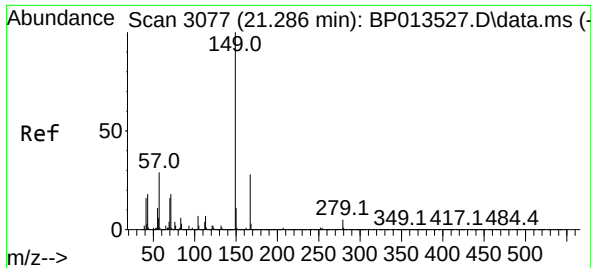

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 150487.199 ng/ul m
 RT: 21.280 min Scan# 3076
 Delta R.T. -0.012 min
 Lab File: BP013531.D
 Acq: 18 Jan 2023 20:29

Instrument :
 BNA_P
 ClientSampleId :
 A4405

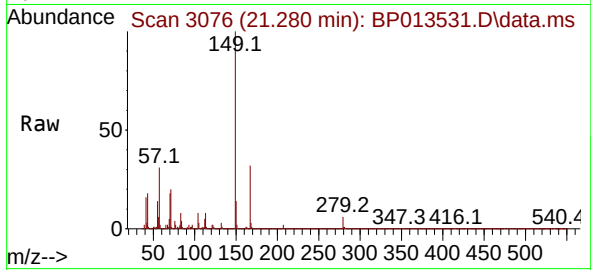

Tgt Ion:149 Resp:1441886
 Ion Ratio Lower Upper
 149 100
 167 31.7 22.2 33.4
 279 5.7 3.5 5.3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

