

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013533.D
 Acq On : 18 Jan 2023 21:38
 Operator : CG/JU
 Sample : 01146-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4412

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

Quant Time: Jan 19 01:49:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	444813	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	1712155	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	970722	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.304	188	2122275	20.000	ng/u1	0.00
79) Chrysene-d12	21.392	240	2126955	20.000	ng/u1	0.00
88) Perylene-d12	23.845	264	2719181	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	41987	3.669	ng/uL	0.00
4) Pyridine-d5	3.728	84	226752	7.104	ng/u1	0.00
7) Phenol-d5	7.057	99	778309	21.087	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	473592	20.338	ng/u1	0.00
11) 2-Chlorophenol-d4	7.428	132	627325	22.790	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	617412	21.956	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	290569	23.835	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	336055	25.182	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	614837	23.118	ng/u1	0.00
31) 4-Chloroaniline-d4	10.851	131	517993	13.825	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	1719261	24.310	ng/u1	0.00
49) Acenaphthylene-d8	14.239	160	2006261	25.627	ng/u1	0.00
54) 4-Nitrophenol-d4	14.751	143	231887	17.913	ng/u1	0.00
60) Fluorene-d10	15.539	176	1534258	24.560	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	233624	17.361	ng/u1	0.00
73) Anthracene-d10	17.404	188	2370135	25.266	ng/u1	0.00
81) Pyrene-d10	19.639	212	3032732	26.207	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.686	264	3498781	26.195	ng/u1	-0.01

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.286	149	31037446m	523.222	ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013533.D
Acq On : 18 Jan 2023 21:38
Operator : CG/JU
Sample : 01146-11
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A4412

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
Supervised By :mohammad ahmed 01/20/2023


Quant Time: Jan 19 01:49:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

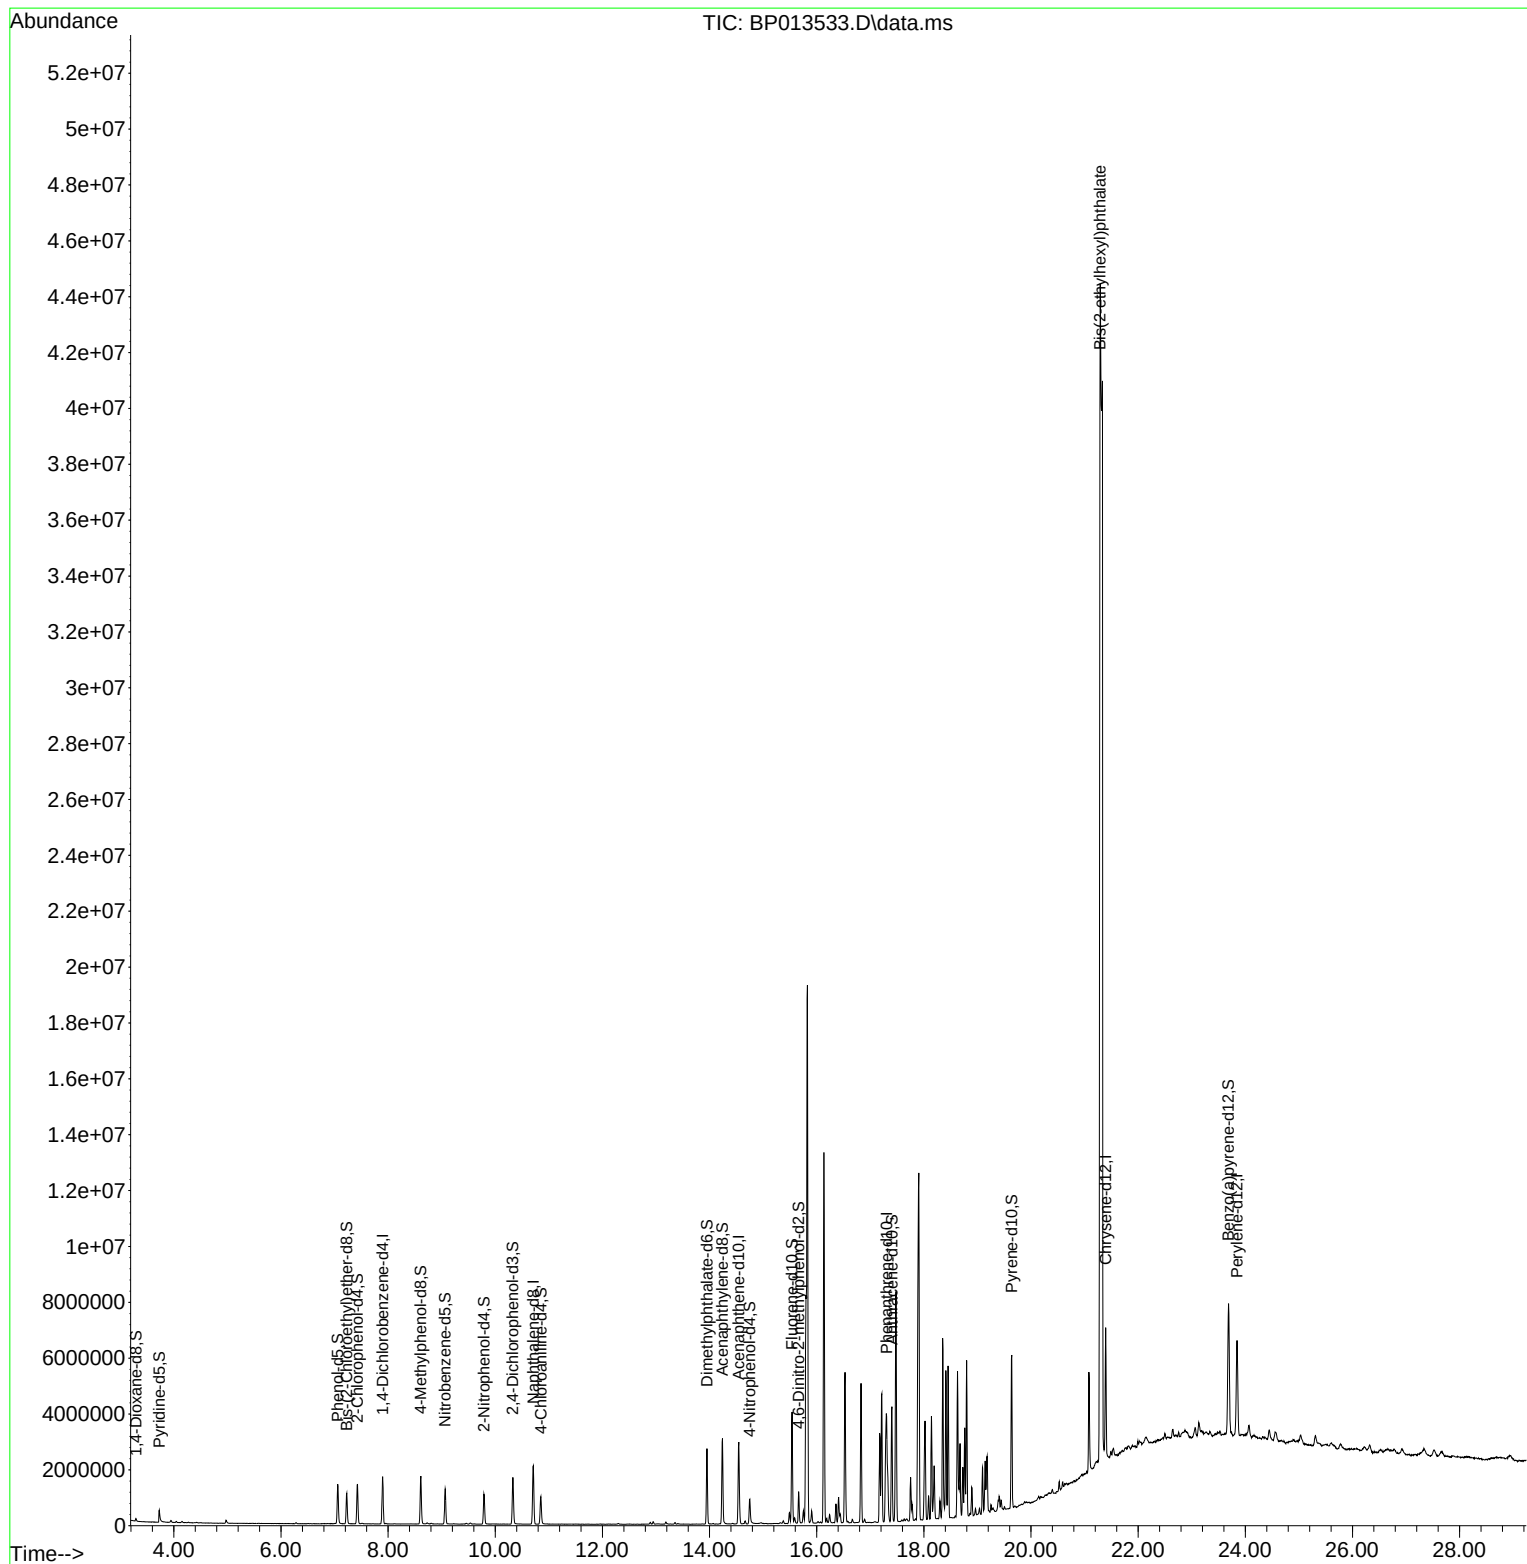

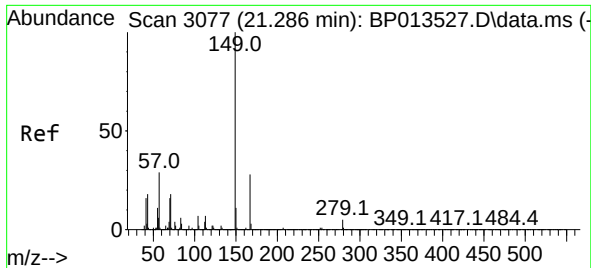

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 523.222 ng/ul m
 RT: 21.286 min Scan# 3077
 Delta R.T. -0.006 min
 Lab File: BP013533.D
 Acq: 18 Jan 2023 21:38

Instrument :
 BNA_P
 ClientSampleId :
 A4412

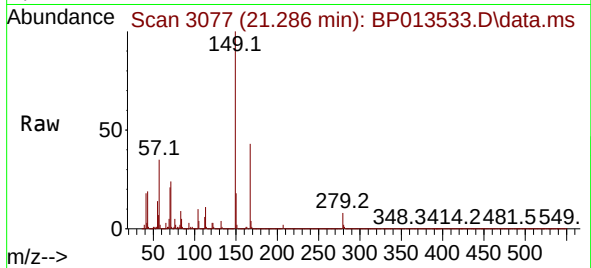

Tgt Ion:149 Resp:31037440
 Ion Ratio Lower Upper
 149 100
 167 43.0 22.2 33.4
 279 8.5 3.5 5.3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/19/2023
 Supervised By :mohammad ahmed 01/20/2023

