

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013535.D
 Acq On : 18 Jan 2023 22:46
 Operator : CG/JU
 Sample : 01146-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4424

Quant Time: Jan 19 01:49:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 18 01:06:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	468718	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	1878277	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	1109253	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.304	188	2226930	20.000	ng/u1	0.00
79) Chrysene-d12	21.392	240	1979464	20.000	ng/u1	0.00
88) Perylene-d12	23.839	264	2590555	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	51584	4.278	ng/uL	0.00
4) Pyridine-d5	3.716	84	716229	21.295	ng/u1	0.00
7) Phenol-d5	7.057	99	909600	23.387	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	572069	23.315	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	741087	25.550	ng/u1	0.00
15) 4-Methylphenol-d8	8.610	113	717047	24.199	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	355622	26.591	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	415211	28.361	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	727981	24.951	ng/u1	0.00
31) 4-Chloroaniline-d4	10.845	131	957703	23.301	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	2006440	24.827	ng/u1	0.00
49) Acenaphthylene-d8	14.239	160	2372303	26.519	ng/u1	0.00
54) 4-Nitrophenol-d4	14.751	143	260323	17.598	ng/u1	0.00
60) Fluorene-d10	15.539	176	1748909	24.500	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.663	200	249273	17.653	ng/u1	0.00
73) Anthracene-d10	17.398	188	2524535	25.648	ng/u1	-0.01
81) Pyrene-d10	19.633	212	2804565	26.041	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.680	264	3223329	25.331	ng/u1	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.286	149	789256	14.296	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013535.D
Acq On : 18 Jan 2023 22:46
Operator : CG/JU
Sample : 01146-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4424

Quant Time: Jan 19 01:49:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 18 01:06:35 2023
Response via : Initial Calibration

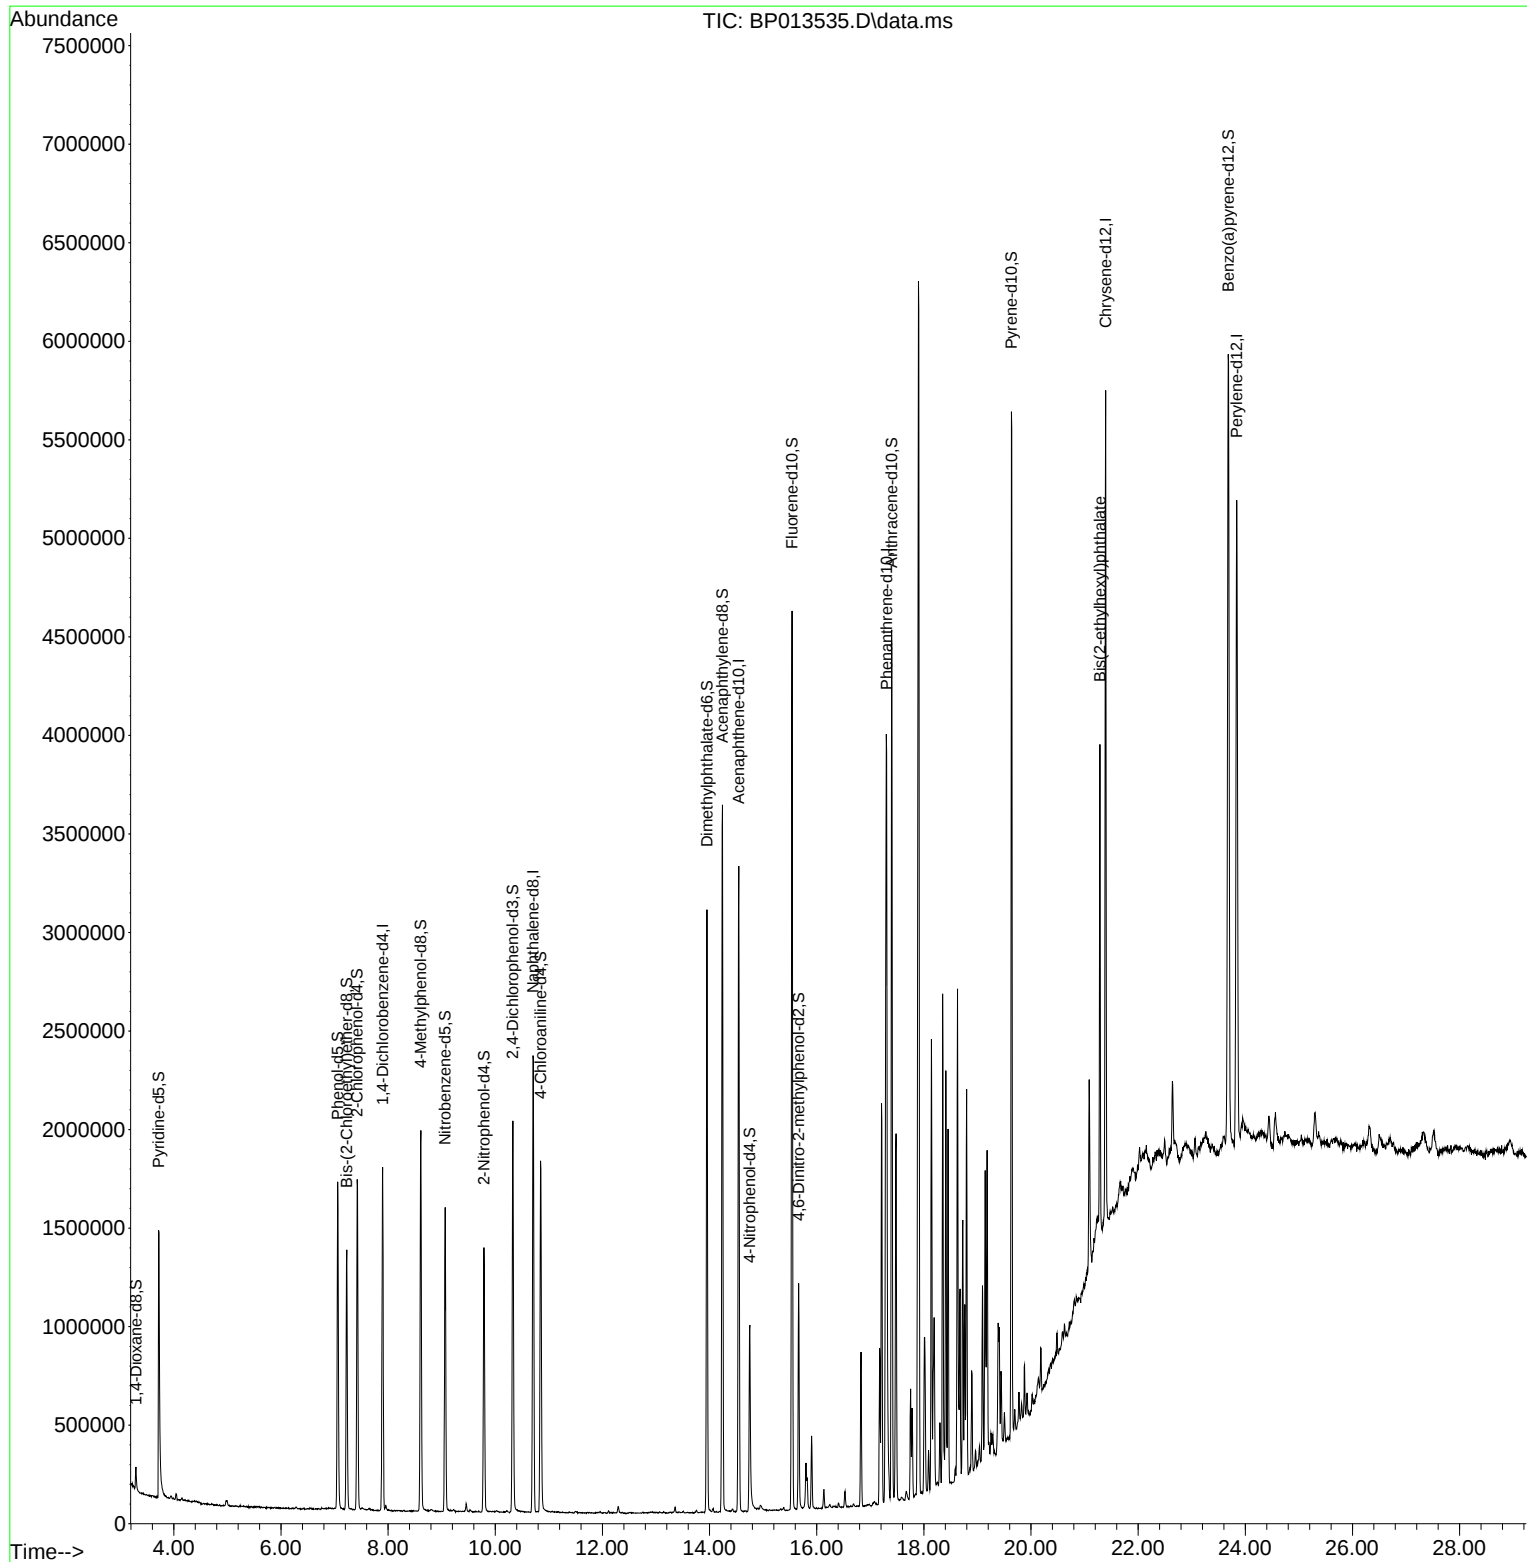

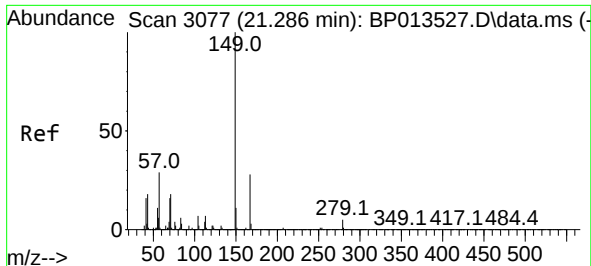

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 14.296 ng/ul
 RT: 21.286 min Scan# 3077
 Delta R.T. -0.006 min
 Lab File: BP013535.D
 Acq: 18 Jan 2023 22:46

Instrument :
 BNA_P
 ClientSampleId :
 A4424

Tgt Ion:149 Resp: 789256
 Ion Ratio Lower Upper
 149 100
 167 28.6 22.2 33.4
 279 4.9 3.5 5.3

