

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013510.D
 Acq On : 18 Jan 2023 00:14
 Operator : CG/JU
 Sample : PB150250BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK250

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.552	58	62	68	rVB	185408	216471	2.90%	0.577%
2	3.646	76	78	82	rVB5	16813	17313	0.23%	0.046%
3	4.040	141	145	152	rVB	51213	72876	0.98%	0.194%
4	4.175	166	168	175	rVB7	8347	13033	0.17%	0.035%
5	4.987	301	306	313	rBV	120658	169790	2.28%	0.452%
6	6.528	563	568	569	rBV5	6048	8566	0.11%	0.023%
7	7.899	793	801	810	rBV	2396542	3765730	50.50%	10.029%
8	10.710	1271	1279	1292	rVV	3030231	5080248	68.12%	13.530%
9	14.545	1923	1931	1940	rBV	4469340	6444354	86.42%	17.163%
10	14.992	2004	2007	2012	rVB7	6199	8419	0.11%	0.022%
11	15.245	2044	2050	2053	rBV7	7860	12314	0.17%	0.033%
12	17.086	2359	2363	2368	rBV3	12503	20277	0.27%	0.054%
13	17.304	2392	2400	2412	rBV	5275541	7457377	100.00%	19.861%
14	17.963	2510	2512	2517	rVB6	13790	15809	0.21%	0.042%
15	18.180	2545	2549	2556	rBV2	63070	105361	1.41%	0.281%
16	19.410	2756	2758	2763	rBV5	39698	53713	0.72%	0.143%
17	21.398	3091	3096	3103	rBV	5504360	6970131	93.47%	18.564%
18	23.851	3507	3513	3522	rVB2	3572927	7115717	95.42%	18.951%




Sum of corrected areas: 37547499

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013510.D
Acq On : 18 Jan 2023 00:14
Operator : CG/JU
Sample : PB150250BL
Misc : GCMS CONFIRMATION
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK250

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

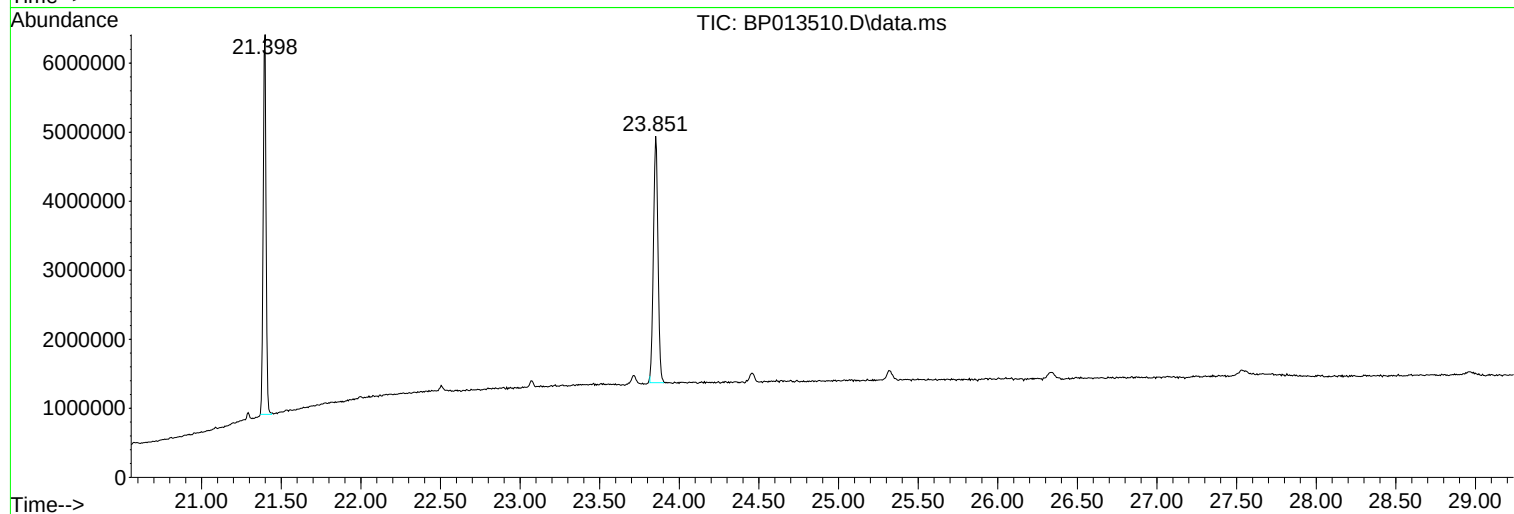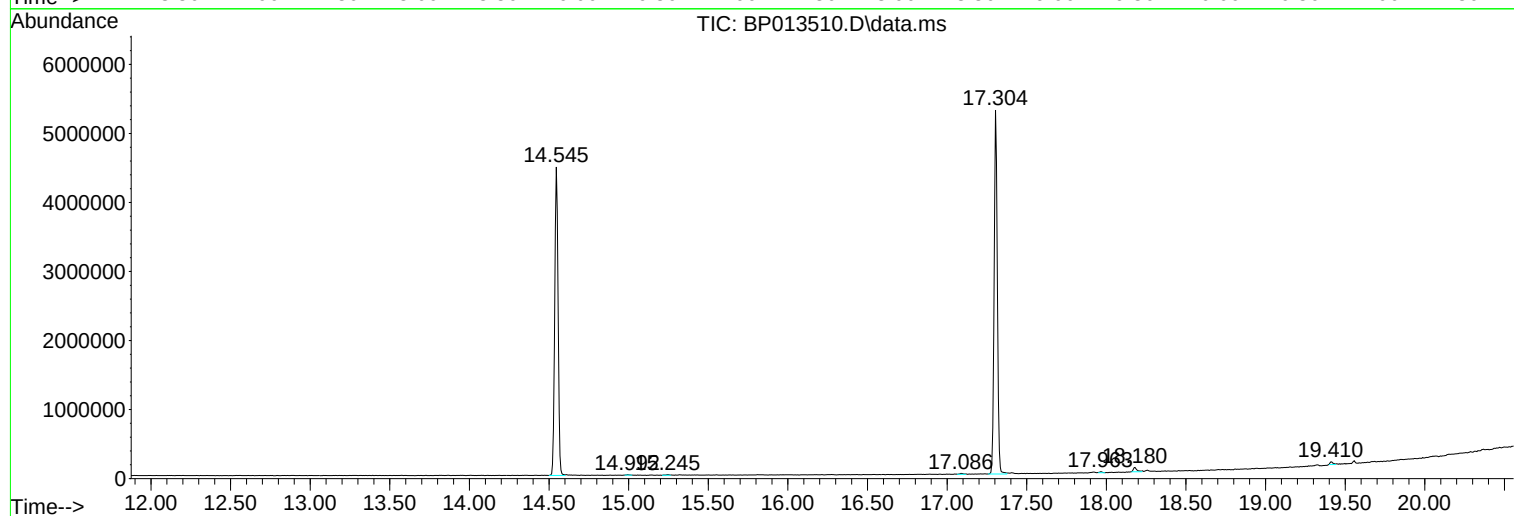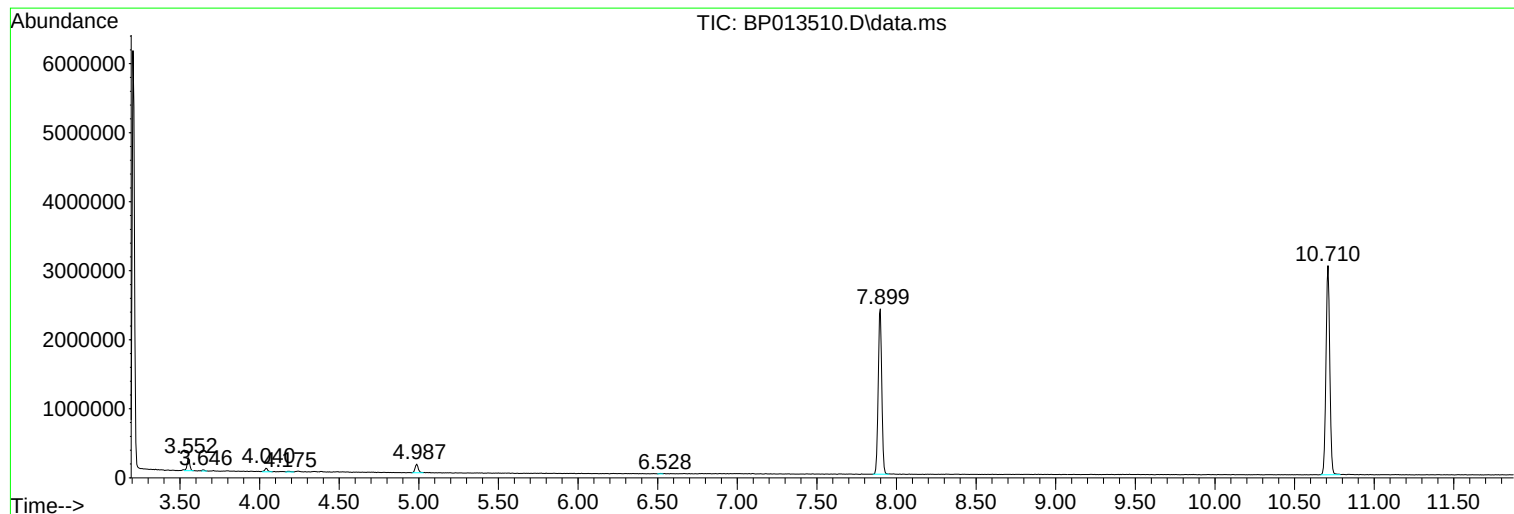

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013510.D
Acq On : 18 Jan 2023 00:14
Operator : CG/JU
Sample : PB150250BL
Misc : GCMS CONFIRMATION
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK250

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013510.D
Acq On : 18 Jan 2023 00:14
Operator : CG/JU
Sample : PB150250BL
Misc : GCMS CONFIRMATION
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK250

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc