

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013518.D
 Acq On : 18 Jan 2023 11:42
 Operator : CG/JU
 Sample : PB150292BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK292

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	14	18	23	rVB	131028	154944	1.72%	0.158%
2	3.723	88	91	109	rBV	1156942	1830622	20.35%	1.868%
3	4.046	142	146	154	rVB	37592	53838	0.60%	0.055%
4	7.064	651	659	672	rBV	1722904	2759012	30.67%	2.816%
5	7.228	680	687	701	rVB	1459373	2217037	24.65%	2.263%
6	7.428	714	721	730	rBV	1808568	2805981	31.19%	2.864%
7	7.899	793	801	809	rBV	1815610	2810276	31.24%	2.868%
8	8.610	915	922	940	rBV	2091388	3289080	36.56%	3.357%
9	9.069	992	1000	1011	rBV	1645347	2663473	29.61%	2.718%
10	9.793	1115	1123	1130	rBV	1373102	2236431	24.86%	2.283%
11	10.328	1207	1214	1225	rBV	1995079	3339102	37.12%	3.408%
12	10.710	1270	1279	1288	rBV	2445522	4045204	44.97%	4.129%
13	10.852	1291	1303	1315	rBV	1499197	2558276	28.44%	2.611%
14	12.299	1543	1549	1554	rBV	36638	56703	0.63%	0.058%
15	12.887	1643	1649	1658	rBV	4150	11538	0.13%	0.012%
16	13.510	1748	1755	1764	rVB	7302	16027	0.18%	0.016%
17	13.957	1823	1831	1842	rBV	3132489	4387670	48.78%	4.478%
18	14.057	1845	1848	1857	rVB10	6206	13740	0.15%	0.014%
19	14.240	1872	1879	1892	rBV	3823327	5492511	61.06%	5.606%
20	14.545	1924	1931	1939	rBV	3569268	5074414	56.41%	5.179%
21	14.751	1958	1966	1985	rBV	1105741	1949281	21.67%	1.989%
22	15.540	2093	2100	2114	rBV	4855504	6597804	73.34%	6.734%
23	15.669	2114	2122	2135	rBV	1432144	2069767	23.01%	2.112%
24	15.781	2137	2141	2147	rVB3	22746	36396	0.40%	0.037%
25	16.328	2231	2234	2239	rVB7	7068	11539	0.13%	0.012%
26	16.981	2339	2345	2346	rBV6	11749	16164	0.18%	0.016%
27	17.092	2360	2364	2369	rBV6	10404	18133	0.20%	0.019%
28	17.304	2393	2400	2408	rBV	3878333	5520109	61.36%	5.634%
29	17.404	2411	2417	2429	rVV2	4764640	6775545	75.32%	6.915%
30	18.175	2544	2548	2555	rBV8	32642	63663	0.71%	0.065%
31	19.216	2722	2725	2731	rVB3	58792	78874	0.88%	0.081%
32	19.286	2733	2737	2742	rBV	58298	82253	0.91%	0.084%
33	19.639	2792	2797	2807	rBV	5942183	7709078	85.70%	7.868%
34	21.398	3091	3096	3104	rBV	4234937	5591739	62.16%	5.707%
35	23.692	3479	3486	3499	rVB2	4501246	8995657	100.00%	9.181%
36	23.851	3507	3513	3522	rVB2	3373688	6647278	73.89%	6.784%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013518.D
Acq On : 18 Jan 2023 11:42
Operator : CG/JU
Sample : PB150292BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK292

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Title : SVOA CALIBRATION




Sum of corrected areas: 97979159

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013518.D
Acq On : 18 Jan 2023 11:42
Operator : CG/JU
Sample : PB150292BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK292

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

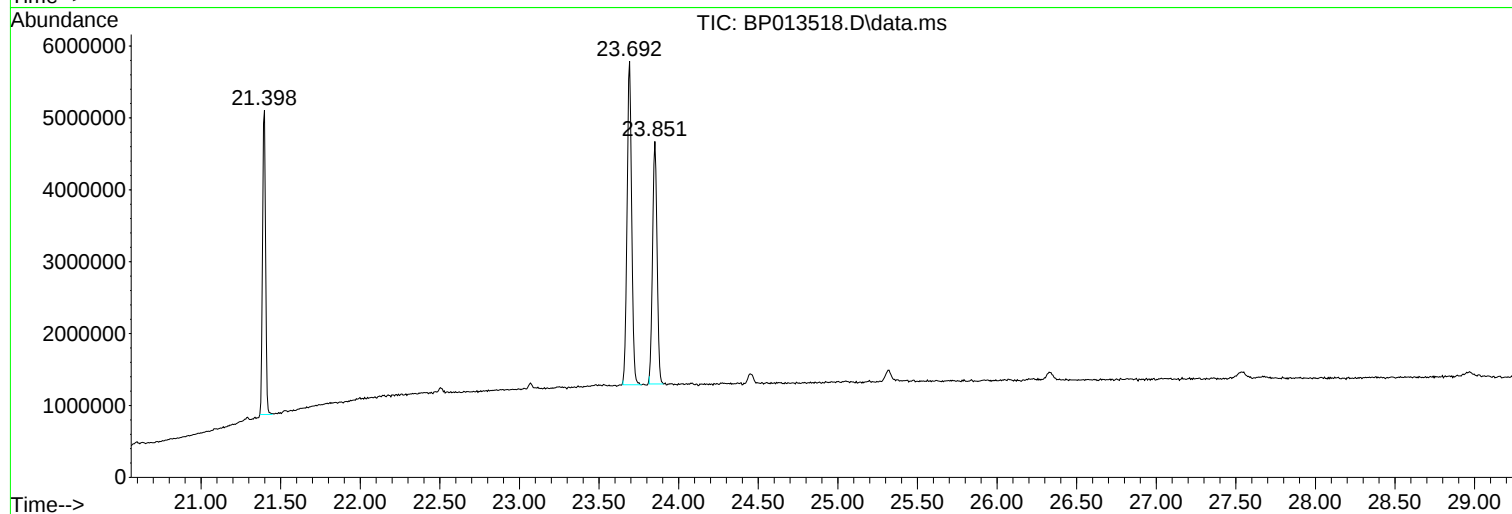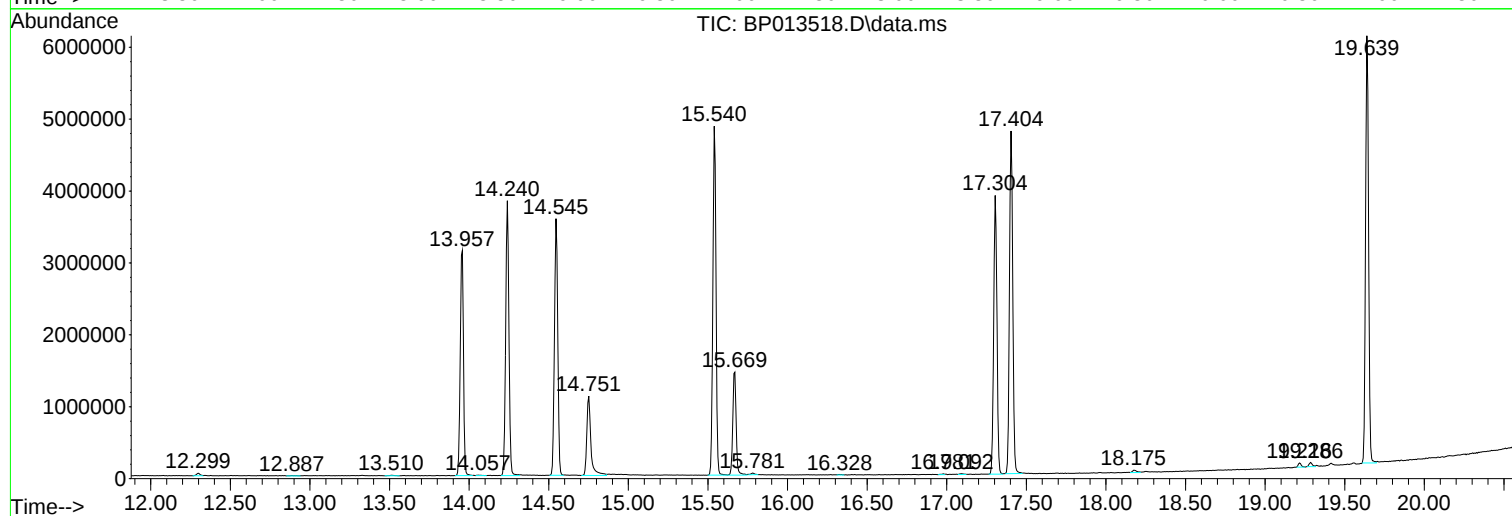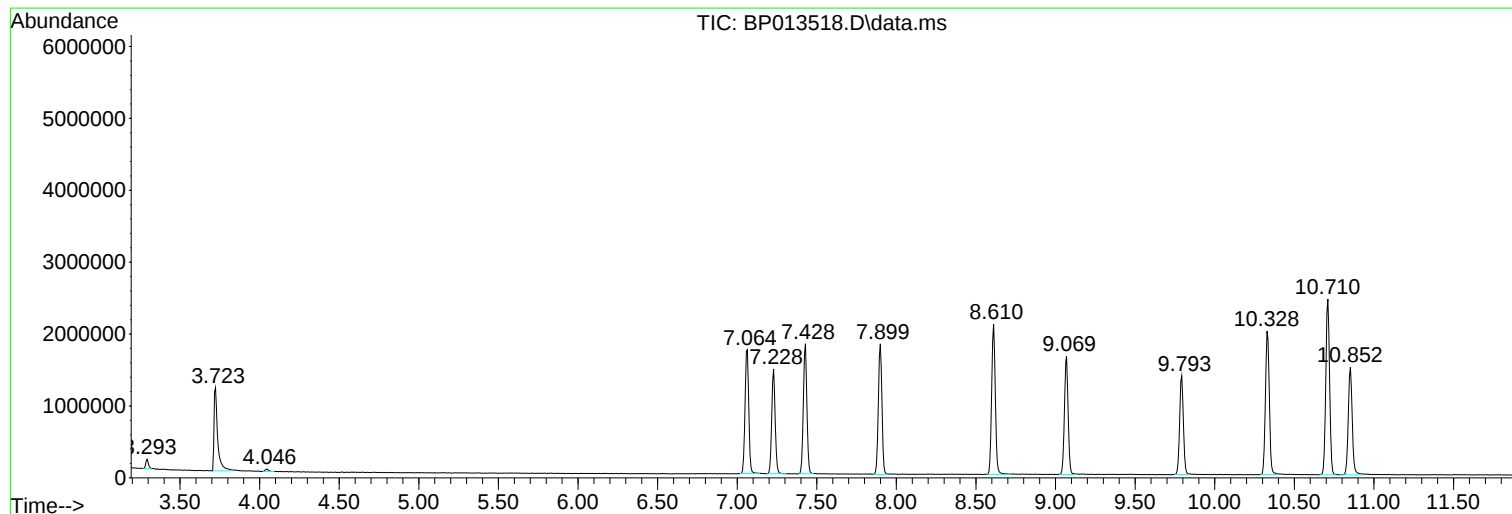

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013518.D
Acq On : 18 Jan 2023 11:42
Operator : CG/JU
Sample : PB150292BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK292

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013518.D
Acq On : 18 Jan 2023 11:42
Operator : CG/JU
Sample : PB150292BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK292

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc