

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013519.D
 Acq On : 18 Jan 2023 12:16
 Operator : CG/JU
 Sample : PB150266BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK266

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	15	18	31	rVB	143489	204589	1.82%	0.195%
2	3.722	87	91	109	rBV	1643508	2548379	22.70%	2.423%
3	4.046	143	146	151	rVB	34313	43700	0.39%	0.042%
4	7.058	651	658	669	rBV	1812538	2886794	25.72%	2.745%
5	7.228	680	687	696	rVB	1497869	2270587	20.23%	2.159%
6	7.428	714	721	731	rBV	1877338	2953247	26.31%	2.808%
7	7.899	794	801	808	rBV	1699053	2625171	23.39%	2.496%
8	8.610	915	922	937	rBV	2124603	3394285	30.24%	3.228%
9	9.069	993	1000	1010	rBV	1690767	2718085	24.21%	2.585%
10	9.793	1115	1123	1135	rBV	1383045	2292418	20.42%	2.180%
11	10.328	1206	1214	1229	rBV	2106760	3451848	30.75%	3.283%
12	10.710	1271	1279	1287	rBV	2221993	3700090	32.96%	3.519%
13	10.851	1296	1303	1316	rBV	1958967	3358071	29.92%	3.193%
14	12.298	1541	1549	1554	rBV2	31126	55911	0.50%	0.053%
15	13.951	1823	1830	1842	rBV	3323300	4471652	39.84%	4.252%
16	14.239	1871	1879	1896	rBV	3884918	5547305	49.42%	5.275%
17	14.545	1923	1931	1942	rBV	3268477	4650411	41.43%	4.422%
18	14.751	1959	1966	1990	rBV	1153297	2093710	18.65%	1.991%
19	15.539	2093	2100	2113	rBV	4807771	6808845	60.66%	6.475%
20	15.663	2115	2121	2137	rVV	1603657	2190512	19.51%	2.083%
21	15.781	2137	2141	2146	rVB3	26469	39221	0.35%	0.037%
22	16.328	2231	2234	2239	rVB6	9438	12838	0.11%	0.012%
23	17.086	2360	2363	2368	rBV4	9676	15109	0.13%	0.014%
24	17.304	2393	2400	2408	rBV	3873092	5322978	47.42%	5.062%
25	17.404	2410	2417	2431	rVV	5367315	7335449	65.35%	6.976%
26	18.175	2545	2548	2553	rBV5	30326	45145	0.40%	0.043%
27	19.216	2722	2725	2731	rVB2	71452	87803	0.78%	0.083%
28	19.286	2733	2737	2741	rVV	58982	85611	0.76%	0.081%
29	19.410	2755	2758	2763	rBV6	34833	55551	0.49%	0.053%
30	19.639	2791	2797	2803	rBV	7288018	9037687	80.51%	8.594%
31	21.392	3090	3095	3101	rBV	5096533	6320560	56.31%	6.011%
32	23.686	3478	3485	3499	rVB2	5725999	11225134	100.00%	10.675%
33	23.845	3506	3512	3521	rVB2	3721129	7309701	65.12%	6.951%




Sum of corrected areas: 105158397

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013519.D
Acq On : 18 Jan 2023 12:16
Operator : CG/JU
Sample : PB150266BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK266

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

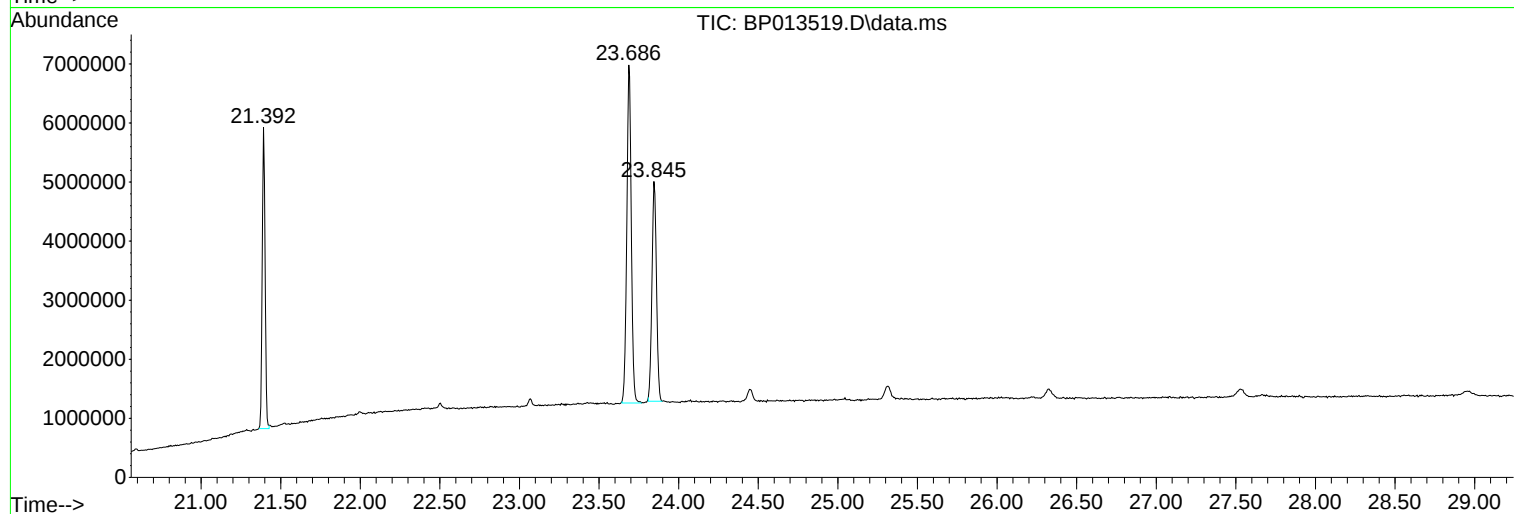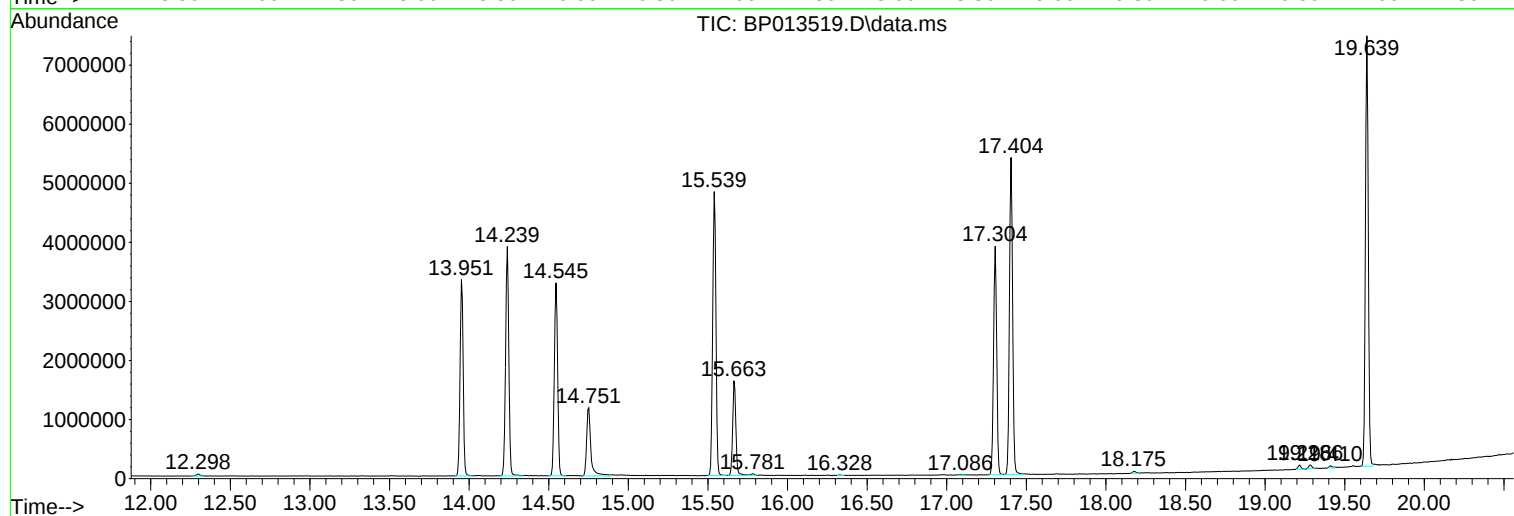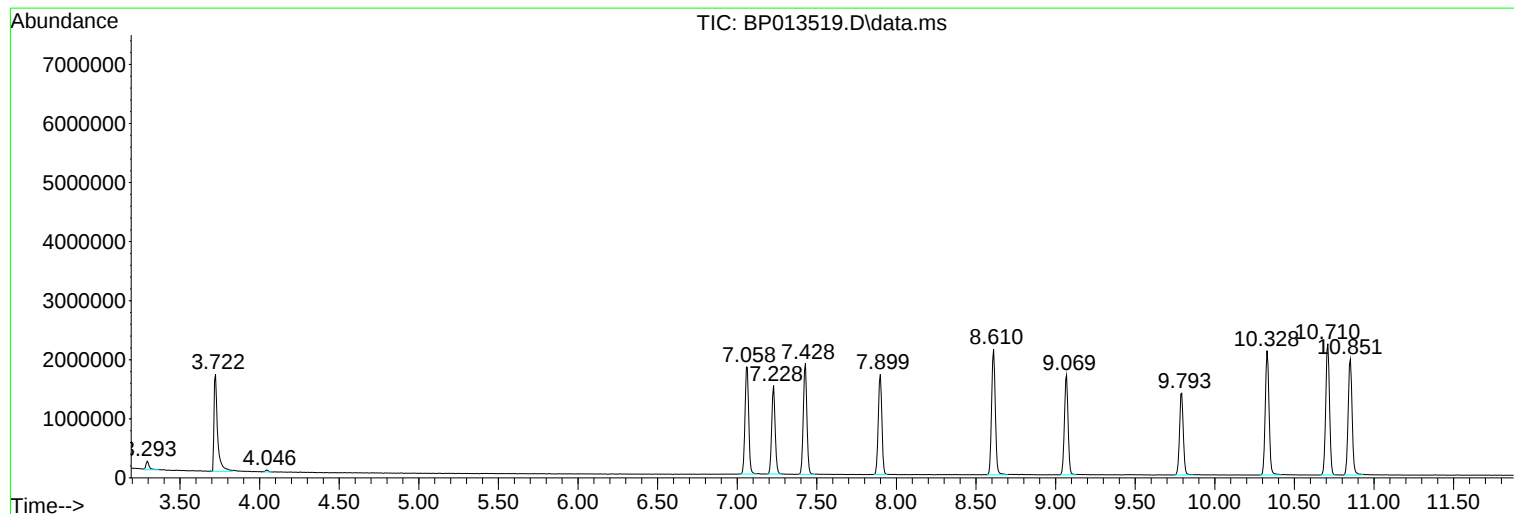

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013519.D
Acq On : 18 Jan 2023 12:16
Operator : CG/JU
Sample : PB150266BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK266

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013519.D
Acq On : 18 Jan 2023 12:16
Operator : CG/JU
Sample : PB150266BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK266

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc