

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
 Data File : BP013528.D
 Acq On : 18 Jan 2023 18:47
 Operator : CG/JU
 Sample : PB150297BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK297

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	14	18	26	rVB	156954	205051	2.12%	0.182%
2	3.716	87	90	108	rBV	1413665	2243047	23.21%	1.990%
3	4.046	142	146	149	rVB	34208	40337	0.42%	0.036%
4	7.057	651	658	674	rBV	2142896	3398874	35.16%	3.015%
5	7.228	680	687	698	rVB	1780867	2713416	28.07%	2.407%
6	7.428	714	721	733	rVB	2169337	3438482	35.57%	3.050%
7	7.899	794	801	808	rBV	1802652	2764576	28.60%	2.453%
8	8.610	911	922	934	rBV	2666535	4155237	42.99%	3.686%
9	9.069	992	1000	1012	rBV	2065093	3359584	34.76%	2.980%
10	9.793	1112	1123	1134	rBV	1735315	2872951	29.72%	2.549%
11	10.328	1206	1214	1226	rBV	2579423	4256173	44.03%	3.776%
12	10.710	1271	1279	1287	rVB	2358280	3909178	40.44%	3.468%
13	10.851	1294	1303	1323	rBV	1853096	3301685	34.16%	2.929%
14	12.298	1542	1549	1559	rBV2	43932	78908	0.82%	0.070%
15	13.516	1753	1756	1759	rVB5	9119	11597	0.12%	0.010%
16	13.951	1824	1830	1842	rVV	4377579	5899281	61.03%	5.234%
17	14.063	1846	1849	1853	rVB6	7686	10250	0.11%	0.009%
18	14.239	1872	1879	1890	rBV	5094456	7230299	74.81%	6.414%
19	14.545	1924	1931	1939	rBV	3610768	5028065	52.02%	4.461%
20	14.645	1945	1948	1955	rVB9	6285	10425	0.11%	0.009%
21	14.745	1958	1965	1983	rBV	1629164	2634336	27.26%	2.337%
22	14.904	1990	1992	1996	rVB5	9026	10570	0.11%	0.009%
23	14.951	1996	2000	2005	rVB8	10708	16202	0.17%	0.014%
24	15.539	2093	2100	2109	rBV	6214094	8716155	90.18%	7.733%
25	15.663	2115	2121	2135	rBV	2077372	2724979	28.19%	2.417%
26	15.781	2137	2141	2147	rVB2	31296	49053	0.51%	0.044%
27	16.969	2341	2343	2350	rVB8	8274	14968	0.15%	0.013%
28	17.304	2393	2400	2410	rBV	3807381	5355462	55.41%	4.751%
29	17.404	2410	2417	2431	rBV	6177081	8758237	90.61%	7.770%
30	17.963	2508	2512	2517	rVB7	19242	24966	0.26%	0.022%
31	18.175	2545	2548	2554	rBV7	21442	28494	0.29%	0.025%
32	19.210	2721	2724	2729	rVB2	72069	97309	1.01%	0.086%
33	19.280	2733	2736	2742	rVV	69291	94647	0.98%	0.084%
34	19.639	2791	2797	2806	rBV	7250994	9245210	95.65%	8.202%
35	21.392	3090	3095	3101	rBV	3830974	4815889	49.83%	4.272%
36	23.680	3478	3484	3494	rVB2	4826042	9665513	100.00%	8.575%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013528.D
Acq On : 18 Jan 2023 18:47
Operator : CG/JU
Sample : PB150297BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK297

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Title : SVOA CALIBRATION

37 23.845 3505 3512 3520 rVB2 2763010 5539876 57.32% 4.915%




Sum of corrected areas: 112719282

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013528.D
Acq On : 18 Jan 2023 18:47
Operator : CG/JU
Sample : PB150297BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK297

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

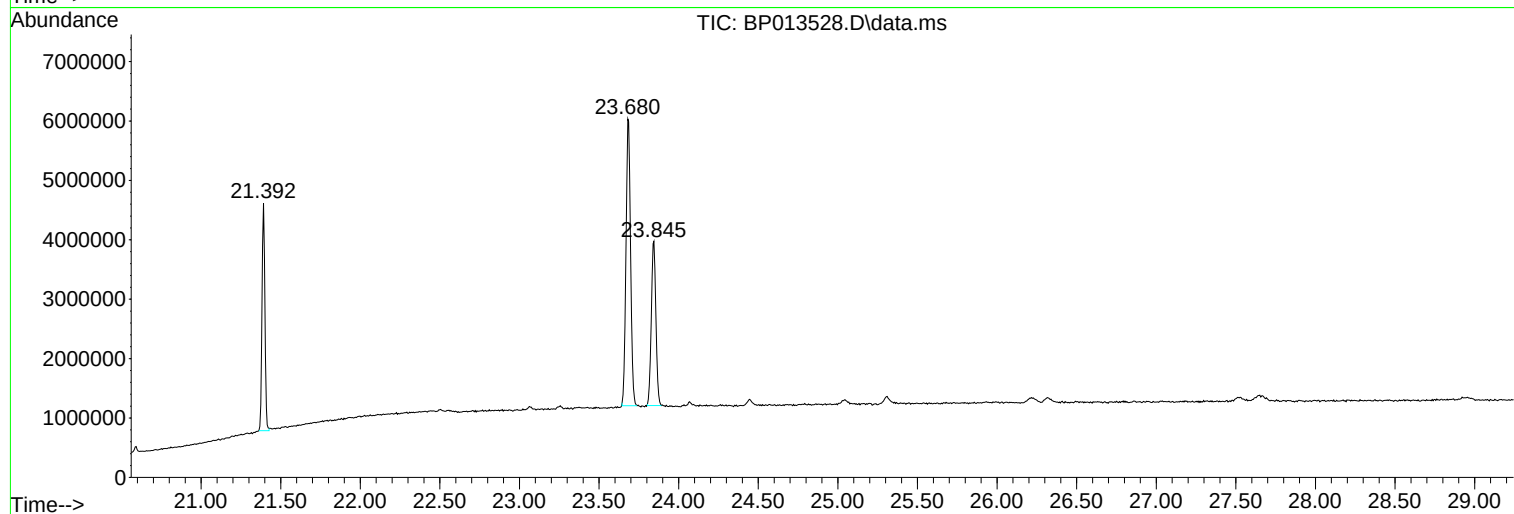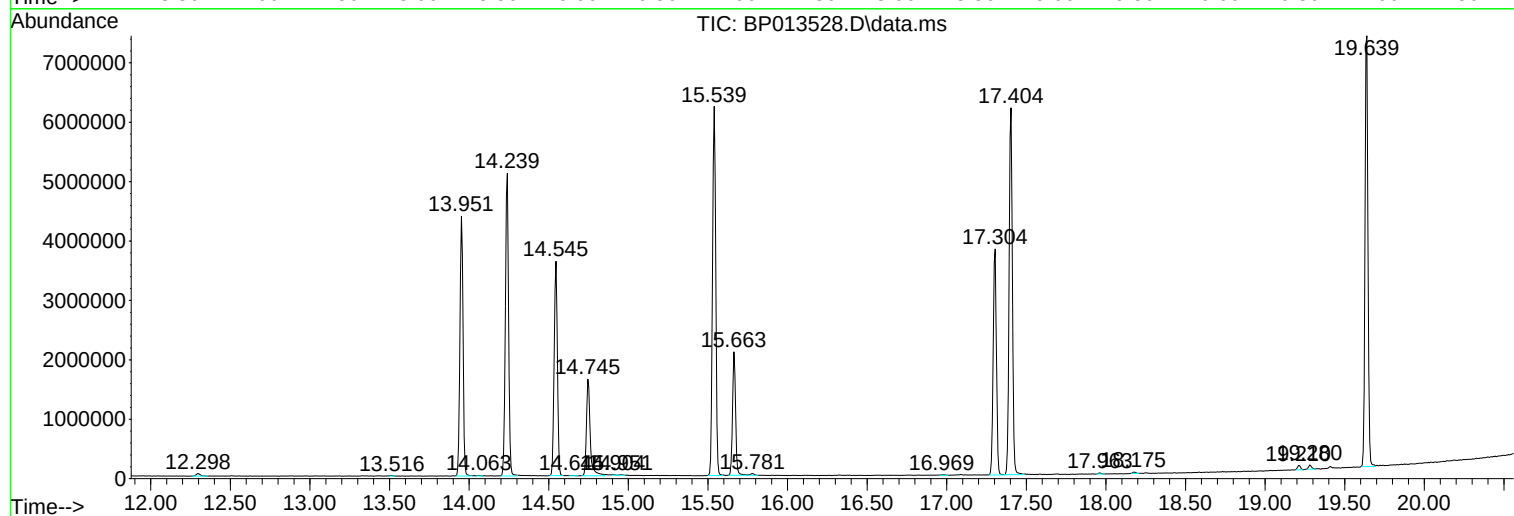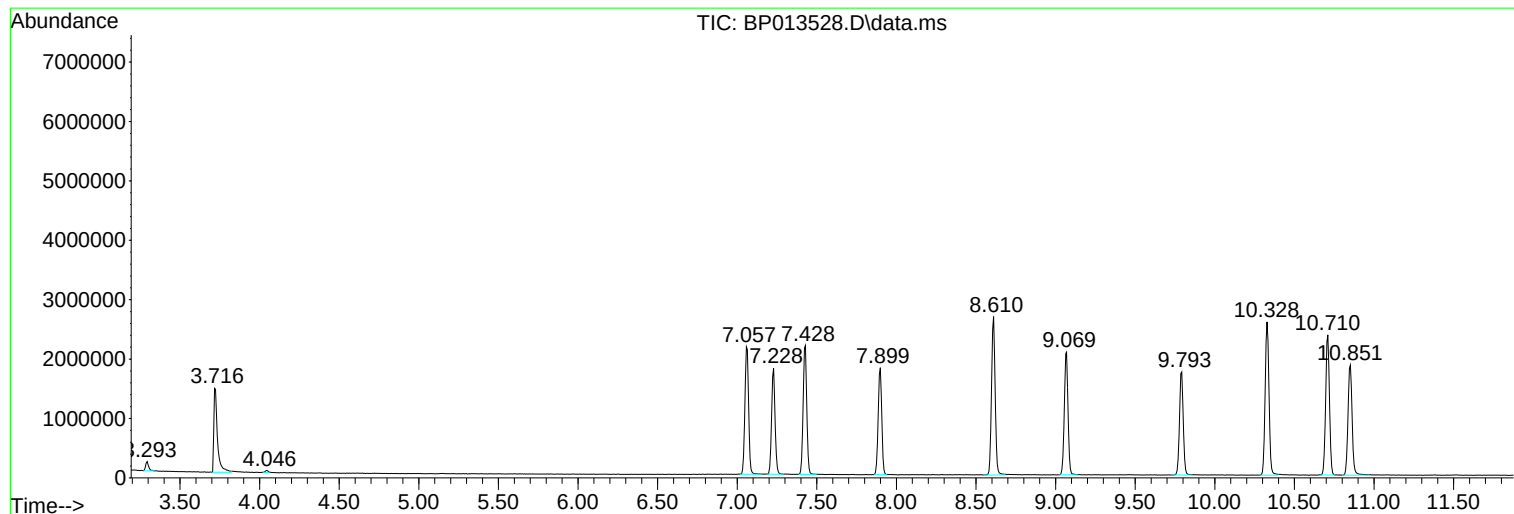

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013528.D
Acq On : 18 Jan 2023 18:47
Operator : CG/JU
Sample : PB150297BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK297

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP011823\
Data File : BP013528.D
Acq On : 18 Jan 2023 18:47
Operator : CG/JU
Sample : PB150297BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK297

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc