


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012022\
 Data File : BP008866.D
 Acq On : 20 Jan 2022 10:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 14 18:05:00 2022

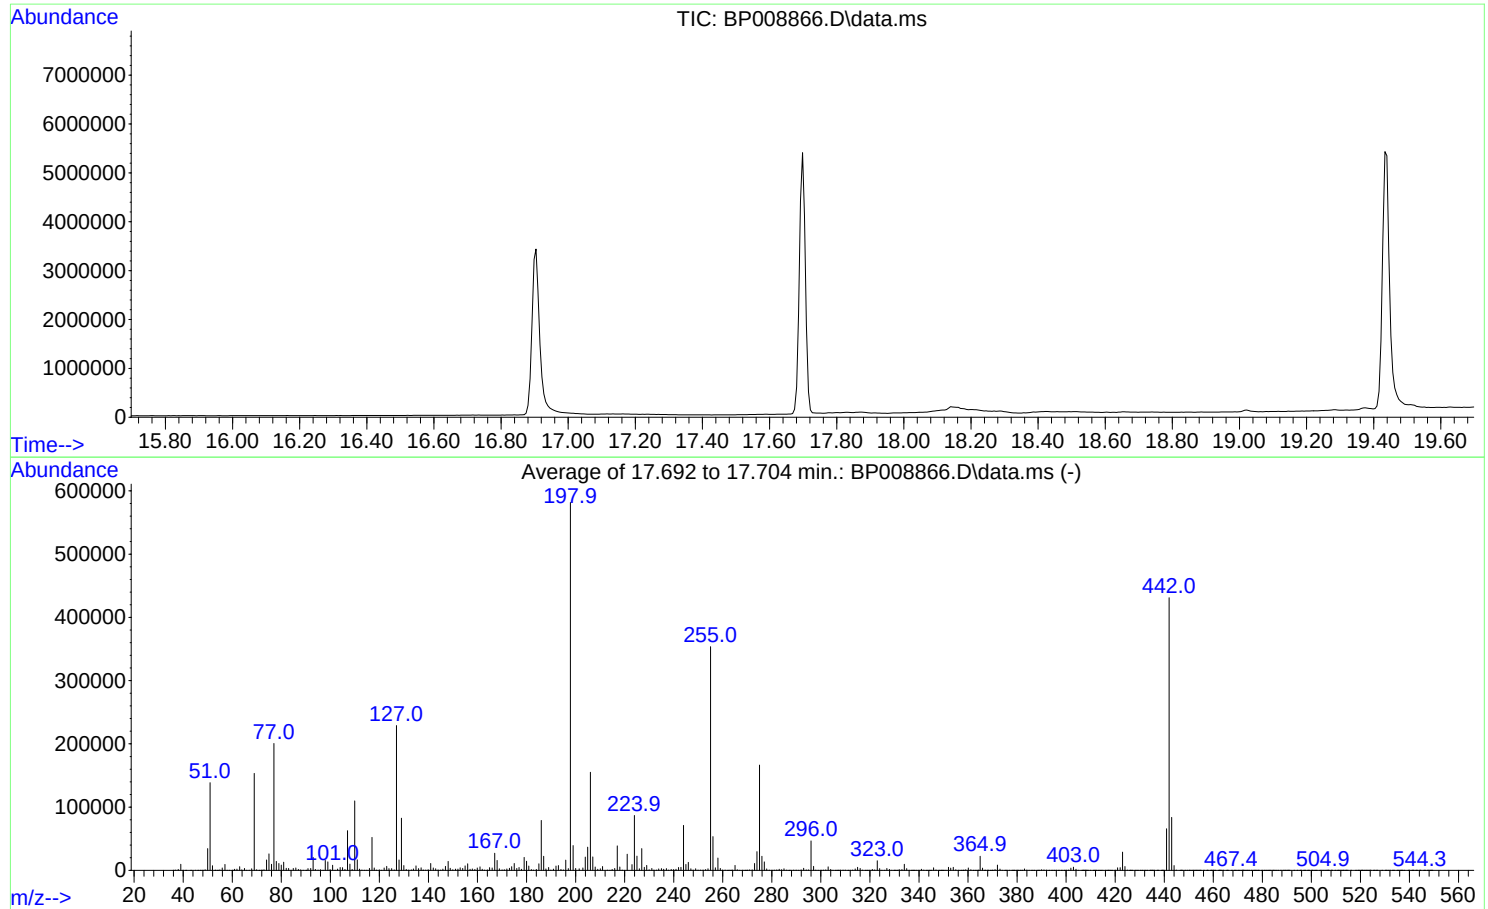




AutoFind: Scans 2500, 2501, 2502; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.8	138536	PASS
68	69	0.00	2	1.7	2541	PASS
69	198	0.00	100	26.4	153269	PASS
70	69	0.00	2	0.6	910	PASS
127	198	10	80	39.4	228961	PASS
197	198	0.00	2	0.5	2774	PASS
198	198	100	100	100.0	581612	PASS
199	198	5	9	6.8	39301	PASS
275	198	10	60	28.6	166375	PASS
365	198	1	100	3.8	22296	PASS
441	198	0.01	100	11.3	65802	PASS
442	442	100	100	100.0	431125	PASS
443	442	15	24	19.4	83733	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012022\
 Data File : BP008866.D
 Acq On : 20 Jan 2022 10:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 21 06:02:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 14 18:05:00 2022
 Response via : Initial Calibration

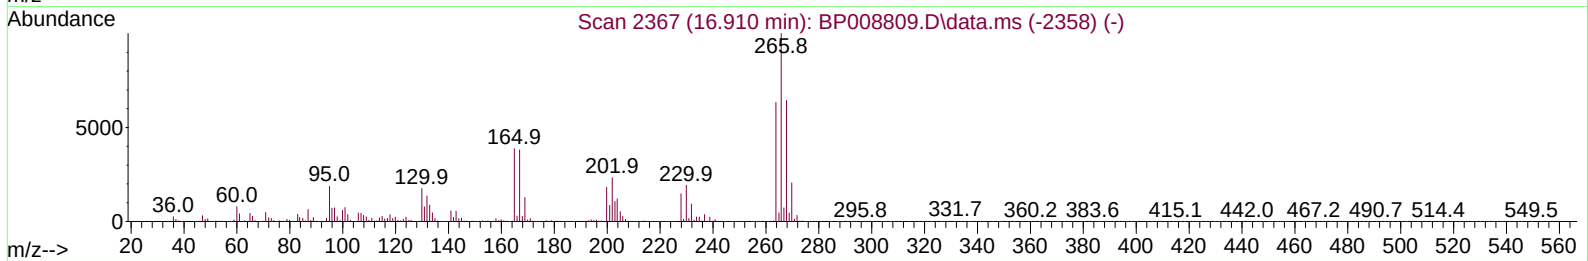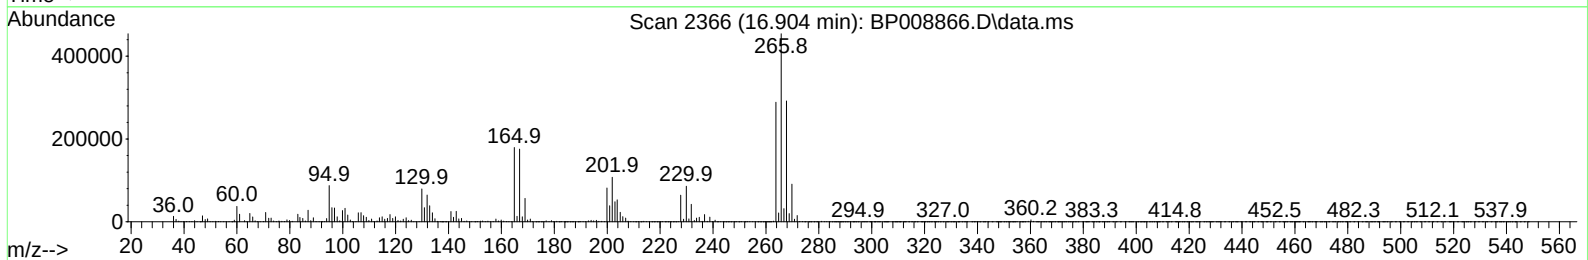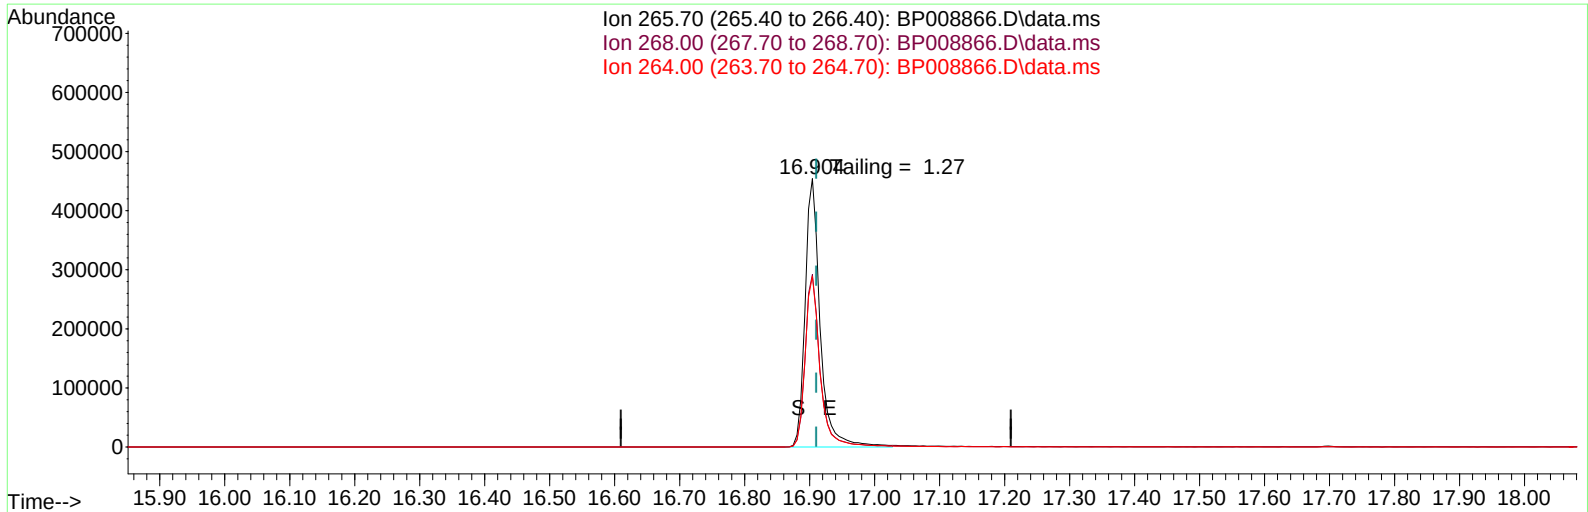

TIC: BP008866.D\data.ms

(70) Pentachlorophenol (C)

16.904min (-0.006) 1539773.99 ng




response 739365

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.27
264.00	62.90	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012022\
 Data File : BP008866.D
 Acq On : 20 Jan 2022 10:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 21 06:02:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP011422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 14 18:05:00 2022
 Response via : Initial Calibration

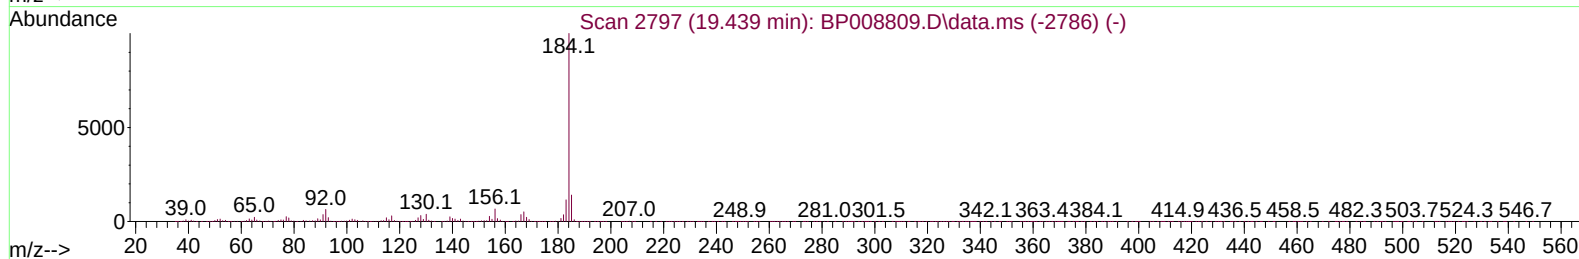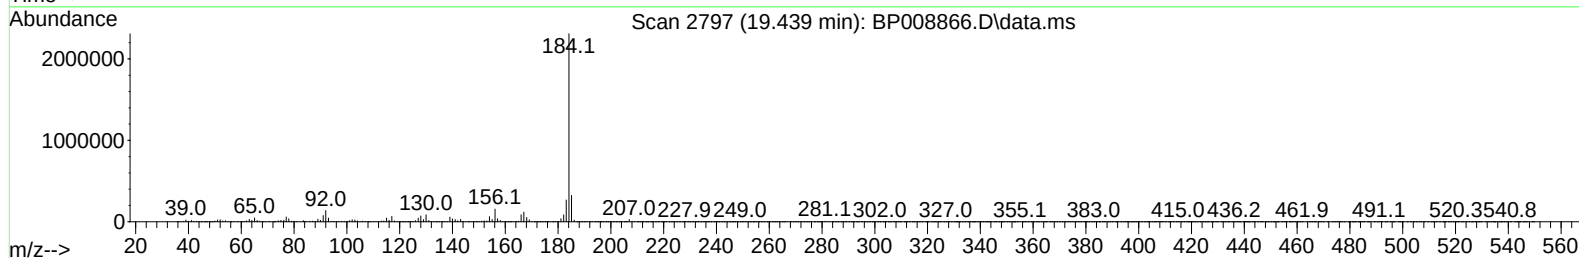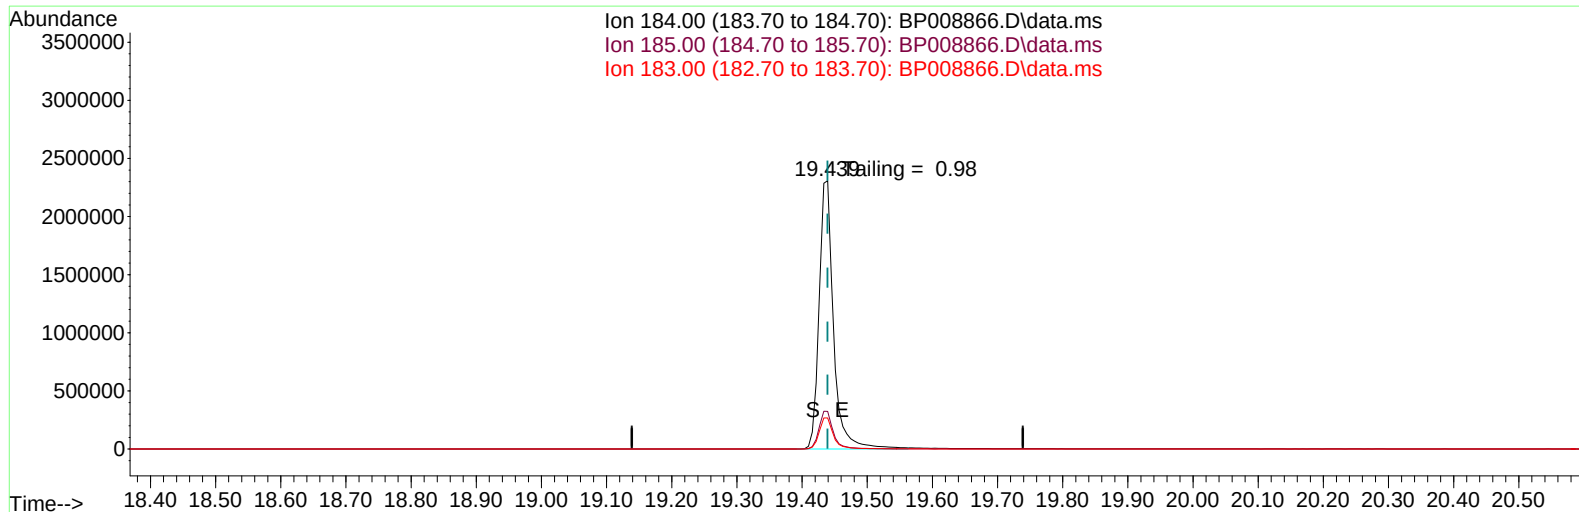

TIC: BP008866.D\data.ms

(77) Benzidine

19.439min (+ 0.000) 696260.33 ng

response 3566614

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.02
183.00	11.90	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/20/2022	BNA_P	<u>BP008866.D</u>
Compound Name	Response	Retention Time
DDT	1956345	20.645
DDD	64177	20.21
DDE	4776	19.716
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
68953	2025298	3.40

Instrument :
BNA_P
ClientSampleId :
DFTPP