

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
 Data File : BP023665.D
 Acq On : 20 Jan 2025 22:37
 Operator : RC/JU
 Sample : Q1086-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE5

Quant Time: Jan 20 23:06:41 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 20 21:50:54 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	775273	20.000	ng/u1	0.00
20) Naphthalene-d8	10.587	136	3249962	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.428	164	2051080	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.222	188	4043565	20.000	ng/u1	0.00
79) Chrysene-d12	21.657	240	4150958	20.000	ng/u1	0.00
88) Perylene-d12	25.045	264	4442264	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	94110	4.476	ng/uL	0.00
4) Pyridine-d5	3.722	84	384780	6.564	ng/u1	0.00
7) Phenol-d5	6.963	99	669262	10.027	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	1376239	35.198	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	1816521	34.462	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	1269375	24.519	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	944017	38.056	ng/u1	0.00
24) 2-Nitrophenol-d4	9.669	143	888586	54.574	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.199	165	1959687	39.569	ng/u1	0.00
31) 4-Chloroaniline-d4	10.710	131	2021512	25.568	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	5739900	35.958	ng/u1	0.00
49) Acenaphthylene-d8	14.122	160	6698864	35.277	ng/u1	0.00
54) 4-Nitrophenol-d4	14.604	143	243056	9.160	ng/u1	0.00
60) Fluorene-d10	15.439	176	5108872	36.981	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.539	200	586553	44.582	ng/u1	0.00
73) Anthracene-d10	17.322	188	8140384	37.294	ng/u1	0.00
81) Pyrene-d10	19.692	212	9487011	41.255	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.815	264	9547490	39.548	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.352	88	160809	7.227	ng/uL	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023665.D
Acq On : 20 Jan 2025 22:37
Operator : RC/JU
Sample : Q1086-20
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE5

Quant Time: Jan 20 23:06:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 21:50:54 2025
Response via : Initial Calibration

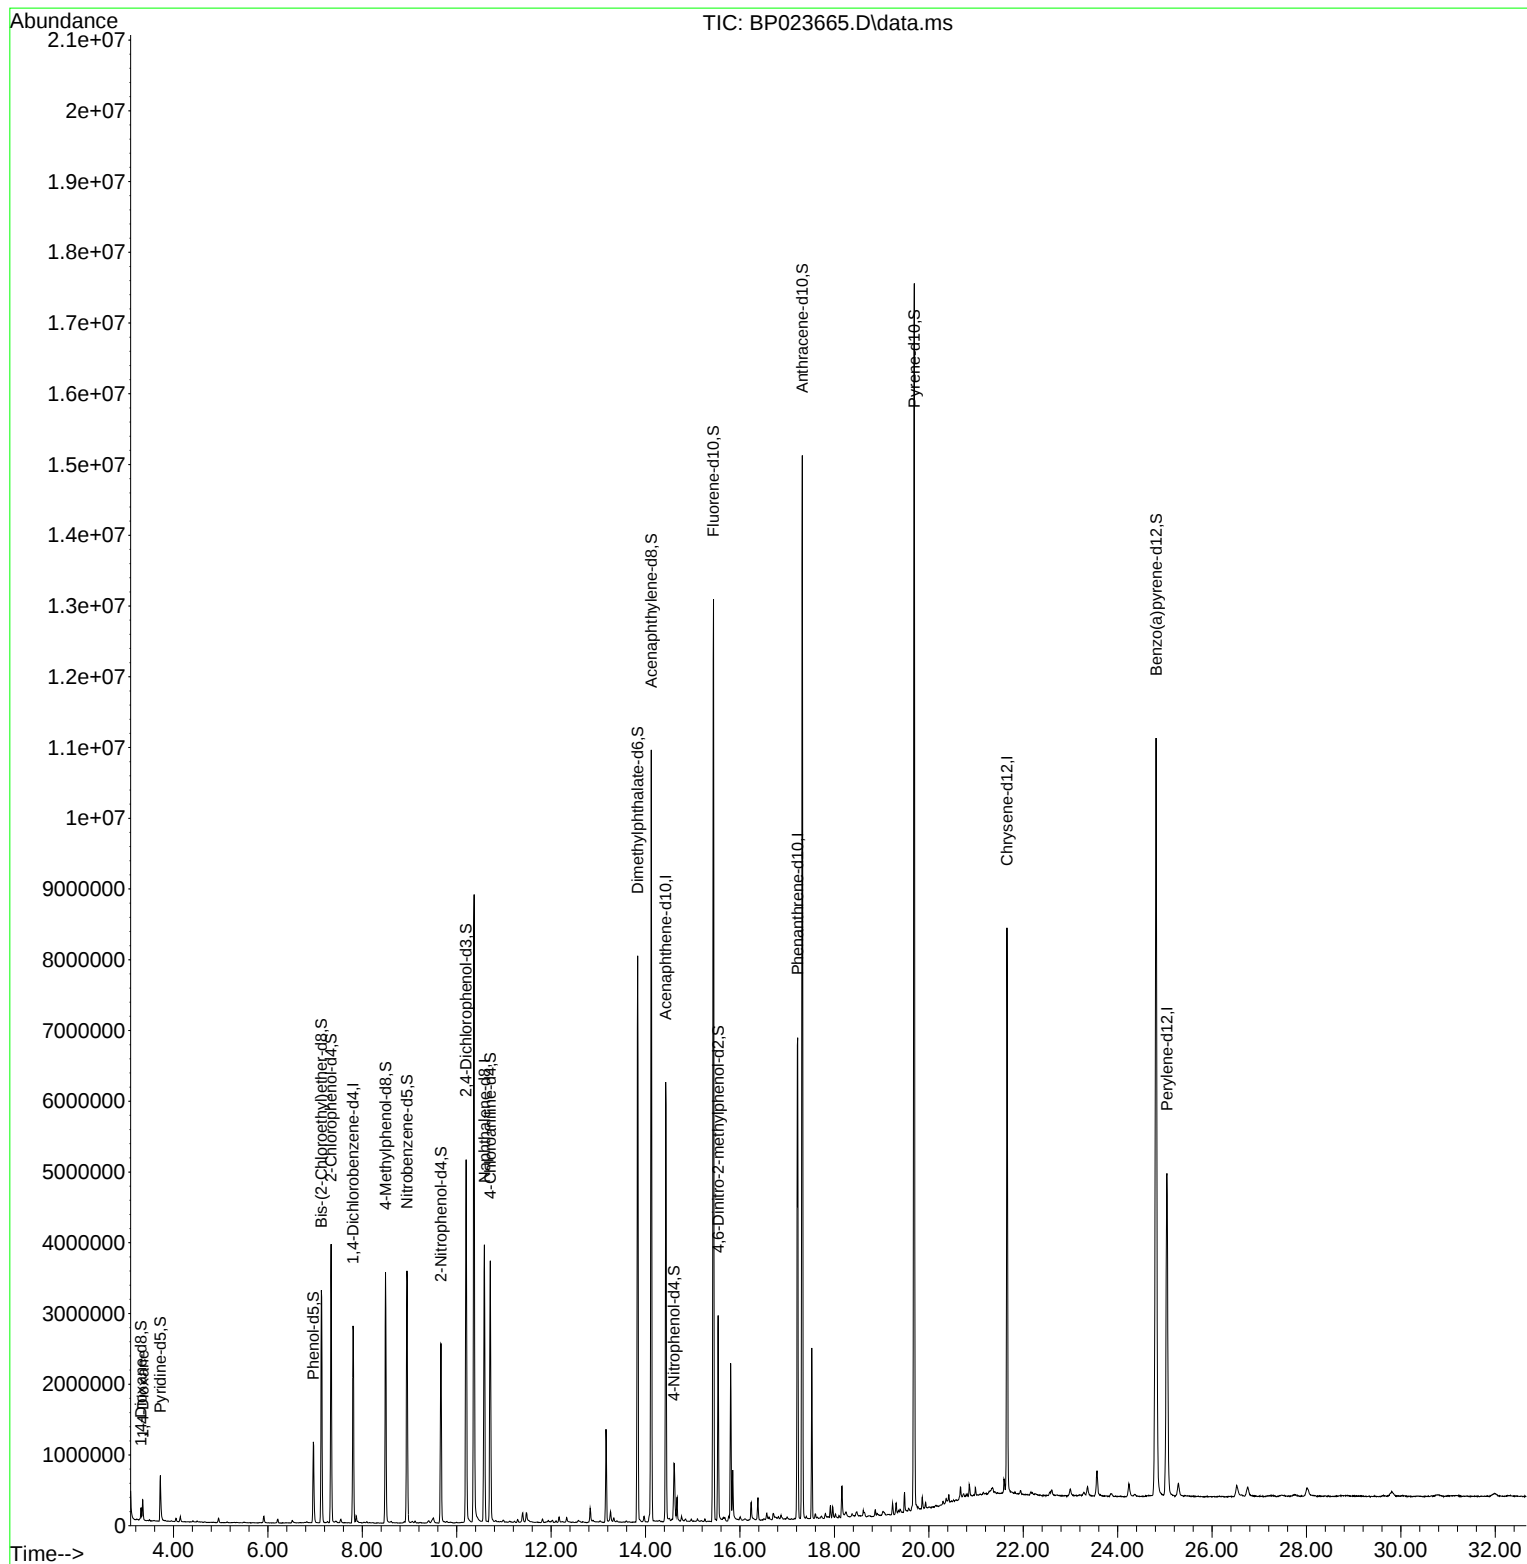

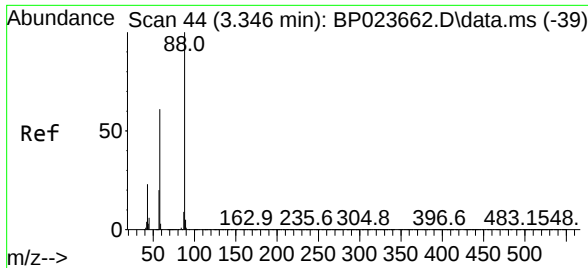

#2
 1,4-Dioxane
 Concen: 7.227 ng/uL
 RT: 3.352 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: BP023665.D
 Acq: 20 Jan 2025 22:37

Instrument :
 BNA_P
 ClientSampleId :
 C0AE5

Tgt Ion: 88 Resp: 160809

Ion	Ratio	Lower	Upper
88	100		
43	22.1	17.3	25.9
58	59.3	47.4	71.0

