

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
 Data File : BP023670.D
 Acq On : 21 Jan 2025 01:58
 Operator : RC/JU
 Sample : Q1126-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF3

Quant Time: Jan 21 02:26:47 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 20 21:50:54 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.811	152	723342	20.000	ng/u1	0.00
20) Naphthalene-d8	10.581	136	2935654	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.422	164	1753725	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.210	188	3367786	20.000	ng/u1	-0.02
79) Chrysene-d12	21.657	240	3332364	20.000	ng/u1	0.00
88) Perylene-d12	25.045	264	3504269	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.317	96	85344	4.350	ng/uL	0.00
4) Pyridine-d5	3.728	84	307976	5.631	ng/u1	0.01
7) Phenol-d5	6.969	99	445807	7.159	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.140	67	947984	25.986	ng/u1	0.00
11) 2-Chlorophenol-d4	7.340	132	1223570	24.879	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	825170	17.083	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	613786	27.393	ng/u1	0.00
24) 2-Nitrophenol-d4	9.663	143	549900	37.389	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.199	165	1225476	27.394	ng/u1	0.00
31) 4-Chloroaniline-d4	10.710	131	427513	5.986	ng/u1	0.00
46) Dimethylphthalate-d6	13.828	166	3598937	26.369	ng/u1	0.00
49) Acenaphthylene-d8	14.116	160	4242440	26.129	ng/u1	0.00
54) 4-Nitrophenol-d4	14.598	143	127907	5.638	ng/u1	0.00
60) Fluorene-d10	15.428	176	3194006	27.040	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.534	200	284471	25.960	ng/u1	-0.01
73) Anthracene-d10	17.310	188	4860529	26.736	ng/u1	-0.02
81) Pyrene-d10	19.681	212	5525427	29.930	ng/u1	-0.02
92) Benzo(a)pyrene-d12	24.804	264	5214843	27.383	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.352	88	34991	1.685	ng/uL#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023670.D
Acq On : 21 Jan 2025 01:58
Operator : RC/JU
Sample : Q1126-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF3

Quant Time: Jan 21 02:26:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 21:50:54 2025
Response via : Initial Calibration

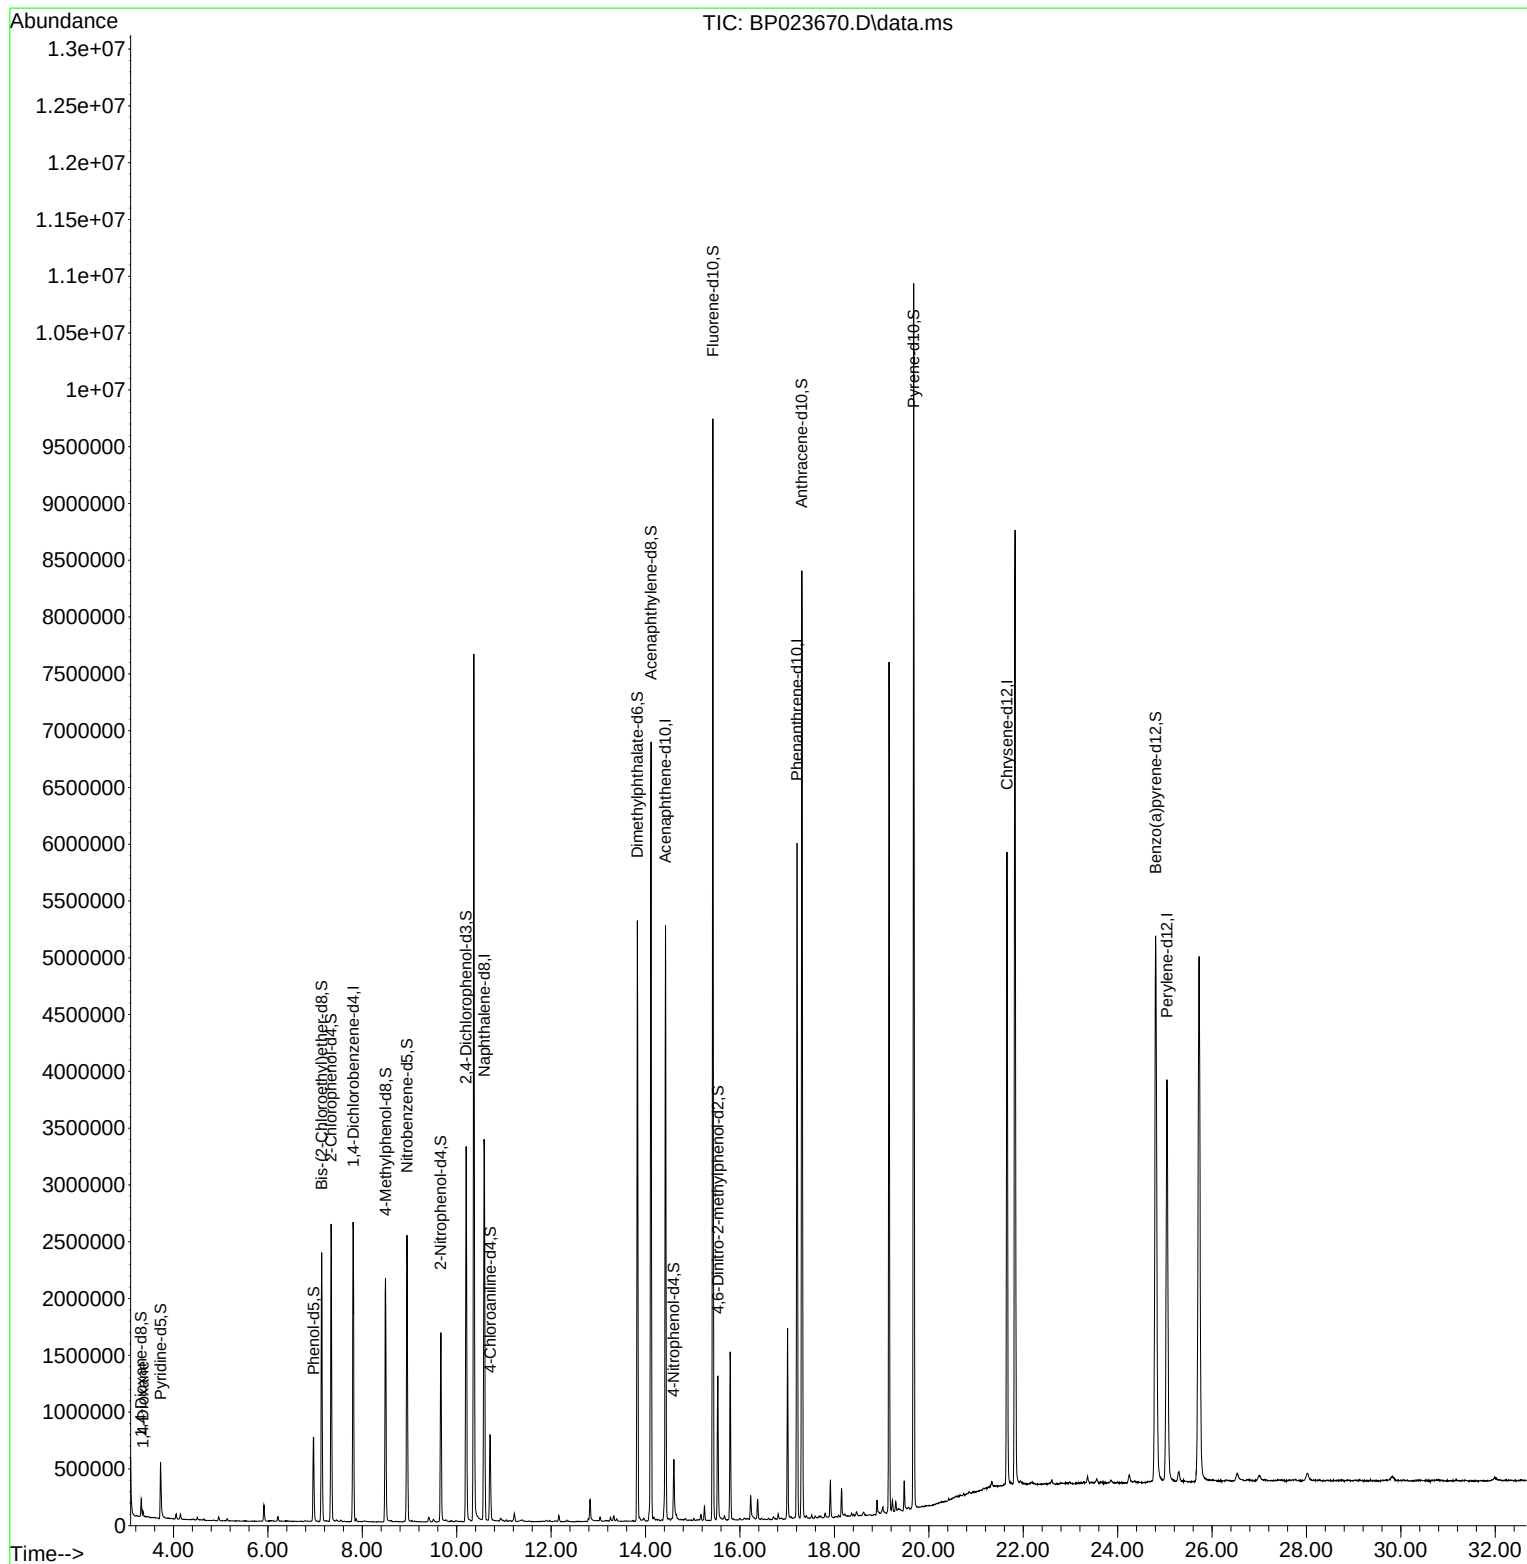

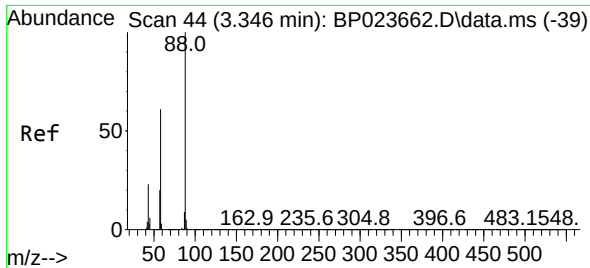

#2
1,4-Dioxane
Concen: 1.685 ng/uL
RT: 3.352 min Scan# 41
Delta R.T. 0.006 min
Lab File: BP023670.D
Acq: 21 Jan 2025 01:58

Instrument :
BNA_P
ClientSampleId :
C0AF3

Tgt Ion: 88 Resp: 34991
Ion Ratio Lower Upper
88 100
43 26.0 17.3 25.9#
58 62.8 47.4 71.0

