

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
 Data File : BP023679.D
 Acq On : 21 Jan 2025 12:06
 Operator : RC/JU
 Sample : Q1108-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YE8F7

Quant Time: Jan 21 22:00:29 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 20 21:50:54 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.805	152	497955	20.000	ng/ul	0.00
20) Naphthalene-d8	10.581	136	1966521	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.428	164	1157367	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.216	188	2266159	20.000	ng/ul	-0.01
79) Chrysene-d12	21.651	240	2290328	20.000	ng/ul	-0.01
88) Perylene-d12	25.039	264	2495673	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	64221	4.755	ng/uL	0.00
4) Pyridine-d5	3.717	84	492010	13.068	ng/ul	0.00
7) Phenol-d5	6.964	99	1110440	25.902	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	678214	27.005	ng/ul	0.00
11) 2-Chlorophenol-d4	7.340	132	899627	26.572	ng/ul	0.00
15) 4-Methylphenol-d8	8.493	113	730234	21.960	ng/ul	0.00
21) Nitrobenzene-d5	8.946	128	428711	28.562	ng/ul	0.00
24) 2-Nitrophenol-d4	9.663	143	359025	36.441	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	763298	25.471	ng/ul	0.00
31) 4-Chloroaniline-d4	10.705	131	1134227	23.708	ng/ul	0.00
46) Dimethylphthalate-d6	13.828	166	2394108	26.580	ng/ul	0.00
49) Acenaphthylene-d8	14.110	160	2953361	27.562	ng/ul	0.00
54) 4-Nitrophenol-d4	14.604	143	305526	20.407	ng/ul	0.00
60) Fluorene-d10	15.428	176	2159067	27.697	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.534	200	124024	16.820	ng/ul	-0.01
73) Anthracene-d10	17.316	188	3409023	27.867	ng/ul	-0.01
81) Pyrene-d10	19.675	212	3897085	30.714	ng/ul	-0.02
92) Benzo(a)pyrene-d12	24.804	264	3722446	27.446	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.993	94	56685	1.240	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023679.D
Acq On : 21 Jan 2025 12:06
Operator : RC/JU
Sample : Q1108-02
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE8F7

Quant Time: Jan 21 22:00:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 20 21:50:54 2025
Response via : Initial Calibration

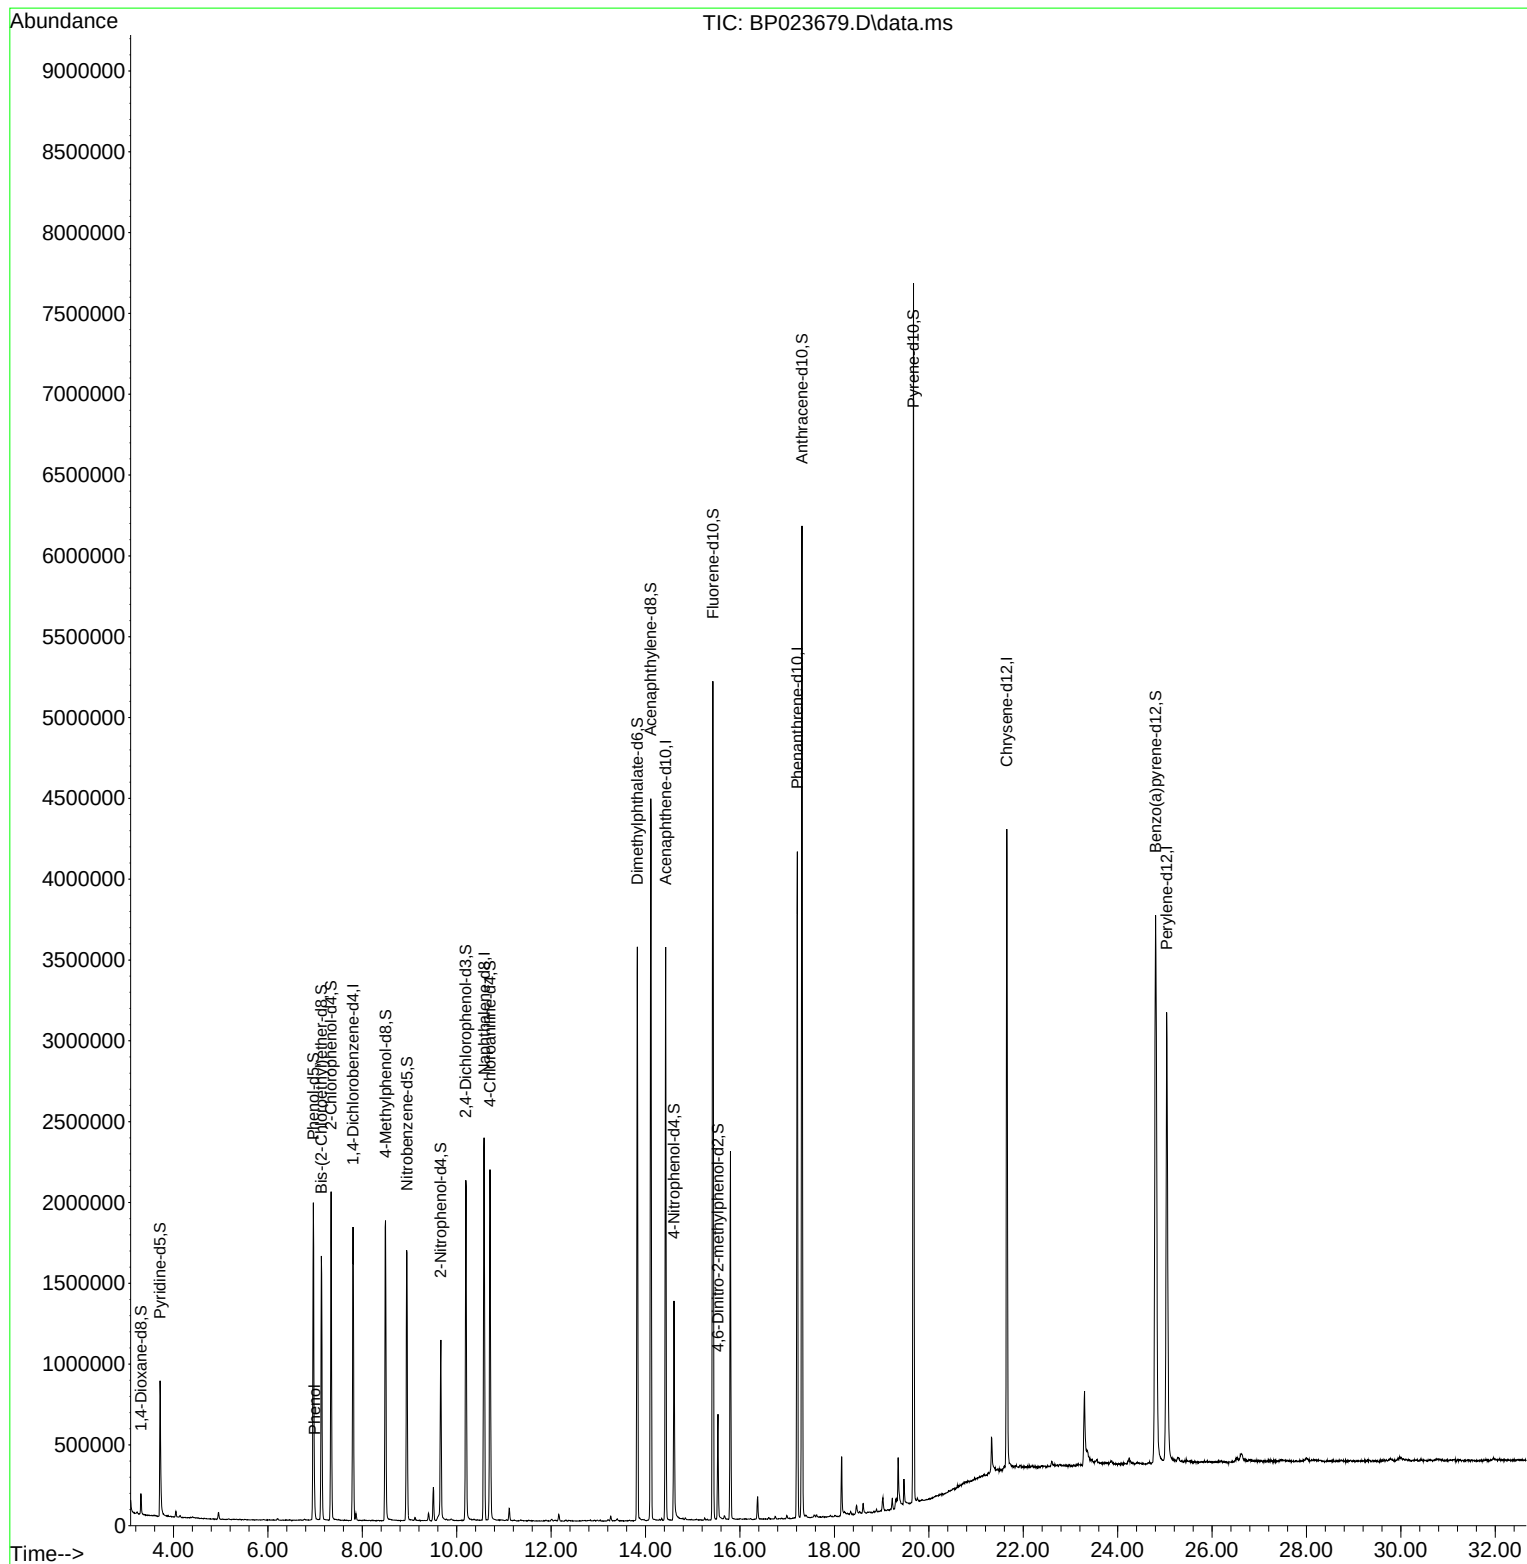

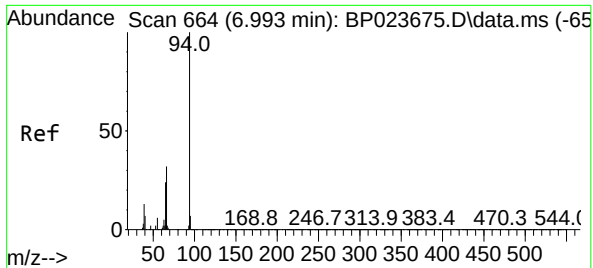

#8
Phenol
Concen: 1.240 ng/ul
RT: 6.993 min Scan# 60
Delta R.T. 0.000 min
Lab File: BP023679.D
Acq: 21 Jan 2025 12:06

Instrument :
BNA_P
ClientSampleId :
YE8F7

Tgt Ion:	94	Resp:	56685
Ion	Ratio	Lower	Upper
94	100		
65	25.5	20.4	30.6
66	32.5	26.1	39.1

