

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
 Data File : BP023653.D
 Acq On : 20 Jan 2025 13:52
 Operator : RC/JU
 Sample : PB166120BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK120

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	34	39	49	rVB	208080	299876	1.70%	0.168%
2	3.717	103	107	133	rBV	2986034	4437477	25.19%	2.483%
3	4.052	160	164	170	rVB	33023	48026	0.27%	0.027%
4	6.963	652	659	674	rBV	3364733	5259441	29.86%	2.943%
5	7.134	681	688	700	rVB	2815676	4301134	24.42%	2.407%
6	7.340	714	723	736	rBV	3490887	5401427	30.66%	3.022%
7	7.805	795	802	813	rBV	2507928	3917449	22.24%	2.192%
8	8.493	911	919	940	rBV	4367597	6573624	37.32%	3.678%
9	8.946	986	996	1009	rBV	2921451	4726437	26.83%	2.645%
10	9.663	1107	1118	1134	rBV	2086235	3286720	18.66%	1.839%
11	10.199	1201	1209	1228	rBV	3870696	6202893	35.21%	3.471%
12	10.581	1263	1274	1283	rBV	3284678	5435102	30.85%	3.041%
13	10.704	1287	1295	1309	rBV	3747661	6441209	36.56%	3.604%
14	12.169	1537	1544	1551	rVB	59919	106502	0.60%	0.060%
15	13.398	1750	1753	1759	rVB4	10870	18117	0.10%	0.010%
16	13.834	1820	1827	1834	rBV	6467549	8588501	48.75%	4.805%
17	14.122	1868	1876	1884	rBV	7872363	11067191	62.82%	6.192%
18	14.434	1921	1929	1937	rBV	4741622	6984879	39.65%	3.908%
19	14.610	1952	1959	1979	rBV	2915411	4041825	22.94%	2.261%
20	15.439	2092	2100	2112	rBV	9463899	13363876	75.86%	7.477%
21	15.545	2112	2118	2132	rBV	1699191	2367615	13.44%	1.325%
22	15.681	2137	2141	2148	rVB	40014	71898	0.41%	0.040%
23	16.998	2360	2365	2373	rVB3	20766	36555	0.21%	0.020%
24	17.222	2396	2403	2412	rBV2	6053726	8146290	46.24%	4.558%
25	17.322	2413	2420	2432	rVV	10033695	14281949	81.07%	7.991%
26	18.163	2559	2563	2568	rBV6	25233	44906	0.25%	0.025%
27	19.239	2742	2746	2753	rBV2	102409	138509	0.79%	0.077%
28	19.310	2754	2758	2764	rVB	88928	130508	0.74%	0.073%
29	19.692	2816	2823	2835	rBV2	11242122	16745948	95.06%	9.370%
30	21.674	3153	3160	3172	rBV2	5883818	9054514	51.40%	5.066%
31	24.827	3685	3696	3723	rBV	6032443	17616244	100.00%	9.857%
32	25.068	3728	3737	3753	rVB	3519456	9588032	54.43%	5.365%




Sum of corrected areas: 178724674

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023653.D
Acq On : 20 Jan 2025 13:52
Operator : RC/JU
Sample : PB166120BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK120

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

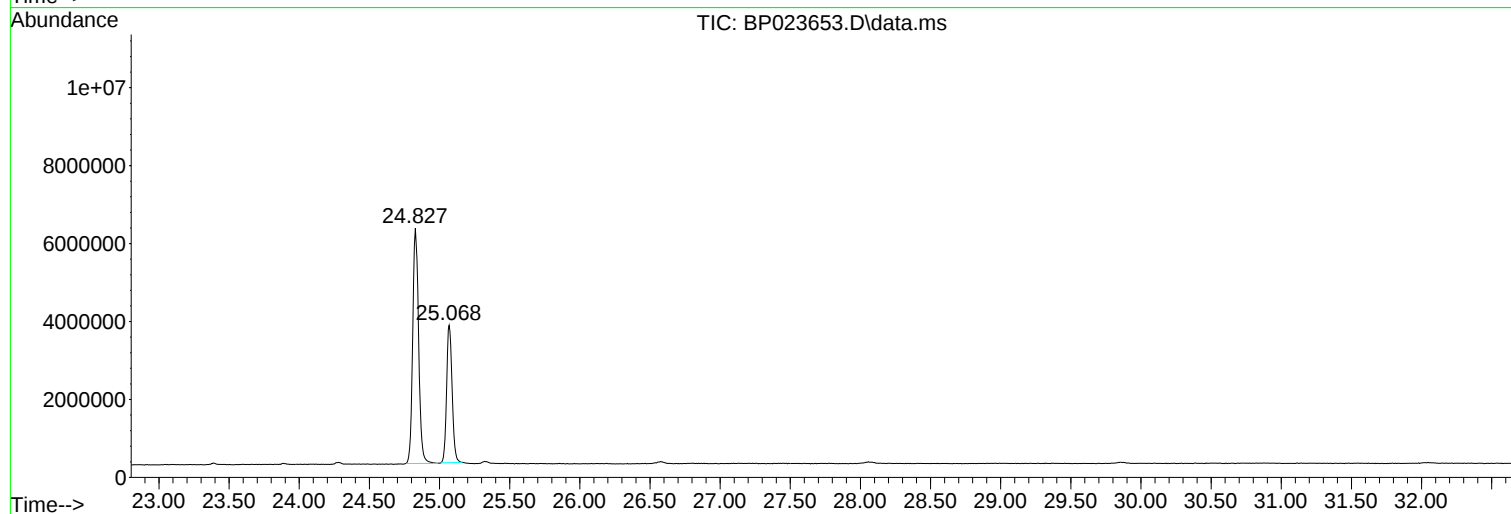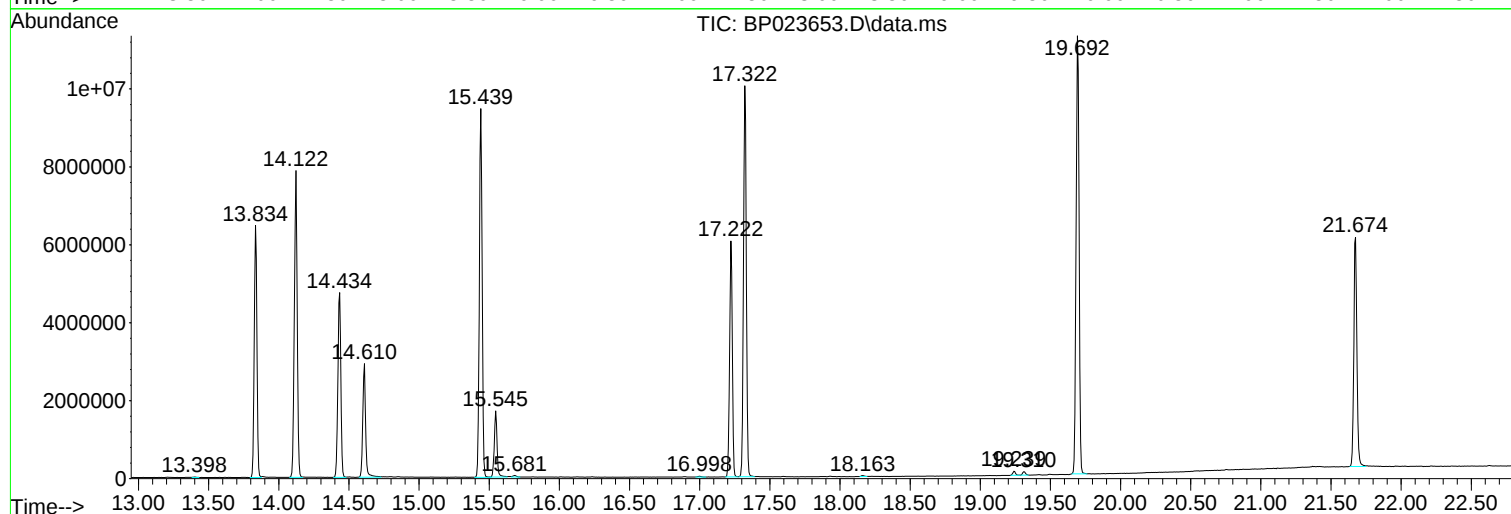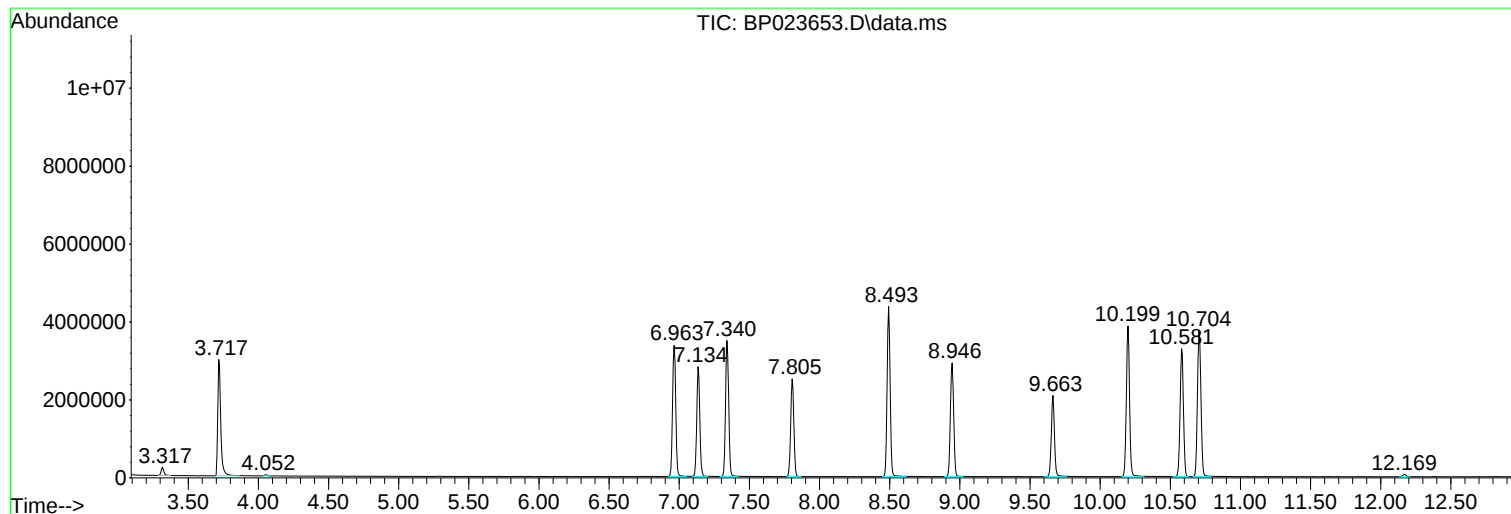

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023653.D
Acq On : 20 Jan 2025 13:52
Operator : RC/JU
Sample : PB166120BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK120

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023653.D
Acq On : 20 Jan 2025 13:52
Operator : RC/JU
Sample : PB166120BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK120

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------