

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
 Data File : BP023676.D
 Acq On : 21 Jan 2025 10:05
 Operator : RC/JU
 Sample : PB166118BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK118

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	45	rVB	247077	355159	1.68%	0.161%
2	3.693	98	103	124	rBV	3363730	5233450	24.72%	2.379%
3	4.023	154	159	163	rBV	36677	55077	0.26%	0.025%
4	6.922	645	652	674	rBV	4012164	6268552	29.60%	2.850%
5	7.099	674	682	698	rVV	3363325	4997623	23.60%	2.272%
6	7.299	706	716	726	rBV	3969830	6349595	29.99%	2.887%
7	7.763	788	795	806	rVB	3342781	4775025	22.55%	2.171%
8	8.452	896	912	932	rBV	5532516	7854352	37.09%	3.571%
9	8.910	981	990	1003	rBV	3131171	5490305	25.93%	2.496%
10	9.634	1105	1113	1127	rBV	2549679	4002882	18.90%	1.820%
11	10.163	1195	1203	1223	rBV	4768117	7469139	35.27%	3.396%
12	10.552	1261	1269	1280	rVB	3618312	6664181	31.47%	3.030%
13	10.675	1283	1290	1306	rBV	4235816	7133717	33.69%	3.243%
14	11.193	1373	1378	1384	rVB3	16201	32889	0.16%	0.015%
15	12.146	1533	1540	1548	rVB	69970	118457	0.56%	0.054%
16	13.398	1744	1753	1759	rBV2	78652	113819	0.54%	0.052%
17	13.828	1818	1826	1841	rBV	7523949	10367560	48.96%	4.713%
18	14.116	1866	1875	1889	rBV2	7886489	13045800	61.61%	5.931%
19	14.251	1891	1898	1900	rBV8	9799	22231	0.10%	0.010%
20	14.434	1921	1929	1935	rBV	6335937	8967916	42.35%	4.077%
21	14.616	1951	1960	1983	rBV	3194850	5275894	24.92%	2.398%
22	14.851	1996	2000	2007	rVB8	13978	28155	0.13%	0.013%
23	15.434	2093	2099	2111	rBV	12134668	16052569	75.81%	7.298%
24	15.545	2111	2118	2134	rVV	2147984	3123310	14.75%	1.420%
25	15.687	2138	2142	2148	rVB2	48171	71843	0.34%	0.033%
26	17.022	2364	2369	2375	rBV	29448	50470	0.24%	0.023%
27	17.245	2398	2407	2416	rBV	5802548	10463623	49.41%	4.757%
28	17.345	2418	2424	2437	rBV	13450955	17474155	82.52%	7.944%
29	18.175	2561	2565	2571	rBV2	88664	127452	0.60%	0.058%
30	18.492	2615	2619	2625	rVB4	25923	44925	0.21%	0.020%
31	19.257	2744	2749	2754	rVB2	118516	177349	0.84%	0.081%
32	19.339	2757	2763	2770	rBV	106908	186637	0.88%	0.085%
33	19.428	2774	2778	2783	rBV	109802	136339	0.64%	0.062%
34	19.510	2788	2792	2796	rBV4	58633	82305	0.39%	0.037%
35	19.710	2816	2826	2834	rBV	15437689	21112310	99.70%	9.598%
36	20.769	3003	3006	3011	rVB	148941	165929	0.78%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023676.D
Acq On : 21 Jan 2025 10:05
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Title : SVOA CALIBRATION

37	21.686	3156	3162	3178	rBV	8571988	11892941	56.16%	5.407%
38	24.857	3691	3701	3726	rVB	8365644	21175005	100.00%	9.626%
39	25.080	3729	3739	3758	rVB	4611920	12464172	58.86%	5.666%
40	25.339	3779	3783	3797	rVB3	243707	546546	2.58%	0.248%




Sum of corrected areas: 219969658

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023676.D
Acq On : 21 Jan 2025 10:05
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

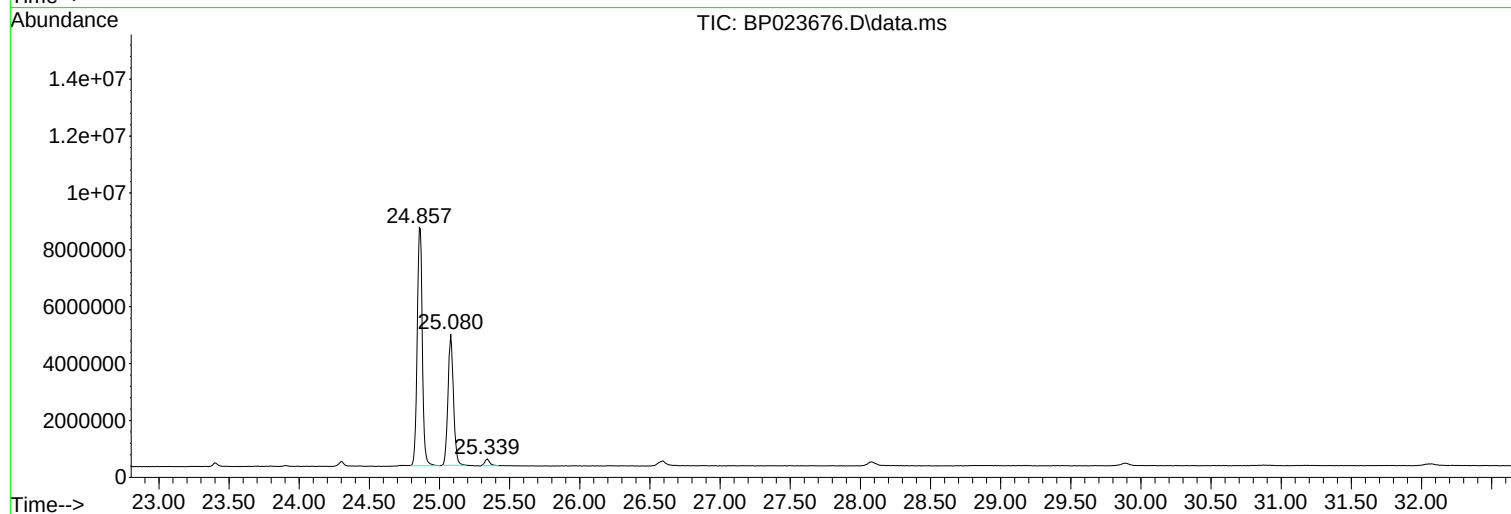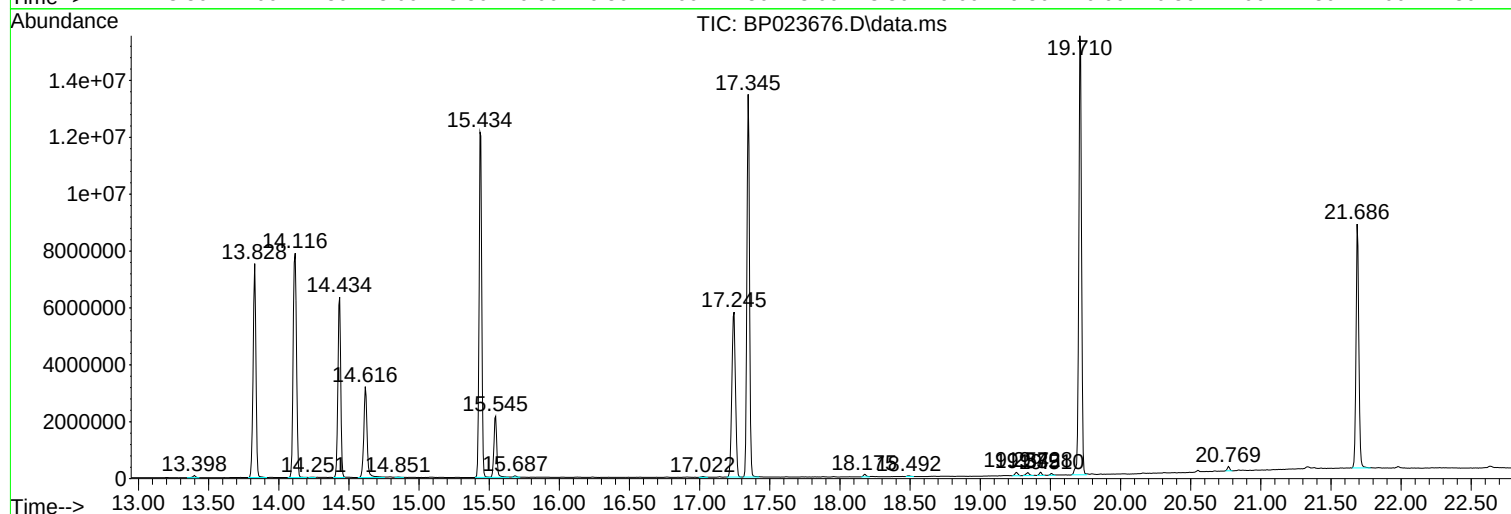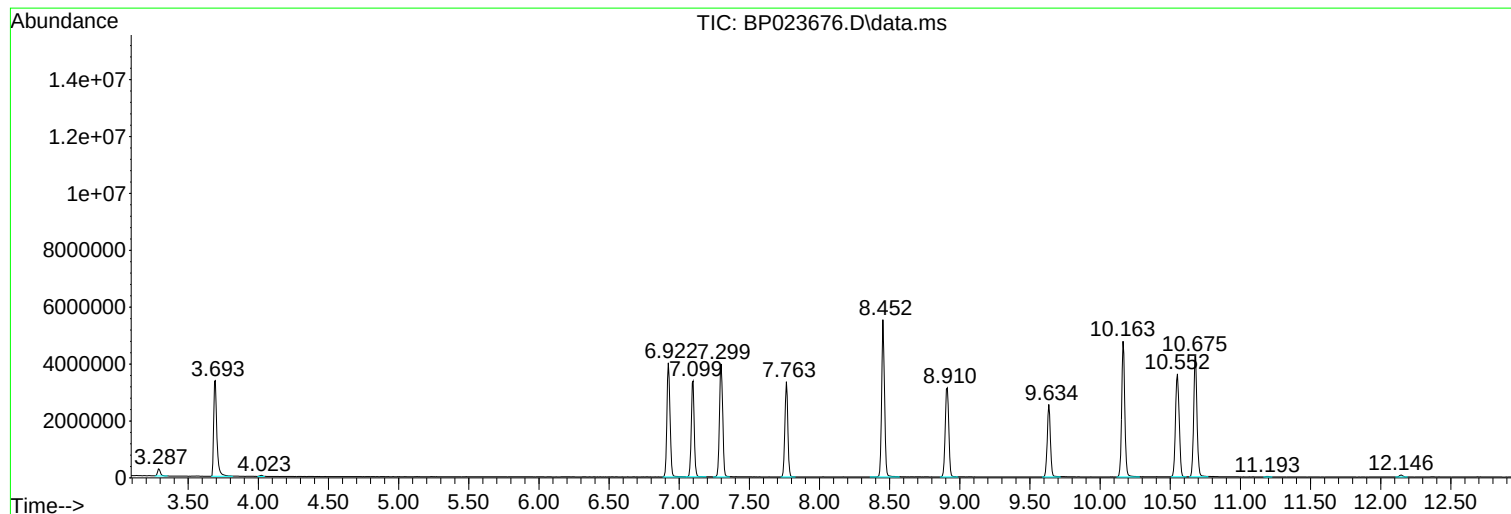

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023676.D
Acq On : 21 Jan 2025 10:05
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023676.D
Acq On : 21 Jan 2025 10:05
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------