

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
 Data File : BP023686.D
 Acq On : 21 Jan 2025 16:48
 Operator : RC/JU
 Sample : PB166145BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK145

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023686.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	34	38	45	rVB	111942	139121	1.66%	0.152%
2	3.717	103	107	126	rBV	1345630	1948113	23.19%	2.126%
3	4.052	159	164	172	rVB	76309	112424	1.34%	0.123%
4	6.964	651	659	671	rBV	1560732	2240134	26.66%	2.445%
5	7.134	682	688	701	rVB	1208106	1868897	22.24%	2.040%
6	7.340	716	723	730	rBV	1522243	2269336	27.01%	2.477%
7	7.805	795	802	811	rBV	2450835	3572906	42.52%	3.900%
8	8.493	912	919	933	rBV	1722407	2722266	32.40%	2.971%
9	8.946	988	996	1008	rBV	1218492	1996544	23.76%	2.179%
10	9.663	1110	1118	1134	rBV	766444	1254498	14.93%	1.369%
11	10.199	1199	1209	1224	rBV	1541402	2521934	30.02%	2.753%
12	10.581	1266	1274	1285	rBV	2965427	4791821	57.03%	5.230%
13	10.705	1288	1295	1313	rVV	1536540	2502838	29.79%	2.732%
14	12.163	1538	1543	1550	rBV2	26837	45892	0.55%	0.050%
15	13.399	1745	1753	1758	rBV6	10164	19671	0.23%	0.021%
16	13.828	1817	1826	1839	rBV	2253817	3333579	39.68%	3.639%
17	14.110	1865	1874	1887	rBV	2904047	4424977	52.66%	4.830%
18	14.422	1920	1927	1937	rBV	3774902	5833479	69.43%	6.367%
19	14.604	1951	1958	1974	rBV	898584	1440013	17.14%	1.572%
20	15.434	2091	2099	2111	rBV	3301330	5312530	63.23%	5.799%
21	15.540	2111	2117	2130	rBV	447357	648436	7.72%	0.708%
22	15.669	2135	2139	2147	rVB3	19923	36833	0.44%	0.040%
23	17.004	2360	2366	2372	rBV	19351	33455	0.40%	0.037%
24	17.228	2397	2404	2411	rBV	4839752	6740598	80.22%	7.358%
25	17.322	2414	2420	2435	rVV	4722493	5783052	68.83%	6.312%
26	18.163	2560	2563	2568	rBV7	11687	19782	0.24%	0.022%
27	19.239	2743	2746	2753	rVB2	37271	50686	0.60%	0.055%
28	19.310	2754	2758	2762	rBV	37476	51405	0.61%	0.056%
29	19.686	2816	2822	2835	rBV	4819204	6804630	80.99%	7.427%
30	21.651	3150	3156	3169	rBV2	4529472	7915306	94.21%	8.640%
31	24.810	3684	3693	3710	rBV	2780449	6776919	80.66%	7.397%
32	25.033	3722	3731	3750	rVB	2827390	8402172	100.00%	9.171%




Sum of corrected areas: 91614247

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023686.D
Acq On : 21 Jan 2025 16:48
Operator : RC/JU
Sample : PB166145BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK145

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

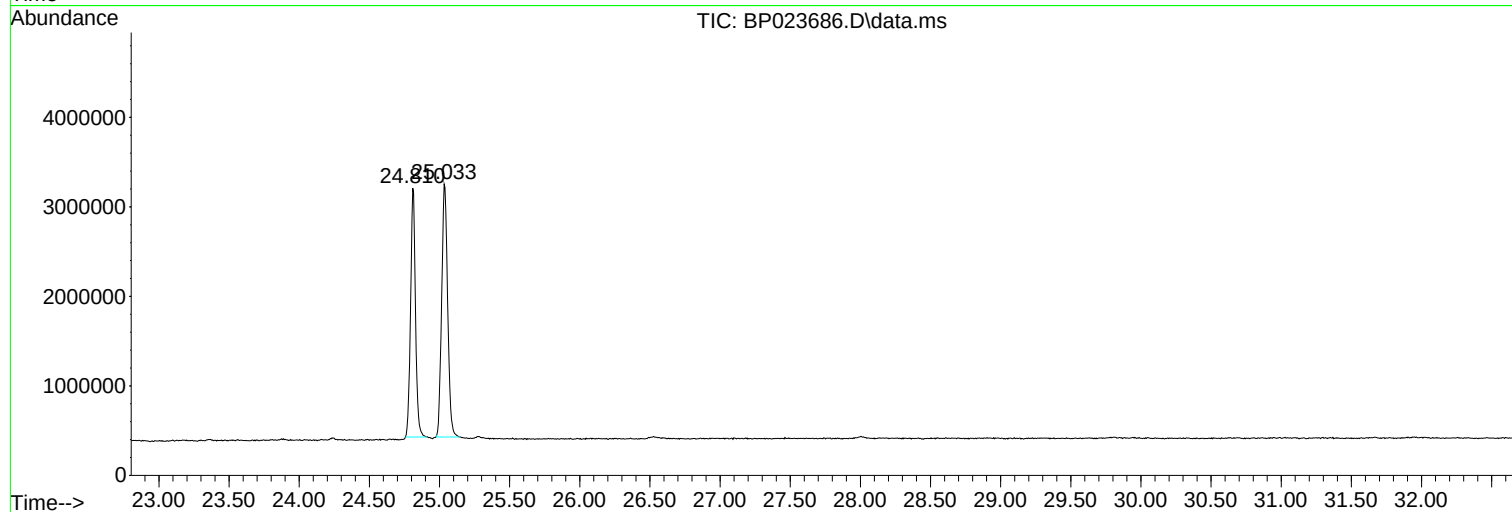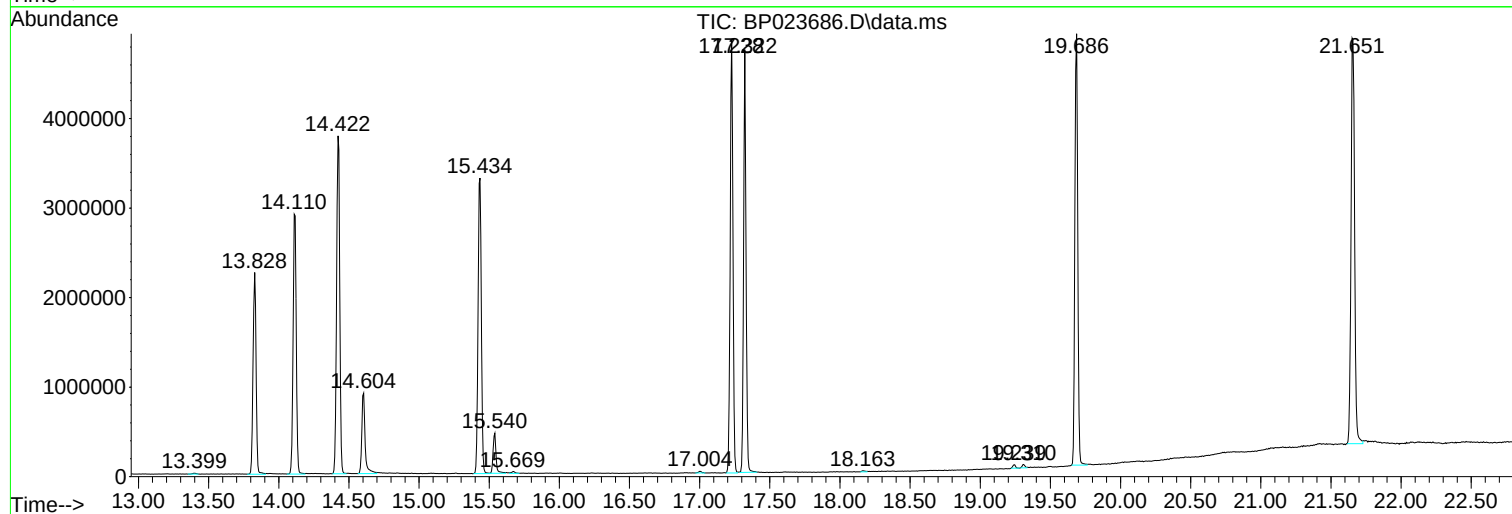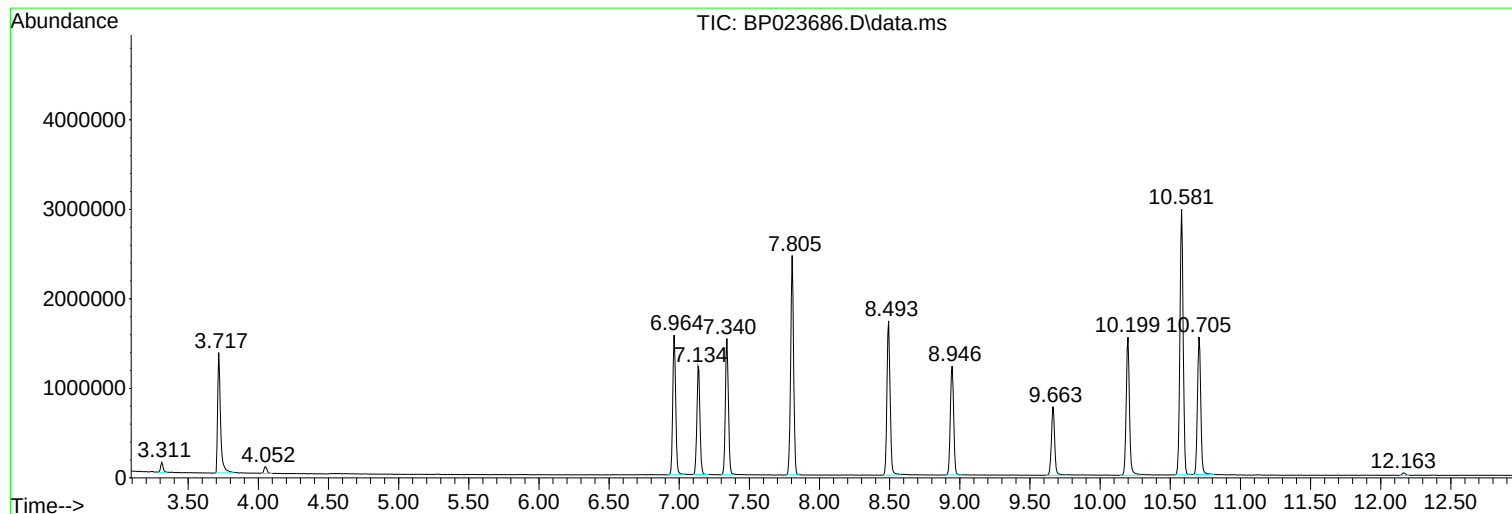

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023686.D
Acq On : 21 Jan 2025 16:48
Operator : RC/JU
Sample : PB166145BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK145

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012025\
Data File : BP023686.D
Acq On : 21 Jan 2025 16:48
Operator : RC/JU
Sample : PB166145BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK145

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP011425.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------