
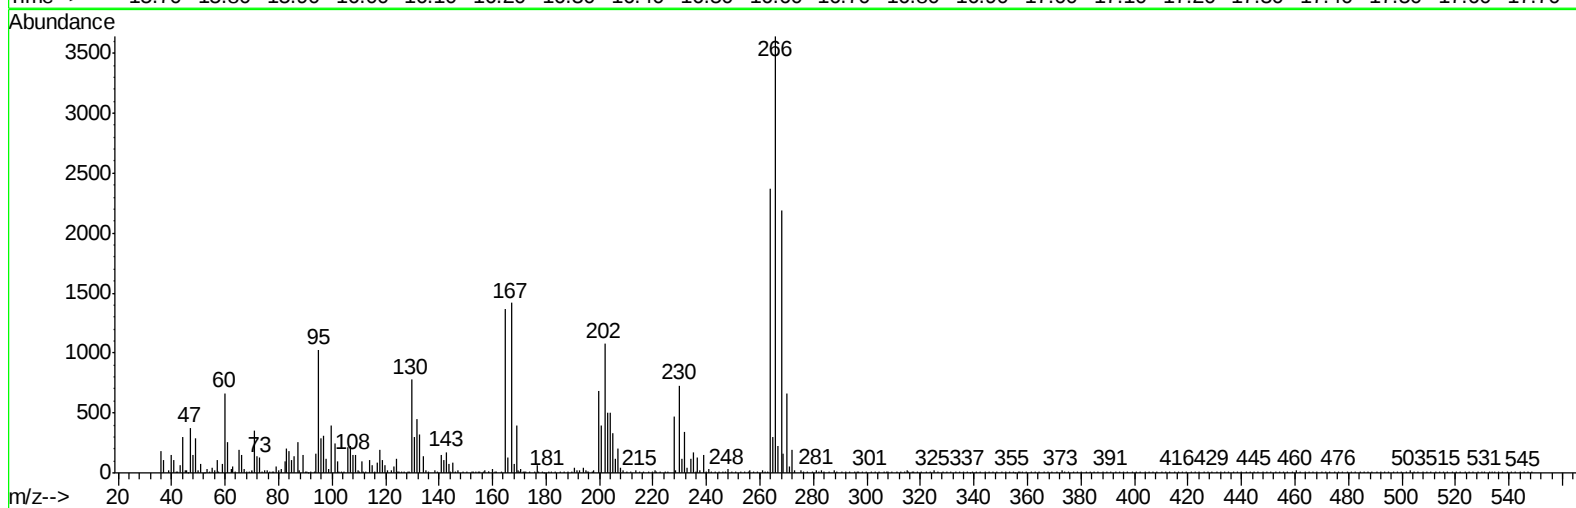


Data File : BP001668.D
Acq On : 21 Jan 2020 12:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 04:03:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 21:52:04 2020
Response via : Initial Calibration

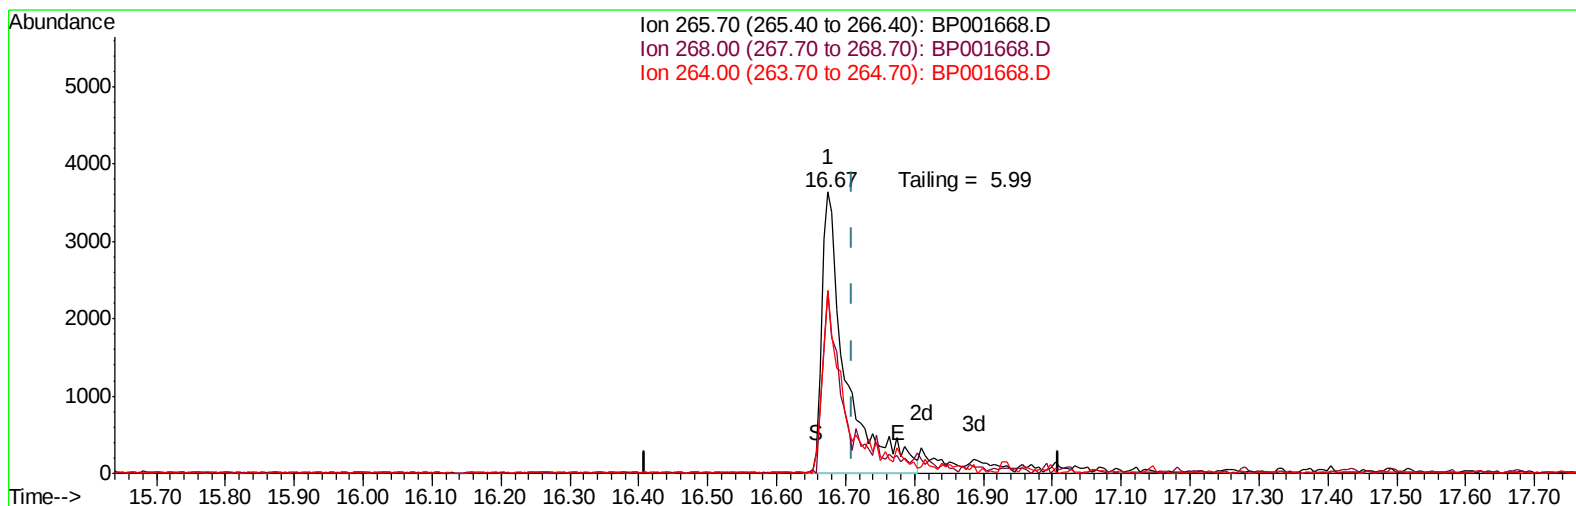

TIC: BP001668.D

(70) Pentachlorophenol (C)



16.675min (-0.035) 99883.78ng

response 7953

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	64.62
264.00	63.60	64.97
0.00	0.00	0.00

Data File : BP001668.D
Acq On : 21 Jan 2020 12:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 04:03:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 14 21:52:04 2020
Response via : Initial Calibration

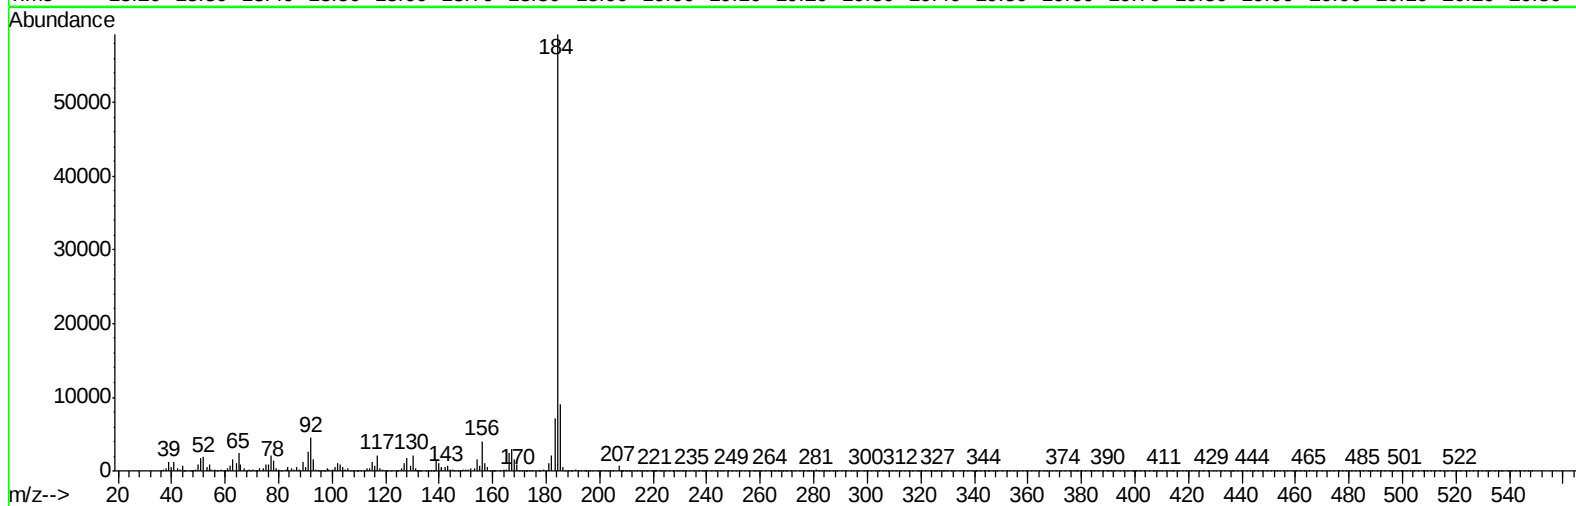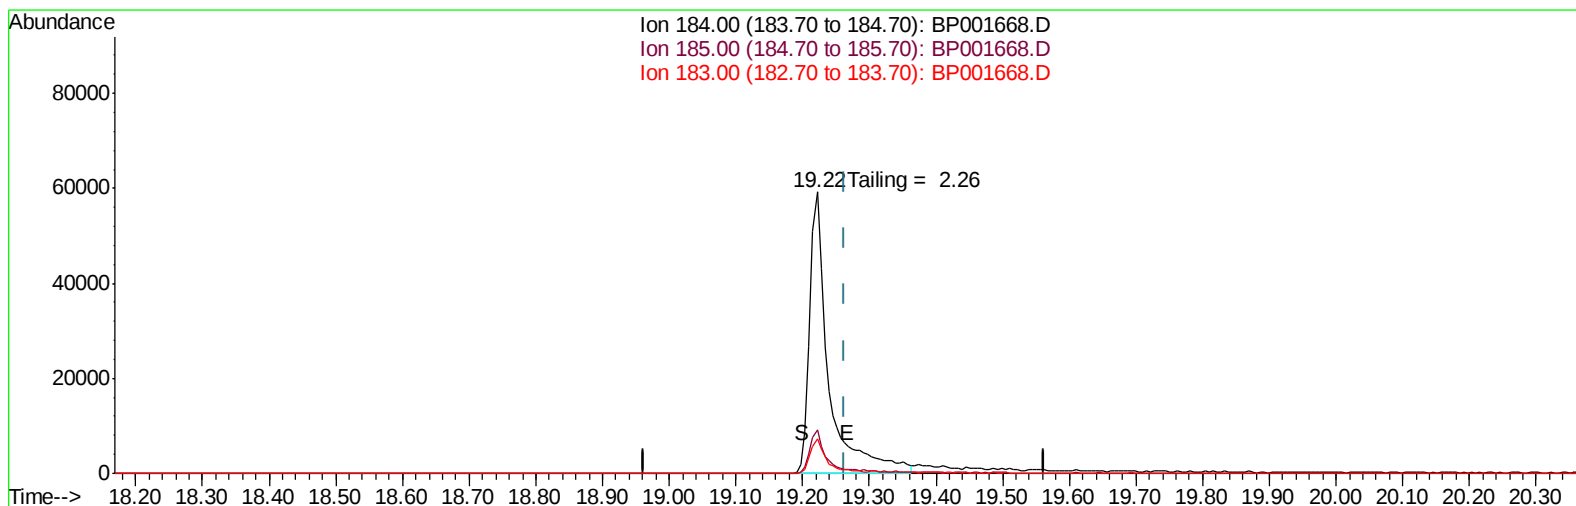

TIC: BP001668.D

(77) Benzidine

19.222min (-0.041) 298088.09ng

response 115709

Ion	Exp%	Act%
184.00	100	100
185.00	13.30	15.29
183.00	11.70	12.13
0.00	0.00	0.00