


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP012120\
 Data File : BP001668.D
 Acq On : 21 Jan 2020 12:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 21:52:04 2020

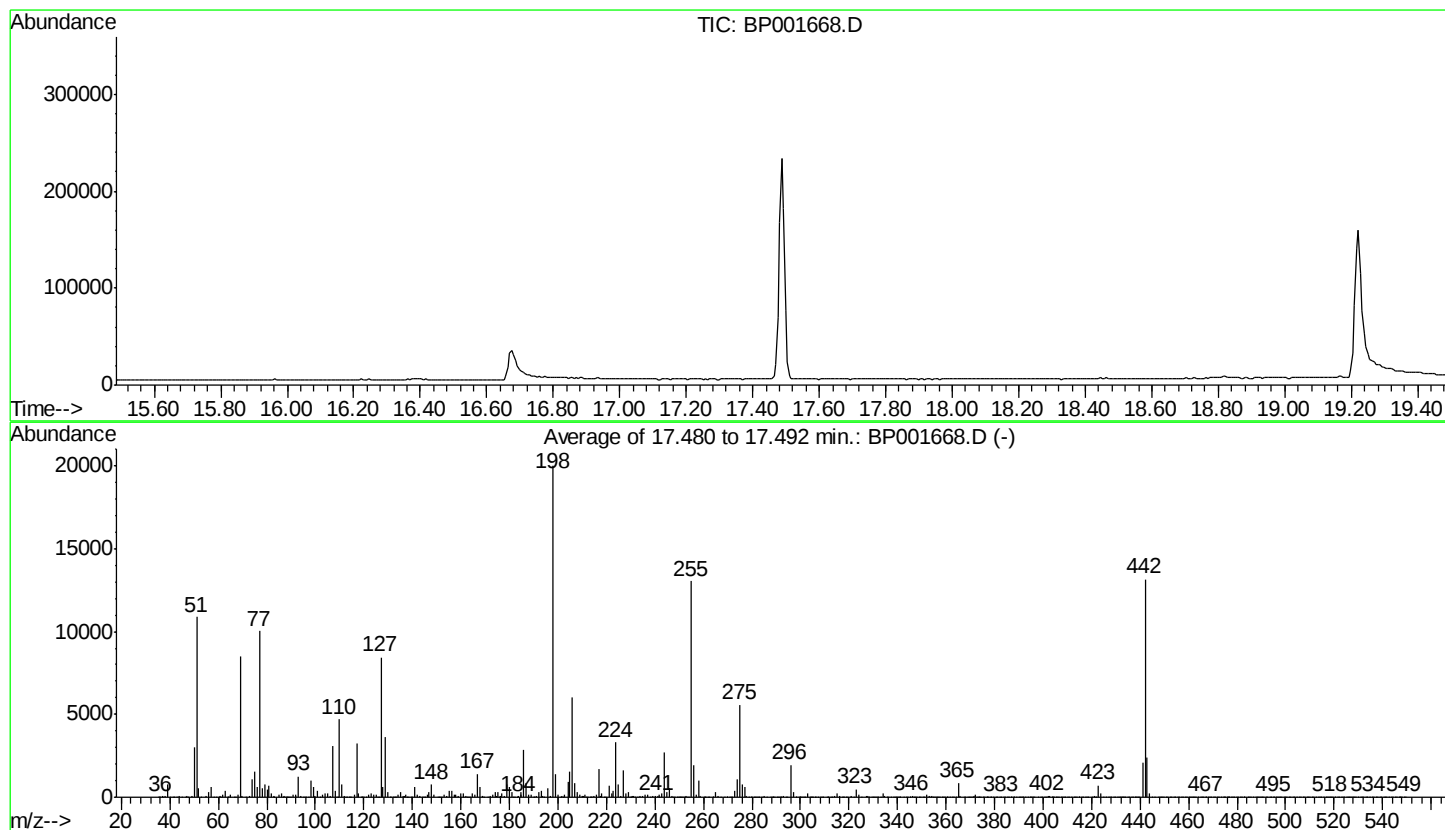

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	10861	PASS
68	69	0.00	2	1.9	166	PASS
69	198	0.00	100	42.6	8524	PASS
70	69	0.00	2	0.7	60	PASS
127	198	10	80	42.1	8420	PASS
197	198	0.00	2	0.5	103	PASS
198	198	100	100	100.0	20008	PASS
199	198	5	9	7.0	1409	PASS
275	198	10	60	28.0	5597	PASS
365	198	1	100	4.4	875	PASS
441	198	0.01	100	10.4	2077	PASS
442	198	50	100	65.8	13160	PASS
443	442	15	24	18.1	2378	PASS