

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012225\
 Data File : BP023702.D
 Acq On : 22 Jan 2025 14:10
 Operator : RC/JU
 Sample : SST01074
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST010610

Quant Time: Jan 22 23:34:59 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 22 23:30:27 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	542723	20.000	ng/u1	0.00
20) Naphthalene-d8	10.575	136	2241394	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.416	164	1394417	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.210	188	2754747	20.000	ng/u1	0.00
79) Chrysene-d12	21.669	240	2930019	20.000	ng/u1	0.02
88) Perylene-d12	25.051	264	2982989	20.000	ng/u1	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	53116	3.942	ng/uL	0.00
4) Pyridine-d5	3.711	84	357347	9.190	ng/u1	0.00
7) Phenol-d5	6.952	99	395042	8.602	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	248685	9.587	ng/u1	0.00
11) 2-Chlorophenol-d4	7.328	132	314354	9.004	ng/u1	0.00
15) 4-Methylphenol-d8	8.481	113	309341	8.566	ng/u1	0.00
21) Nitrobenzene-d5	8.934	128	152675	9.041	ng/u1	0.00
24) 2-Nitrophenol-d4	9.652	143	124952	8.071	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	288951	8.879	ng/u1	0.00
31) 4-Chloroaniline-d4	10.693	131	470208	9.035	ng/u1	0.00
46) Dimethylphthalate-d6	13.822	166	948758	9.461	ng/u1	0.00
49) Acenaphthylene-d8	14.104	160	1091785	9.407	ng/u1	0.00
54) 4-Nitrophenol-d4	14.592	143	155589	7.722	ng/u1	-0.01
60) Fluorene-d10	15.422	176	816068	9.507	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.528	200	83169	6.131	ng/u1	0.00
73) Anthracene-d10	17.316	188	1246904	9.428	ng/u1	0.00
81) Pyrene-d10	19.692	212	1401361	9.399	ng/u1	0.01
92) Benzo(a)pyrene-d12	24.821	264	1340389	8.977	ng/u1	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.334	88	56236	3.945	ng/uL	99
5) Pyridine	3.728	79	369708	9.405	ng/u1	97
6) Benzaldehyde	6.940	77	278225	12.029	ng/u1	100
8) Phenol	6.981	94	432353	8.997	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.216	93	353213	9.449	ng/u1	99
12) 2-Chlorophenol	7.358	128	344812	9.317	ng/u1	99
13) 2-Methylphenol	8.222	108	298806	8.569	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.310	45	378057	9.750	ng/u1	99
16) Acetophenone	8.605	105	546740	9.427	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.587	70	247853	9.238	ng/u1	99
18) 4-Methylphenol	8.540	108	345135	8.902	ng/u1	98
19) Hexachloroethane	8.869	117	143722	9.502	ng/u1	98
22) Nitrobenzene	8.975	77	366953	9.300	ng/u1	100
23) Isophorone	9.499	82	682394	9.093	ng/u1	99
25) 2-Nitrophenol	9.681	139	152862	8.410	ng/u1	99
26) 2,4-Dimethylphenol	9.740	107	344979	9.157	ng/u1	98
27) Bis(2-Chloroethoxy)met...	9.975	93	462232	9.506	ng/u1	100
29) 2,4-Dichlorophenol	10.216	162	306239	9.103	ng/u1	97
30) Naphthalene	10.622	128	1160935	9.625	ng/u1	99
32) 4-Chloroaniline	10.716	127	457316	9.204	ng/u1	100
33) Hexachlorobutadiene	10.916	225	200663	9.475	ng/u1	98
34) Caprolactam	11.475	113	96720	7.943	ng/u1	94
35) 4-Chloro-3-methylphenol	11.840	107	306291	8.788	ng/u1	98
36) 2-Methylnaphthalene	12.228	142	761846	9.353	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012225\
 Data File : BP023702.D
 Acq On : 22 Jan 2025 14:10
 Operator : RC/JU
 Sample : SSTD01074
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010610


Quant Time: Jan 22 23:34:59 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jan 22 23:30:27 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.445	142	764050	9.384	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.598	216	393681	9.505	ng/ul	98
40) Hexachlorocyclopentadiene	12.587	237	173954	8.243	ng/ul	100
41) 2,4,6-Trichlorophenol	12.834	196	211763	8.696	ng/ul	99
42) 2,4,5-Trichlorophenol	12.904	196	241221	8.969	ng/ul	99
43) 1,1'-Biphenyl	13.245	154	1010478	9.631	ng/ul	99
44) 2-Chloronaphthalene	13.281	162	791764	9.693	ng/ul	99
45) 2-Nitroaniline	13.481	65	168968	8.710	ng/ul	99
47) Dimethylphthalate	13.869	163	954681	9.483	ng/ul	100
48) 2,6-Dinitrotoluene	13.981	165	150273	8.369	ng/ul	95
50) Acenaphthylene	14.140	152	1205316	9.578	ng/ul	99
51) 3-Nitroaniline	14.304	138	179905	8.585	ng/ul#	91
52) Acenaphthene	14.487	153	848051	9.531	ng/ul	100
53) 2,4-Dinitrophenol	14.516	184	49333	5.596	ng/ul	96
55) 4-Nitrophenol	14.610	109	128953	8.721	ng/ul	97
56) Dibenzofuran	14.822	168	1173468	9.589	ng/ul	100
57) 2,4-Dinitrotoluene	14.769	165	226034	8.414	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	15.045	232	189748	8.590	ng/ul	95
59) Diethylphthalate	15.251	149	925538	9.347	ng/ul	99
61) Fluorene	15.481	166	978148	9.591	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.481	204	476561	9.547	ng/ul	99
63) 4-Nitroaniline	15.481	138	198085	9.290	ng/ul	95
66) 4,6-Dinitro-2-methylph...	15.545	198	98115	6.431	ng/ul	97
67) N-Nitrosodiphenylamine	15.692	169	784671	9.484	ng/ul	100
68) 4-Bromophenyl-phenylether	16.386	248	271826	9.216	ng/ul	98
69) Hexachlorobenzene	16.498	284	338094	9.420	ng/ul	97
70) Atrazine	16.663	200	262118	8.589	ng/ul	99
71) Pentachlorophenol	16.851	266	158948	7.332	ng/ul	97
72) Phenanthrene	17.257	178	1503138	9.658	ng/ul	99
74) Anthracene	17.357	178	1513991	9.793	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.204	216	382168	9.562	ng/ul	97
76) Pentachlorobenzene	14.740	250	403949	9.515	ng/ul	99
77) Carbazole	17.628	167	1348975	9.940	ng/ul	100
78) Di-n-butylphthalate	18.228	149	1427394	9.238	ng/ul	99
80) Fluoranthene	19.345	202	1655716	9.767	ng/ul	99
82) Pyrene	19.722	202	1822099	9.896	ng/ul	99
83) Butylbenzylphthalate	20.680	149	553487	8.335	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.563	252	410862	7.946	ng/ul	99
85) Benzo(a)anthracene	21.651	228	1794894	9.663	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.610	149	830592	8.388	ng/ul	100
87) Chrysene	21.716	228	1708227	9.823	ng/ul	99
89) Di-n-octyl phthalate	22.916	149	1125903	7.534	ng/ul	100
90) Benzo(b)fluoranthene	23.980	252	1599052	9.024	ng/ul	99
91) Benzo(k)fluoranthene	24.057	252	1695769	9.283	ng/ul	98
93) Benzo(a)pyrene	24.892	252	1516105	9.090	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	28.903	276	1554212	7.509	ng/ul	100
95) Dibenzo(a,h)anthracene	28.986	278	1508478	8.978	ng/ul	99
96) Benzo(g,h,i)perylene	30.045	276	573819	3.599	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jan 22 23:34:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jan 22 23:30:27 2025
Response via : Initial Calibration







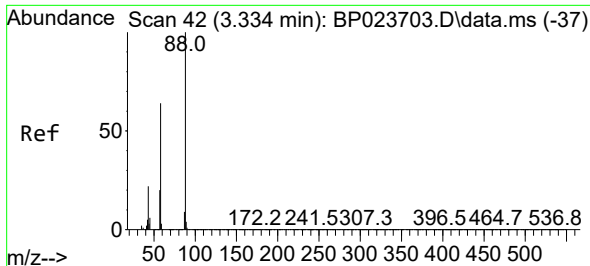

#2
1,4-Dioxane
Concen: 3.945 ng/uL
RT: 3.334 min Scan# 41
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion: 88 Resp: 56236
Ion Ratio Lower Upper
88 100
43 23.9 18.3 27.5
58 62.5 50.7 76.1

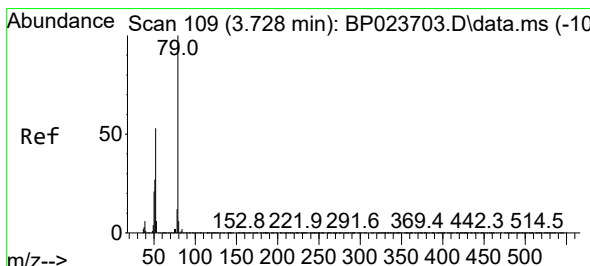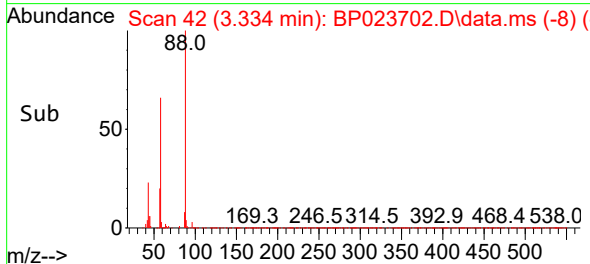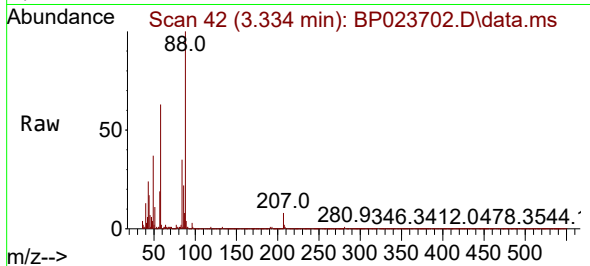

#5
Pyridine
Concen: 9.405 ng/uL
RT: 3.728 min Scan# 109
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion: 79 Resp: 369708
Ion Ratio Lower Upper
79 100
52 58.3 45.0 67.4
51 29.9 22.2 33.4


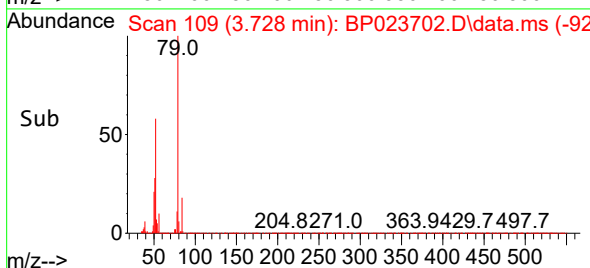
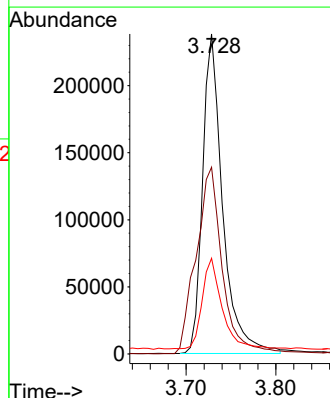
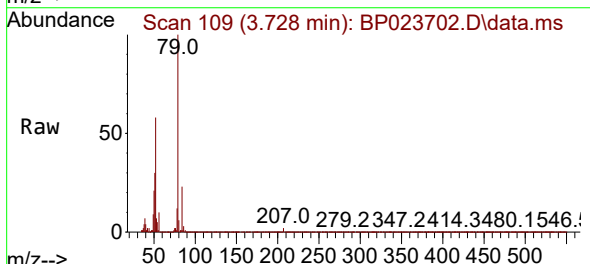




#6
Benzaldehyde
Concen: 12.029 ng/ul
RT: 6.940 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion: 77 Resp: 278225
Ion Ratio Lower Upper
77 100
105 101.2 81.0 121.6
106 99.0 78.6 118.0

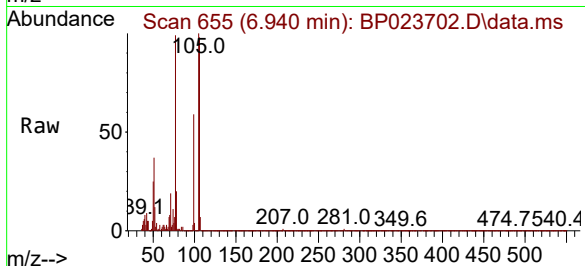

#8
Phenol
Concen: 8.997 ng/ul
RT: 6.981 min Scan# 662
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion: 94 Resp: 432353
Ion Ratio Lower Upper
94 100
65 25.1 20.2 30.2
66 32.0 26.0 39.0



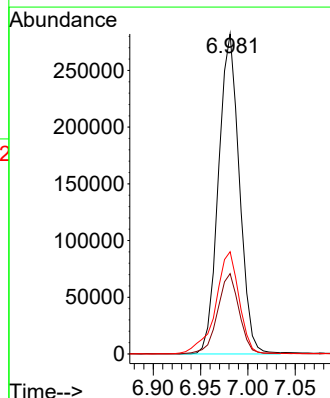
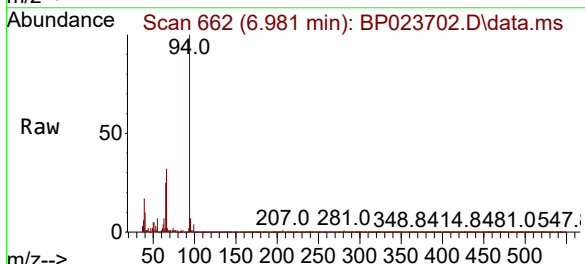




#10
Bis(2-Chloroethyl)ether
Concen: 9.449 ng/ul
RT: 7.216 min Scan# 703
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion: 93 Resp: 353213
Ion Ratio Lower Upper
93 100
63 67.6 52.9 79.3
95 32.5 26.1 39.1



#12
2-Chlorophenol
Concen: 9.317 ng/ul
RT: 7.358 min Scan# 726
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:128 Resp: 344812
Ion Ratio Lower Upper
128 100
64 40.0 32.4 48.6
130 32.1 26.2 39.4









#13
2-Methylphenol
Concen: 8.569 ng/ul
RT: 8.222 min Scan# 873
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:108 Resp: 298806
Ion Ratio Lower Upper
108 100
107 89.0 69.6 104.4



#14
2,2'-oxybis(1-Chloropropane)
Concen: 9.750 ng/ul
RT: 8.310 min Scan# 888
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion: 45 Resp: 378057
Ion Ratio Lower Upper
45 100
77 18.7 14.8 22.2
79 13.7 10.6 16.0


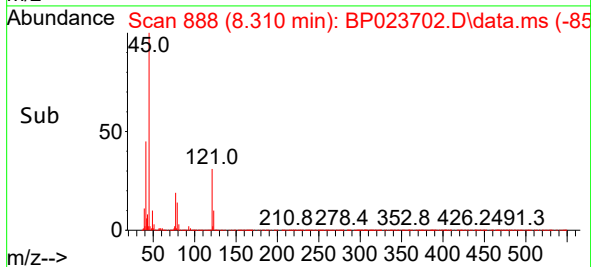

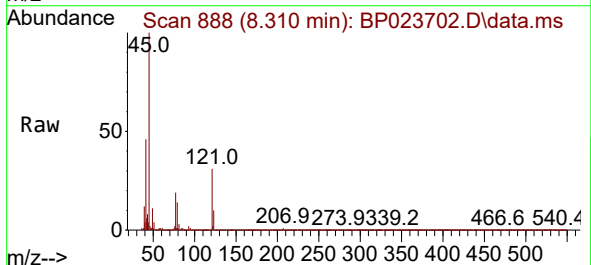




#16
Acetophenone
Concen: 9.427 ng/ul
RT: 8.605 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:105 Resp: 546740
Ion Ratio Lower Upper
105 100
77 73.6 58.1 87.1
51 21.6 16.4 24.6



#17
N-Nitroso-di-n-propylamine
Concen: 9.238 ng/ul
RT: 8.587 min Scan# 935
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion: 70 Resp: 247853
Ion Ratio Lower Upper
70 100
42 47.8 37.7 56.5
101 9.7 8.4 12.6
130 22.6 18.3 27.5



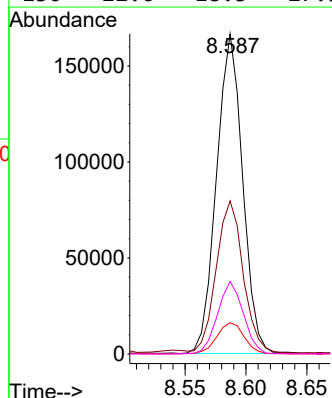





#18
4-Methylphenol
Concen: 8.902 ng/ul
RT: 8.540 min Scan# 91
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:108 Resp: 345135
Ion Ratio Lower Upper
108 100
107 111.7 91.2 136.8



#19
Hexachloroethane
Concen: 9.502 ng/ul
RT: 8.869 min Scan# 983
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:117 Resp: 143722
Ion Ratio Lower Upper
117 100
201 97.1 76.6 114.8
199 63.6 48.7 73.1



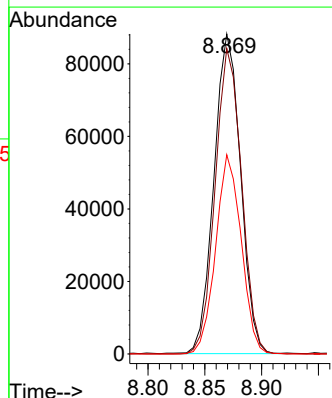





#22
Nitrobenzene
Concen: 9.300 ng/ul
RT: 8.975 min Scan# 1001
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion: 77 Resp: 366953
Ion Ratio Lower Upper
77 100
123 47.4 38.0 57.0
65 12.5 9.8 14.6



#23
Isophorone
Concen: 9.093 ng/ul
RT: 9.499 min Scan# 1090
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion: 82 Resp: 682394
Ion Ratio Lower Upper
82 100
95 7.1 5.2 7.8
138 18.3 14.9 22.3









#25
2-Nitrophenol
Concen: 8.410 ng/ul
RT: 9.681 min Scan# 1122
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:139 Resp: 152862
Ion Ratio Lower Upper
139 100
65 48.1 37.4 56.2
109 28.9 22.8 34.2



#26
2,4-Dimethylphenol
Concen: 9.157 ng/ul
RT: 9.740 min Scan# 1131
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:107 Resp: 344979
Ion Ratio Lower Upper
107 100
121 51.0 42.0 63.0
122 89.6 70.2 105.4



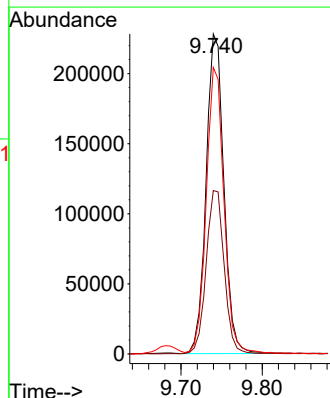





#27
 Bis(2-Chloroethoxy)methane
 Concen: 9.506 ng/ul
 RT: 9.975 min Scan# 1171
 Delta R.T. -0.006 min
 Lab File: BP023702.D
 Acq: 22 Jan 2025 14:10




Instrument :
 BNA_P
 ClientSampleId :
 SST010610


Tgt Ion: 93 Resp: 462232
 Ion Ratio Lower Upper
 93 100
 95 32.3 25.8 38.8
 123 11.2 9.4 14.2



#29
 2,4-Dichlorophenol
 Concen: 9.103 ng/ul
 RT: 10.216 min Scan# 1212
 Delta R.T. -0.006 min
 Lab File: BP023702.D
 Acq: 22 Jan 2025 14:10

Tgt Ion: 162 Resp: 306239
 Ion Ratio Lower Upper
 162 100
 164 63.3 52.3 78.5
 98 33.4 28.3 42.5









#30
Naphthalene
Concen: 9.625 ng/ul
RT: 10.622 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:128 Resp: 1160935
Ion Ratio Lower Upper
128 100
129 11.1 8.6 12.8
127 12.6 10.2 15.4



#32
4-Chloroaniline
Concen: 9.204 ng/ul
RT: 10.716 min Scan# 1297
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:127 Resp: 457316
Ion Ratio Lower Upper
127 100
129 32.6 26.2 39.4









#33
Hexachlorobutadiene
Concen: 9.475 ng/ul
RT: 10.916 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:225 Resp: 200663
Ion Ratio Lower Upper
225 100
223 64.7 50.9 76.3
227 63.0 51.8 77.8



#34
Caprolactam
Concen: 7.943 ng/ul
RT: 11.475 min Scan# 1426
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:113 Resp: 96720
Ion Ratio Lower Upper
113 100
55 139.5 105.8 158.6
56 104.1 79.3 118.9



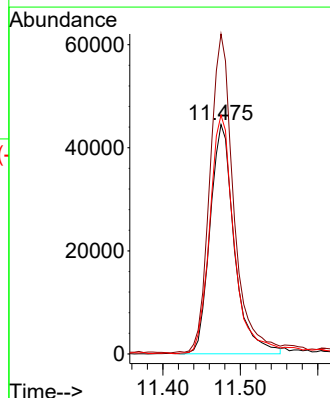





#35
4-Chloro-3-methylphenol
Concen: 8.788 ng/ul
RT: 11.840 min Scan# 1489
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:107 Resp: 306291
Ion Ratio Lower Upper
107 100
144 26.8 21.3 31.9
142 83.9 65.5 98.3



#36
2-Methylnaphthalene
Concen: 9.353 ng/ul
RT: 12.228 min Scan# 1554
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:142 Resp: 761846
Ion Ratio Lower Upper
142 100
141 88.9 70.5 105.7









#37
1-Methylnaphthalene
Concen: 9.384 ng/ul
RT: 12.445 min Scan# 1591
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:142 Resp: 764050
Ion Ratio Lower Upper
142 100
141 91.6 72.1 108.1
116 3.8 2.9 4.3

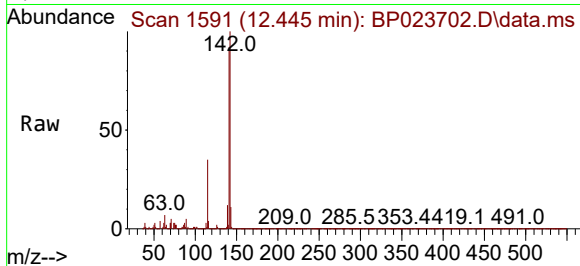

#39
1,2,4,5-Tetrachlorobenzene
Concen: 9.505 ng/ul
RT: 12.598 min Scan# 1617
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:216 Resp: 393681
Ion Ratio Lower Upper
216 100
214 77.8 63.2 94.8
179 20.5 16.9 25.3
108 19.1 14.3 21.5




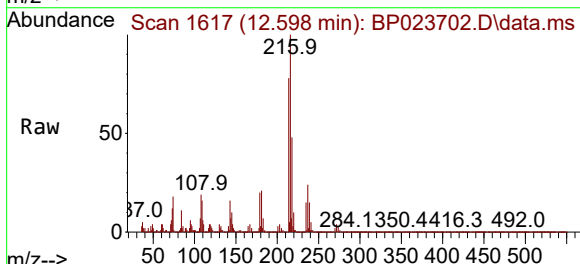




#40
Hexachlorocyclopentadiene
Concen: 8.243 ng/ul
RT: 12.587 min Scan# 1615
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:237 Resp: 173954
Ion Ratio Lower Upper
237 100
235 62.8 50.4 75.6
272 13.9 10.9 16.3

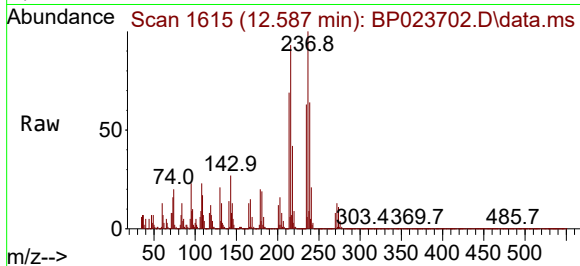

#41
2,4,6-Trichlorophenol
Concen: 8.696 ng/ul
RT: 12.834 min Scan# 1657
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:196 Resp: 211763
Ion Ratio Lower Upper
196 100
198 95.9 77.6 116.4
200 30.6 24.5 36.7

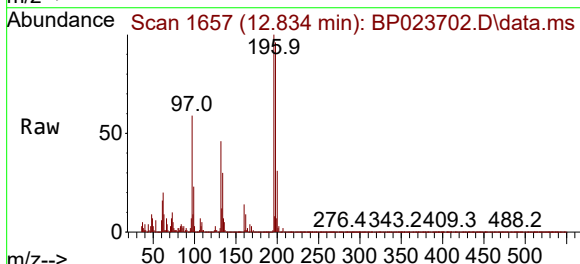



#42

2,4,5-Trichlorophenol

Concen: 8.969 ng/ul

RT: 12.904 min Scan# 1669

Delta R.T. -0.006 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:196 Resp: 241221

Ion Ratio Lower Upper

196 100

198 96.0 77.4 116.2

200 30.6 25.0 37.4



#43

1,1'-Biphenyl

Concen: 9.631 ng/ul

RT: 13.245 min Scan# 1727

Delta R.T. 0.000 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion:154 Resp: 1010478


Ion Ratio Lower Upper

154 100

153 39.0 32.2 48.2

76 12.8 10.2 15.2

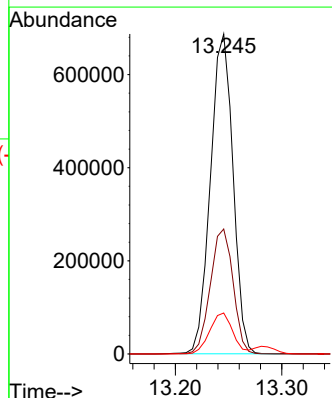



#44

2-Chloronaphthalene

Concen: 9.693 ng/ul

RT: 13.281 min Scan# 1734

Delta R.T. -0.006 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:162 Resp: 791764

Ion Ratio Lower Upper

162 100

164 32.0 26.2 39.2

127 38.3 30.5 45.7

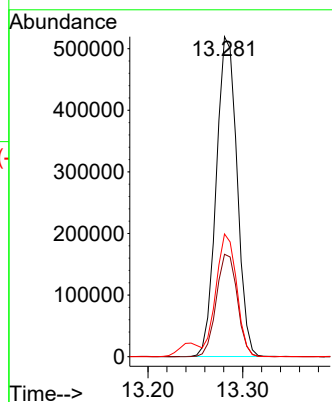

#45

2-Nitroaniline

Concen: 8.710 ng/ul

RT: 13.481 min Scan# 1767

Delta R.T. 0.000 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion: 65 Resp: 168968


Ion Ratio Lower Upper

65 100

92 74.2 61.0 91.4

138 117.0 94.2 141.2









#47
Dimethylphthalate
Concen: 9.483 ng/ul
RT: 13.869 min Scan# 1833
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:163 Resp: 954681
Ion Ratio Lower Upper
163 100
194 4.3 3.3 4.9
164 10.1 8.2 12.2

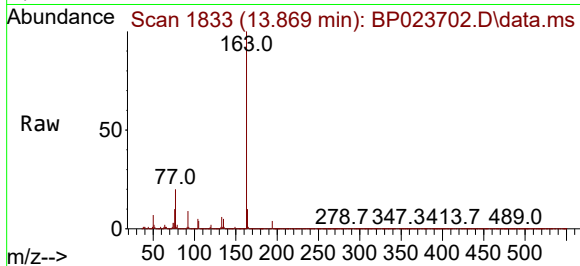

#48
2,6-Dinitrotoluene
Concen: 8.369 ng/ul
RT: 13.981 min Scan# 1852
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:165 Resp: 150273
Ion Ratio Lower Upper
165 100
89 59.2 44.8 67.2
121 24.0 17.0 25.4

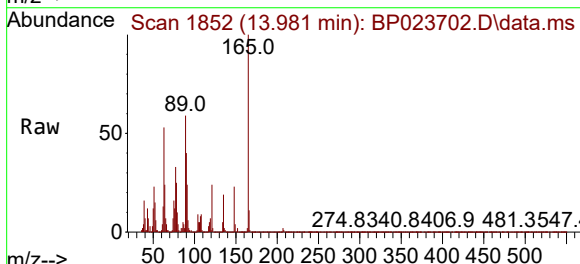



#50

Acenaphthylene

Concen: 9.578 ng/ul

RT: 14.140 min Scan# 1879

Delta R.T. 0.000 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:152 Resp: 1205316

Ion Ratio Lower Upper

152 100

151 19.4 15.8 23.8

153 12.4 10.6 15.8



#51

3-Nitroaniline

Concen: 8.585 ng/ul

RT: 14.304 min Scan# 1907

Delta R.T. -0.006 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion:138 Resp: 179905


Ion Ratio Lower Upper

138 100

108 15.9 9.7 14.5#

92 121.7 89.8 134.6









#52
Acenaphthene
Concen: 9.531 ng/ul
RT: 14.487 min Scan# 1938
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:153 Resp: 848051
Ion Ratio Lower Upper
153 100
152 48.9 39.1 58.7
154 89.1 71.4 107.0

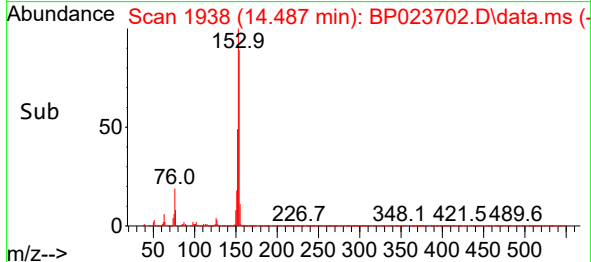

#53
2,4-Dinitrophenol
Concen: 5.596 ng/ul
RT: 14.516 min Scan# 1943
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:184 Resp: 49333
Ion Ratio Lower Upper
184 100
63 62.3 47.8 71.8
154 69.0 52.1 78.1


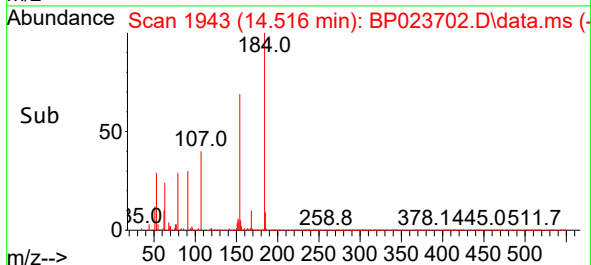
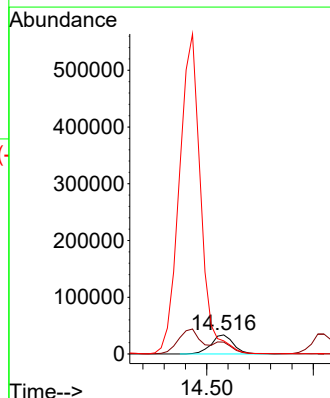
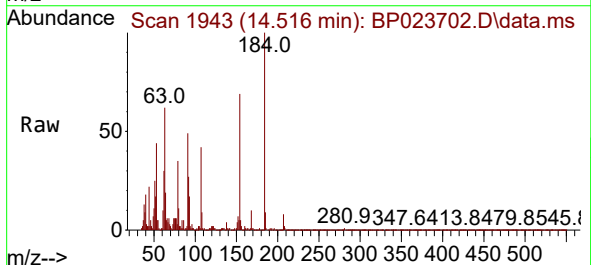




#55
4-Nitrophenol
Concen: 8.721 ng/ul
RT: 14.610 min Scan# 1959
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:109 Resp: 128953
Ion Ratio Lower Upper
109 100
139 142.3 114.3 171.5
65 122.0 103.0 154.6

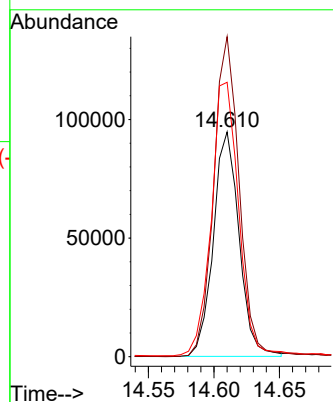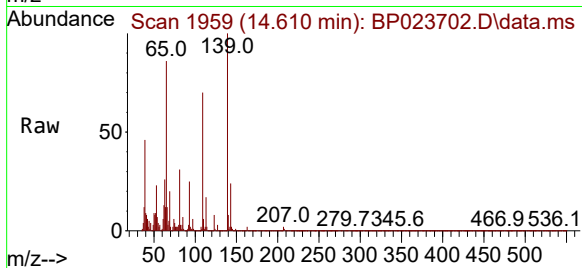

#56
Dibenzofuran
Concen: 9.589 ng/ul
RT: 14.822 min Scan# 1995
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:168 Resp: 1173468
Ion Ratio Lower Upper
168 100
139 36.3 29.3 43.9



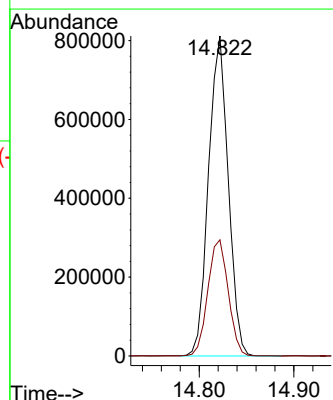
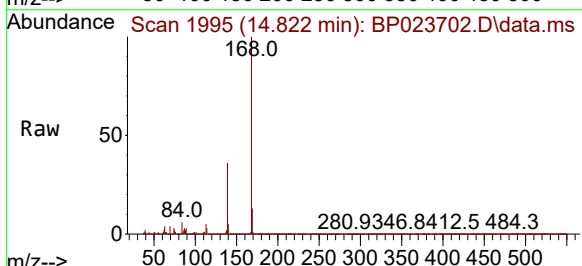




#57
2,4-Dinitrotoluene
Concen: 8.414 ng/ul
RT: 14.769 min Scan# 1986
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:165 Resp: 226034
Ion Ratio Lower Upper
165 100
63 43.8 31.0 46.6
182 2.6 2.2 3.4



#58
2,3,4,6-Tetrachlorophenol
Concen: 8.590 ng/ul
RT: 15.045 min Scan# 2033
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:232 Resp: 189748
Ion Ratio Lower Upper
232 100
131 49.7 36.1 54.1
130 2.5 1.8 2.8
166 31.5 24.2 36.4



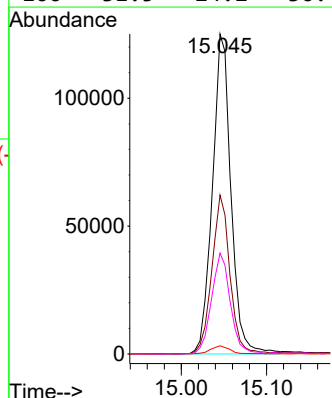





#59
Diethylphthalate
Concen: 9.347 ng/ul
RT: 15.251 min Scan# 2068
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:149 Resp: 925538
Ion Ratio Lower Upper
149 100
177 21.4 17.7 26.5
150 12.3 9.8 14.6

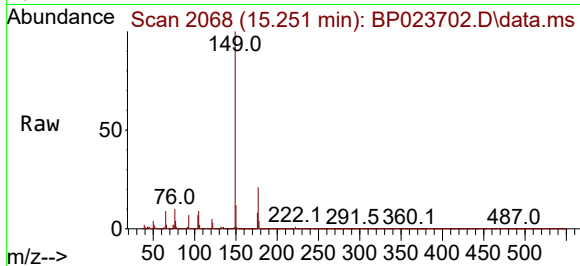

#61
Fluorene
Concen: 9.591 ng/ul
RT: 15.481 min Scan# 2107
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:166 Resp: 978148
Ion Ratio Lower Upper
166 100
165 97.5 77.8 116.8
167 13.5 10.6 16.0




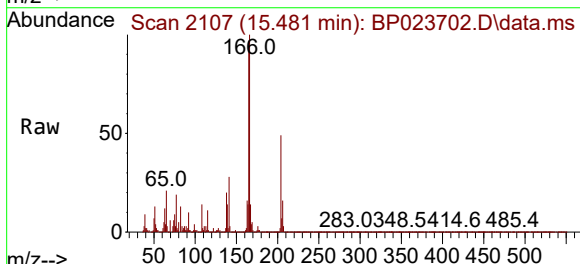




#62
4-Chlorophenyl-phenylether
Concen: 9.547 ng/ul
RT: 15.481 min Scan# 2107
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:204 Resp: 476561
Ion Ratio Lower Upper
204 100
206 32.6 26.2 39.2
141 57.6 45.4 68.2

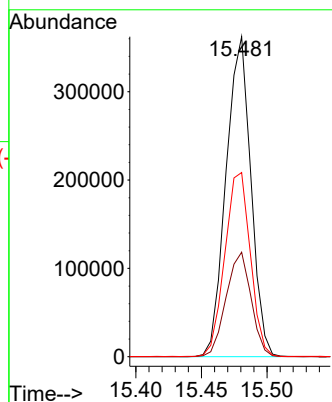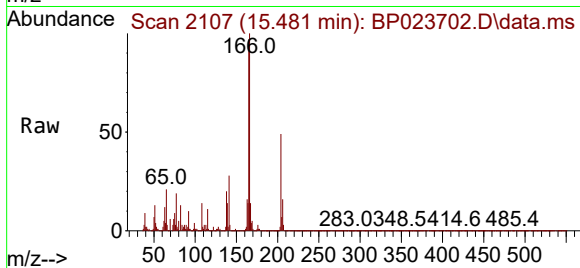

#63
4-Nitroaniline
Concen: 9.290 ng/ul
RT: 15.481 min Scan# 2107
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:138 Resp: 198085
Ion Ratio Lower Upper
138 100
92 48.6 37.0 55.4
108 72.1 54.4 81.6




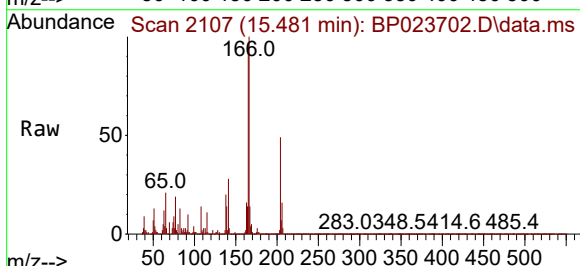




#66
4,6-Dinitro-2-methylphenol
Concen: 6.431 ng/ul
RT: 15.545 min Scan# 2118
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:198 Resp: 98115
Ion Ratio Lower Upper
198 100
182 5.6 3.9 5.9
77 26.7 20.3 30.5

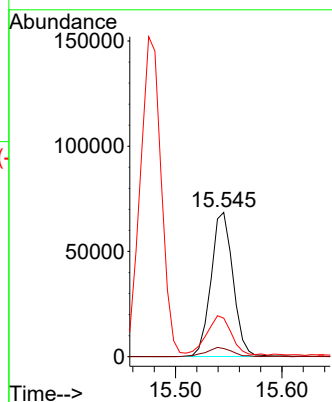

#67
N-Nitrosodiphenylamine
Concen: 9.484 ng/ul
RT: 15.692 min Scan# 2143
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:169 Resp: 784671
Ion Ratio Lower Upper
169 100
168 67.4 53.6 80.4
167 36.6 29.2 43.8









#68
4-Bromophenyl-phenylether
Concen: 9.216 ng/ul
RT: 16.386 min Scan# 211
Delta R.T. 0.000 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10




Instrument :
BNA_P
ClientSampleId :
SSTD010610


Tgt Ion:248 Resp: 271826
Ion Ratio Lower Upper
248 100
250 97.9 77.7 116.5
141 71.2 55.0 82.6



#69
Hexachlorobenzene
Concen: 9.420 ng/ul
RT: 16.498 min Scan# 2280
Delta R.T. -0.006 min
Lab File: BP023702.D
Acq: 22 Jan 2025 14:10

Tgt Ion:284 Resp: 338094
Ion Ratio Lower Upper
284 100
142 33.2 28.1 42.1
249 28.1 23.8 35.8





#70

Atrazine

Concen: 8.589 ng/ul

RT: 16.663 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:200 Resp: 262118

Ion Ratio Lower Upper

200 100

173 27.4 21.8 32.6

215 50.4 39.3 58.9

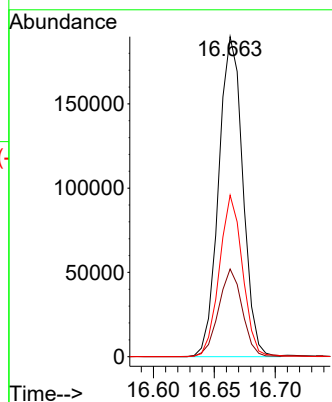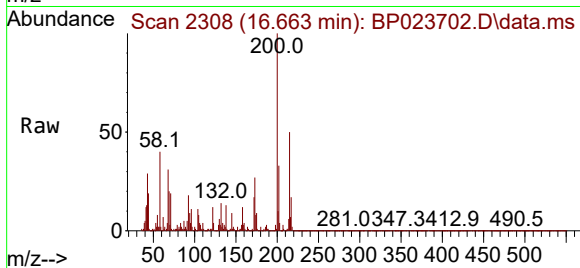

#71

Pentachlorophenol

Concen: 7.332 ng/ul

RT: 16.851 min Scan# 2340

Delta R.T. 0.000 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion:266 Resp: 158948


Ion Ratio Lower Upper

266 100

264 61.0 50.9 76.3

268 63.9 52.2 78.4

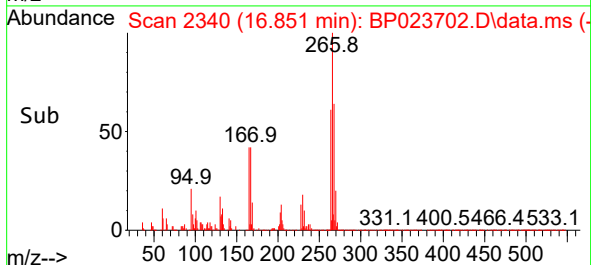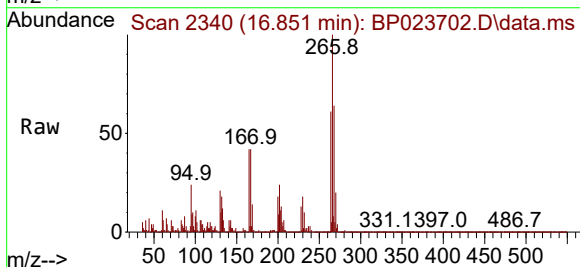



#72

Phenanthrene

Concen: 9.658 ng/ul

RT: 17.257 min Scan# 2409

Delta R.T. 0.006 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:178 Resp: 1503138

Ion Ratio Lower Upper

178 100

179 15.4 12.5 18.7

176 19.1 15.7 23.5

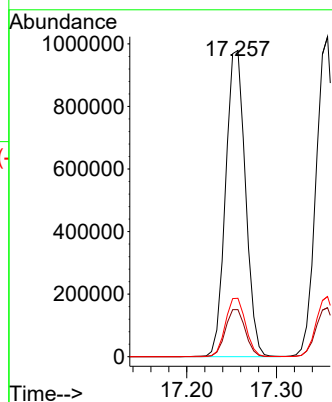

#74

Anthracene

Concen: 9.793 ng/ul

RT: 17.357 min Scan# 2426

Delta R.T. 0.012 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion:178 Resp: 1513991


Ion Ratio Lower Upper

178 100

179 15.3 12.4 18.6

176 18.8 15.0 22.6



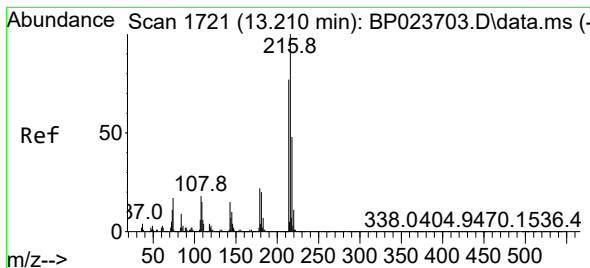

#75

1,2,3,4-Tetrachlorobenzene

Concen: 9.562 ng/uL

RT: 13.204 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:216 Resp: 382168

Ion Ratio Lower Upper

216 100

214 80.3 61.5 92.3

218 48.4 38.4 57.6

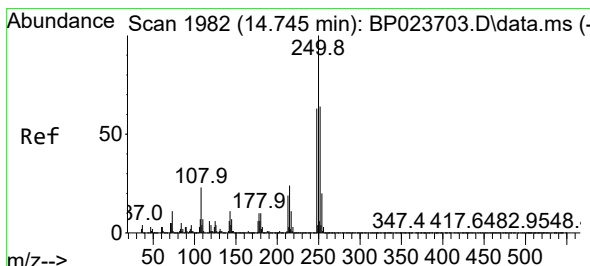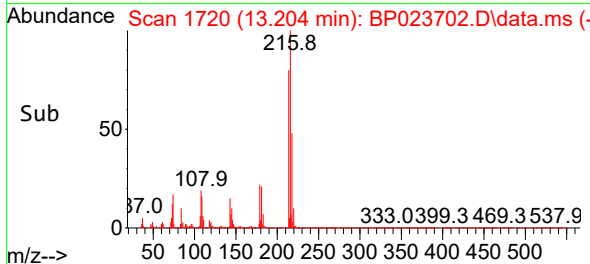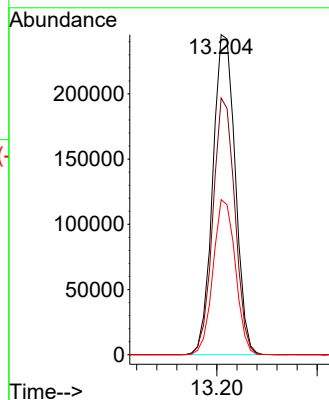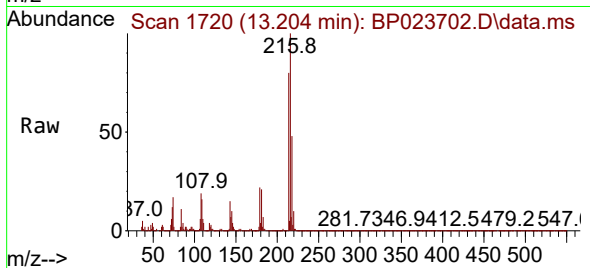

#76

Pentachlorobenzene

Concen: 9.515 ng/uL

RT: 14.740 min Scan# 1981

Delta R.T. -0.006 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion:250 Resp: 403949


Ion Ratio Lower Upper

250 100

248 62.0 50.2 75.2

252 64.5 51.0 76.6

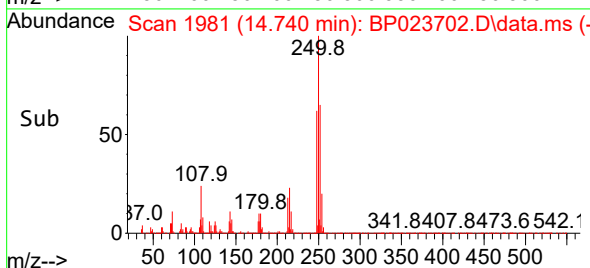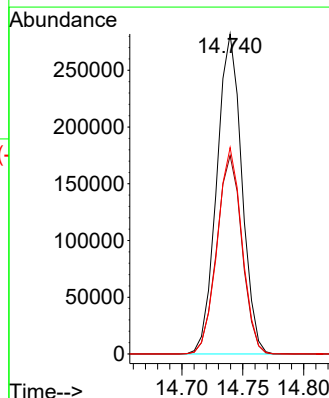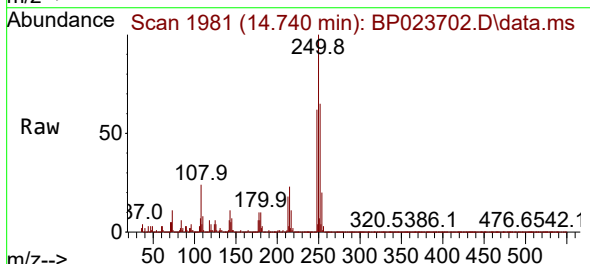




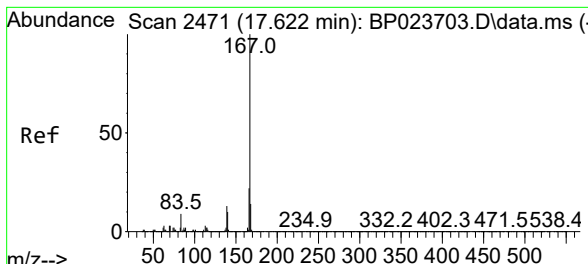


#77
 Carbazole
 Concen: 9.940 ng/ul
 RT: 17.628 min Scan# 2471
 Delta R.T. 0.006 min
 Lab File: BP023702.D
 Acq: 22 Jan 2025 14:10

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010610

Tgt Ion:167 Resp: 1348975




Ion	Ratio	Lower	Upper
167	100		
166	21.6	17.4	26.0
139	13.0	10.6	15.8

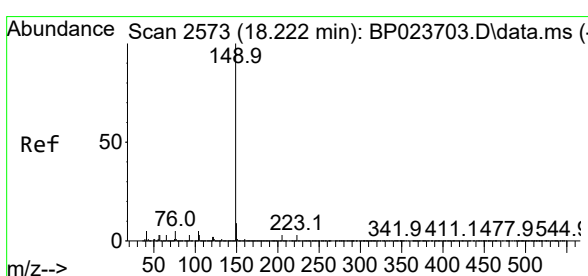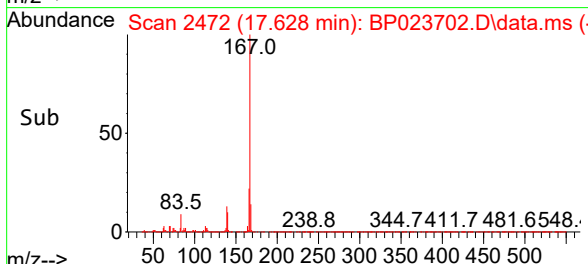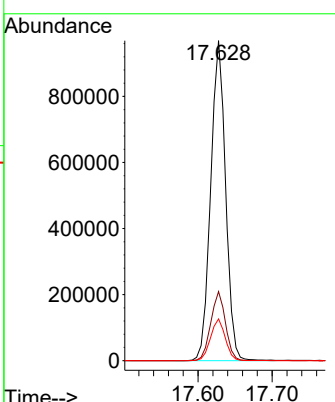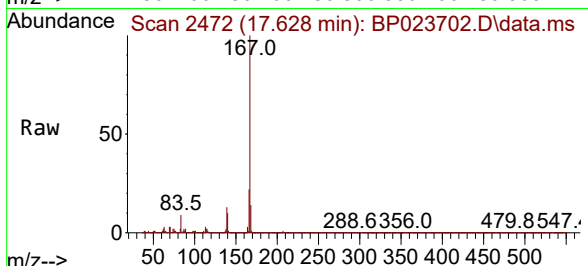


#78
 Di-n-butylphthalate
 Concen: 9.238 ng/ul
 RT: 18.228 min Scan# 2574
 Delta R.T. 0.006 min
 Lab File: BP023702.D
 Acq: 22 Jan 2025 14:10

Tgt Ion:149 Resp: 1427394

Ion	Ratio	Lower	Upper
149	100		
150	9.0	7.5	11.3
104	5.4	4.2	6.2

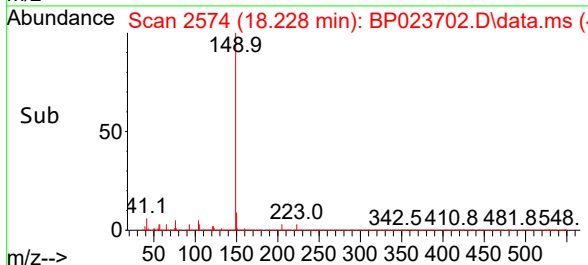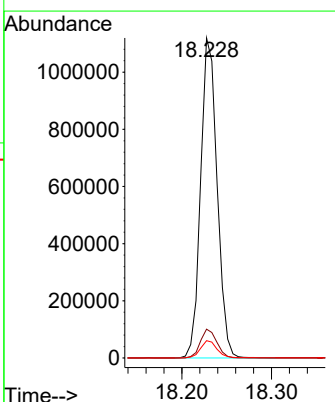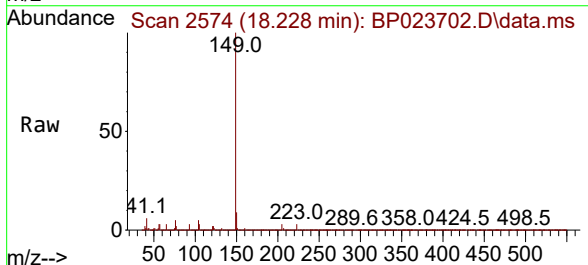



#80

Fluoranthene

Concen: 9.767 ng/ul

RT: 19.345 min Scan# 21

Delta R.T. 0.012 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:202 Resp: 1655716

Ion Ratio Lower Upper

202 100

101 12.1 9.2 13.8

100 9.2 7.0 10.6

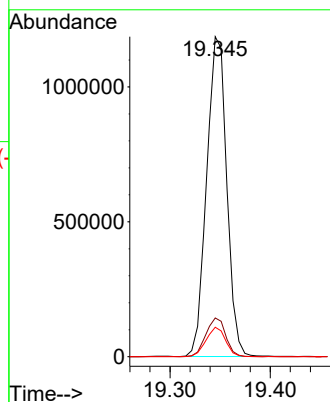

#82

Pyrene

Concen: 9.896 ng/ul

RT: 19.722 min Scan# 2828

Delta R.T. 0.018 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion:202 Resp: 1822099


Ion Ratio Lower Upper

202 100

101 13.9 11.6 17.4

100 11.6 9.6 14.4





#83

Butylbenzylphthalate

Concen: 8.335 ng/ul

RT: 20.680 min Scan# 2991

Delta R.T. 0.018 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:149 Resp: 553487

Ion Ratio Lower Upper

149 100

91 67.4 56.6 84.8

206 21.0 16.3 24.5

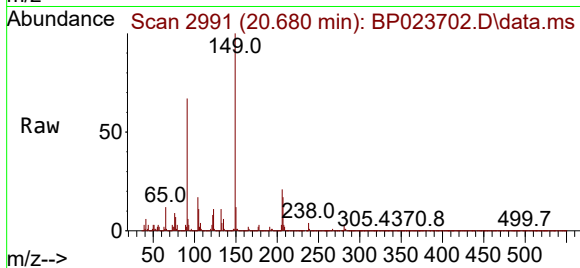

#84

3,3'-Dichlorobenzidine

Concen: 7.946 ng/ul

RT: 21.563 min Scan# 3141

Delta R.T. 0.012 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion:252 Resp: 410862


Ion Ratio Lower Upper

252 100

254 64.4 52.1 78.1

126 11.6 9.4 14.0

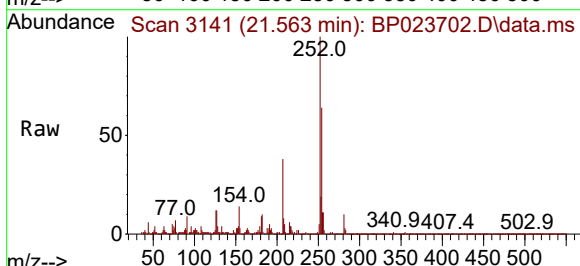

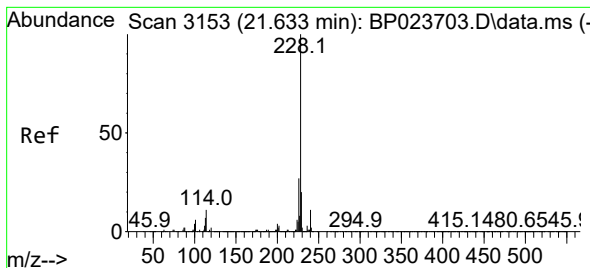

#85

Benzo(a)anthracene

Concen: 9.663 ng/ul

RT: 21.651 min Scan# 3153

Delta R.T. 0.018 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:228 Resp: 1794894

Ion Ratio Lower Upper

228 100

229 19.5 15.8 23.8

226 27.2 21.8 32.8

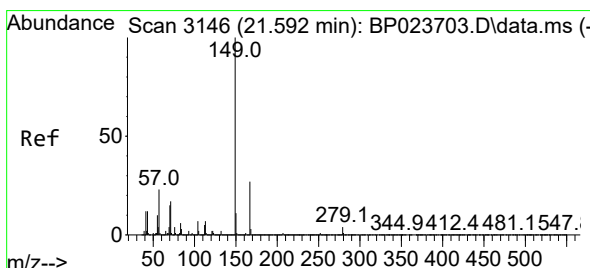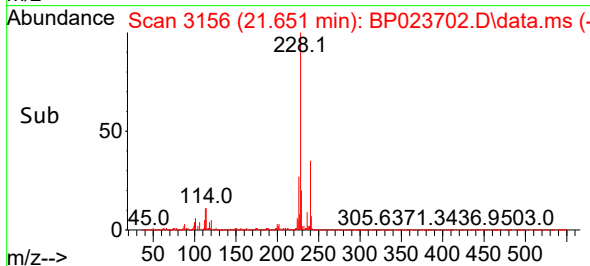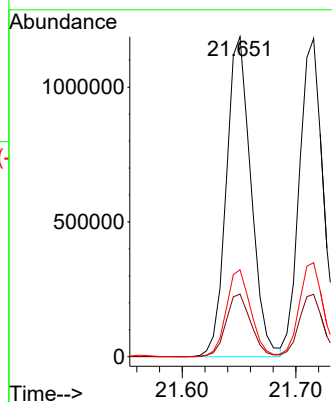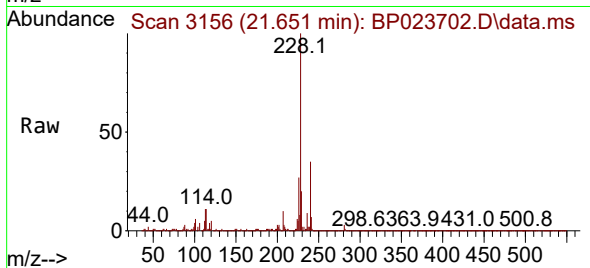

#86

Bis(2-ethylhexyl)phthalate

Concen: 8.388 ng/ul

RT: 21.610 min Scan# 3149

Delta R.T. 0.018 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion:149 Resp: 830592


Ion Ratio Lower Upper

149 100

167 27.2 21.7 32.5

279 4.3 3.4 5.2

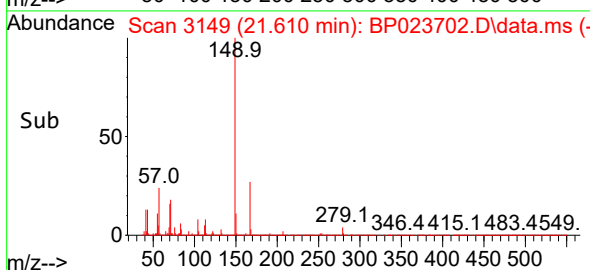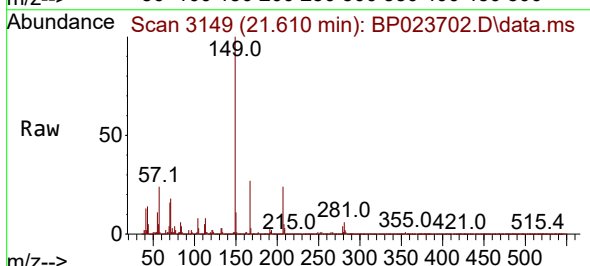



#87

Chrysene

Concen: 9.823 ng/ul

RT: 21.716 min Scan# 3164

Delta R.T. 0.018 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:228 Resp: 1708227

Ion Ratio Lower Upper

228 100

226 29.6 24.3 36.5

229 19.6 15.8 23.6



#89

Di-n-octyl phthalate

Concen: 7.534 ng/ul




RT: 22.916 min Scan# 3371


Delta R.T. 0.018 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Tgt Ion:149 Resp: 1125903

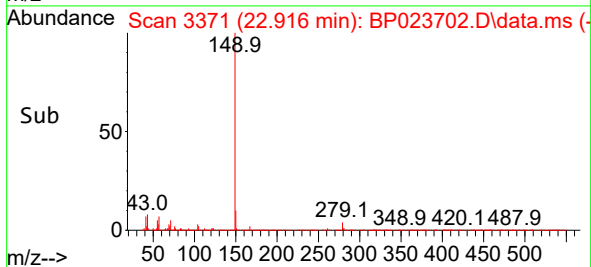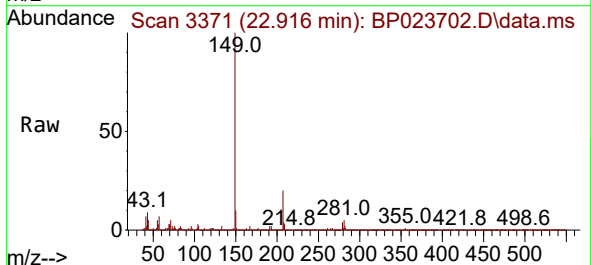



#90

Benzo(b)fluoranthene

Concen: 9.024 ng/ul

RT: 23.980 min Scan# 3552

Delta R.T. 0.006 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:252 Resp: 1599052

Ion Ratio Lower Upper

252 100

253 21.5 17.5 26.3

125 10.4 8.2 12.4

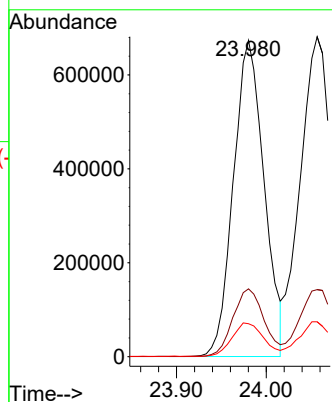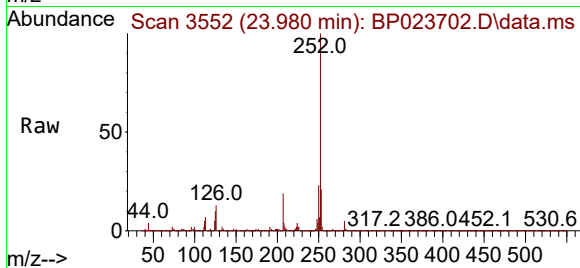

#91

Benzo(k)fluoranthene

Concen: 9.283 ng/ul

RT: 24.057 min Scan# 3565

Delta R.T. 0.018 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion:252 Resp: 1695769


Ion Ratio Lower Upper

252 100

253 21.0 17.7 26.5

125 10.9 8.6 13.0

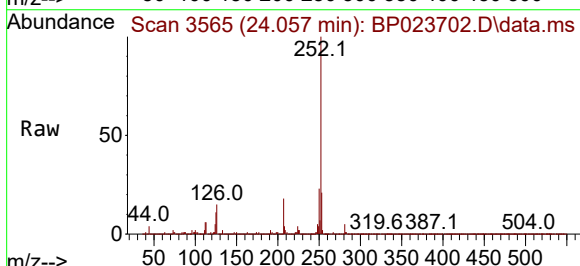



#93

Benzo(a)pyrene

Concen: 9.090 ng/ul

RT: 24.892 min Scan# 31

Delta R.T. 0.012 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10

Instrument :

BNA_P

ClientSampleId :

SSTD010610





Tgt Ion:252 Resp: 1516105

Ion Ratio Lower Upper

252 100

253 22.2 17.5 26.3

125 11.9 9.1 13.7

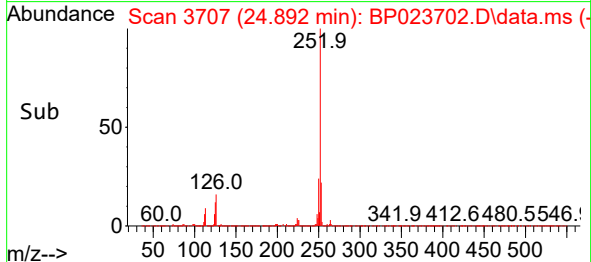

#94

Indeno(1,2,3-cd)pyrene

Concen: 7.509 ng/ul

RT: 28.903 min Scan# 4389

Delta R.T. 0.018 min

Lab File: BP023702.D

Acq: 22 Jan 2025 14:10




Tgt Ion:276 Resp: 1554212


Ion Ratio Lower Upper

276 100

138 20.5 16.6 25.0

277 24.1 19.2 28.8


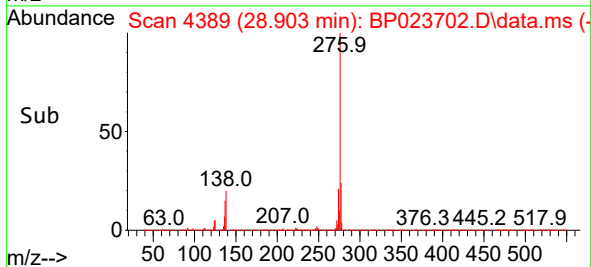

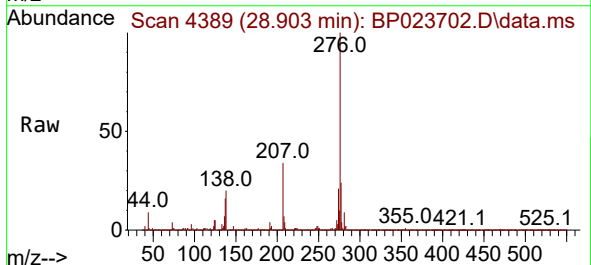




#95
 Dibenzo(a,h)anthracene
 Concen: 8.978 ng/ul
 RT: 28.986 min Scan# 4400
 Delta R.T. 0.018 min
 Lab File: BP023702.D
 Acq: 22 Jan 2025 14:10

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010610

Tgt Ion:278 Resp: 1508478
 Ion Ratio Lower Upper
 278 100
 139 15.9 13.4 20.2
 279 24.1 19.4 29.2



#96
 Benzo(g,h,i)perylene
 Concen: 3.599 ng/ul
 RT: 30.045 min Scan# 4583
 Delta R.T. -0.023 min
 Lab File: BP023702.D
 Acq: 22 Jan 2025 14:10

Tgt Ion:276 Resp: 573819
 Ion Ratio Lower Upper
 276 100
 138 23.6 18.5 27.7
 277 24.4 19.0 28.6

