

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
 Data File : BP019421.D
 Acq On : 23 Jan 2024 15:36
 Operator : MA/JU
 Sample : P1157-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB6

Quant Time: Jan 23 16:16:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 22 11:49:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	158374	20.000	ng/u1	0.00
20) Naphthalene-d8	10.563	136	609672	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.416	164	418259	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.169	188	846467	20.000	ng/u1	0.00
79) Chrysene-d12	21.274	240	624205	20.000	ng/u1	0.00
88) Perylene-d12	23.621	264	684467	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	0.000	99	0d	0.000	ng/u1	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0d	0.000	ng/u1	
11) 2-Chlorophenol-d4	0.000	132	0d	0.000	ng/u1	
15) 4-Methylphenol-d8	0.000	113	0d	0.000	ng/u1	
21) Nitrobenzene-d5	0.000	128	0d	0.000	ng/u1	
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.000	ng/u1	
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/u1	
46) Dimethylphthalate-d6	0.000	166	0d	0.000	ng/u1	
49) Acenaphthylene-d8	0.000	160	0d	0.000	ng/u1	
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	0.000	176	0d	0.000	ng/u1	
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	0.000	188	0d	0.000	ng/u1	
81) Pyrene-d10	0.000	212	0d	0.000	ng/u1	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/u1	
Target Compounds						
					Qvalue	
80) Fluoranthene	19.192	202	97096	2.018	ng/u1	99
87) Chrysene	21.310	228	71041	1.599	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
Data File : BP019421.D
Acq On : 23 Jan 2024 15:36
Operator : MA/JU
Sample : P1157-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Time: Jan 23 16:16:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jan 22 11:49:04 2024
Response via : Initial Calibration




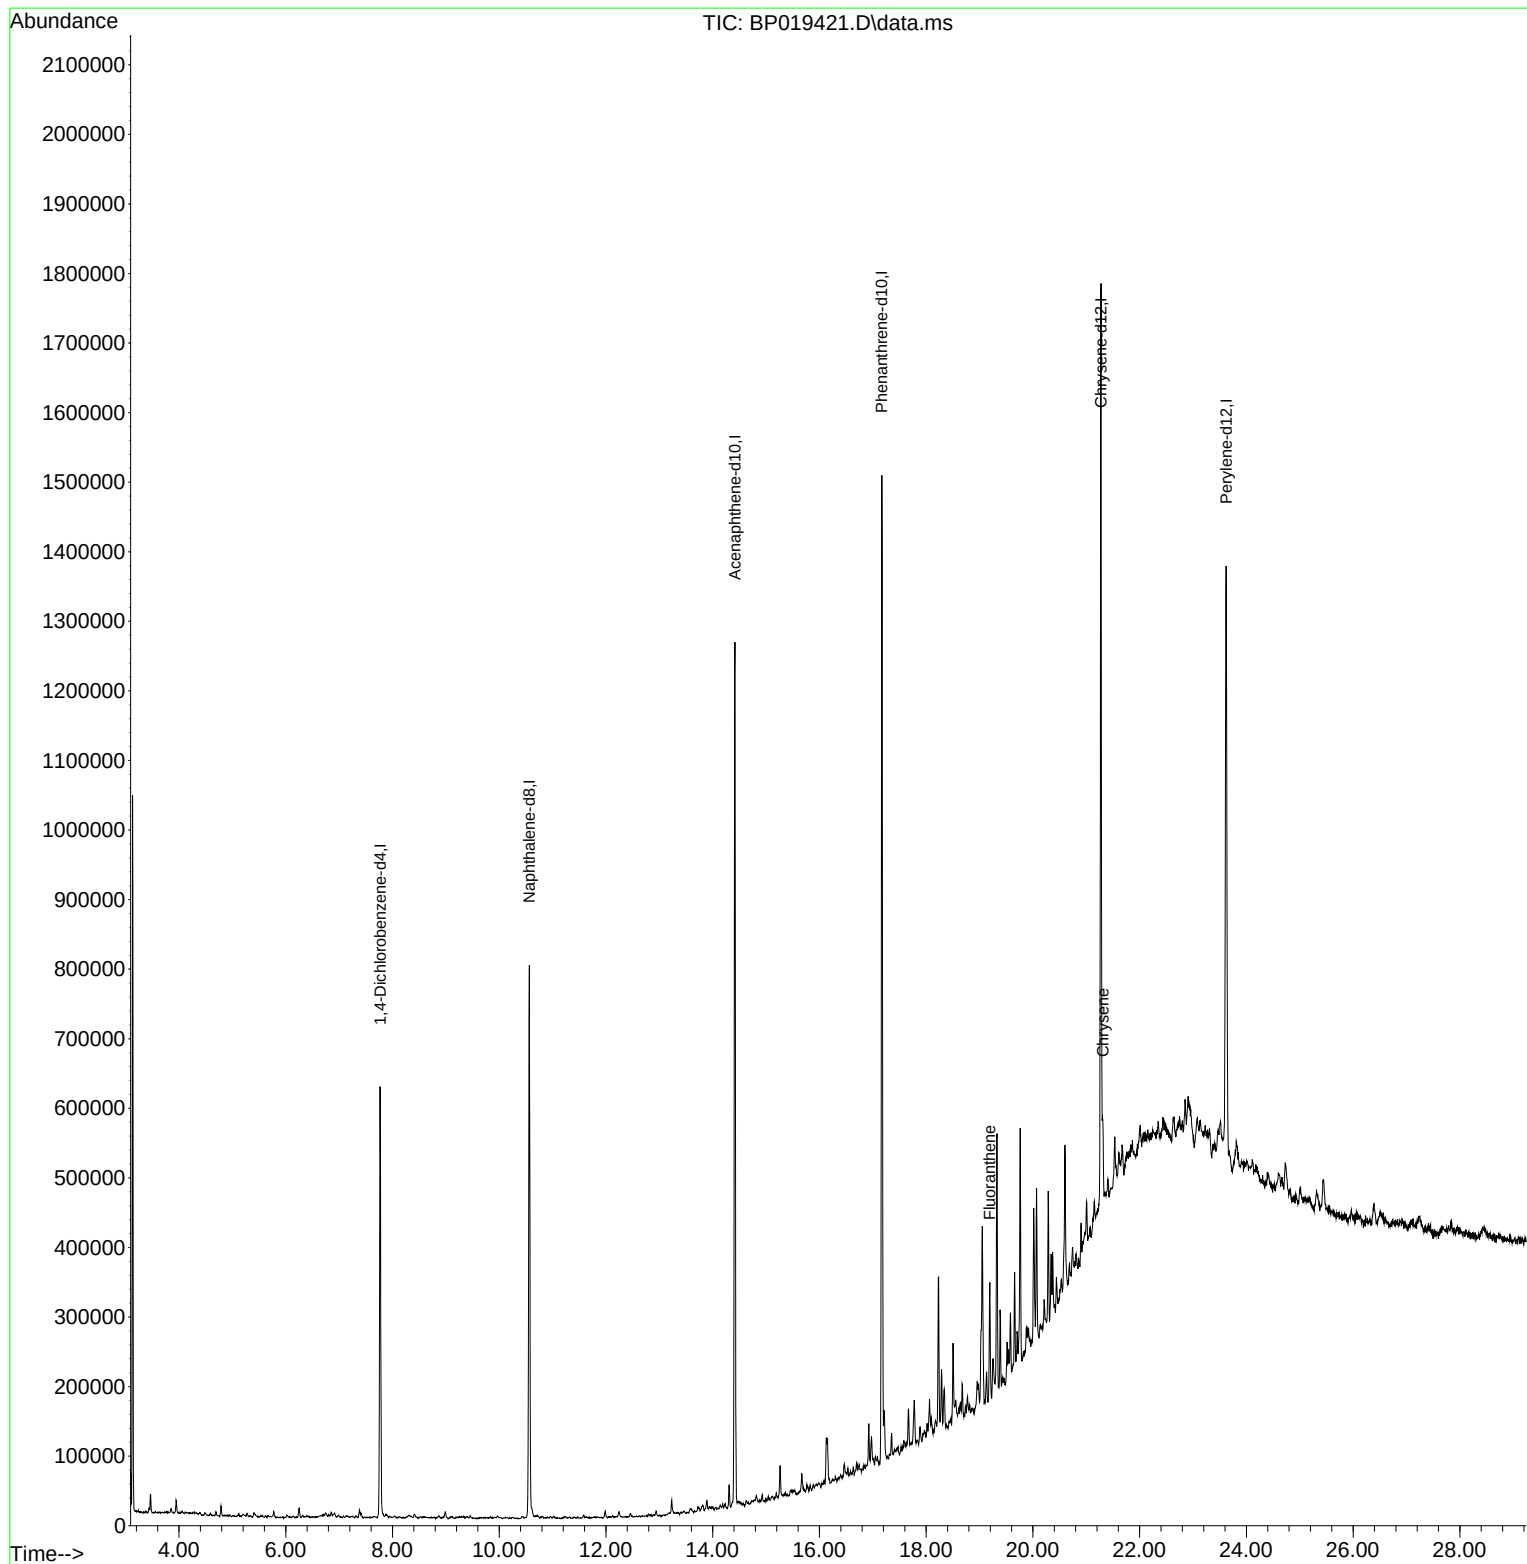


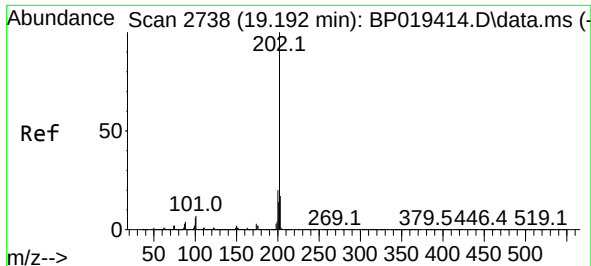

#80
Fluoranthene
Concen: 2.018 ng/ul
RT: 19.192 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP019421.D
Acq: 23 Jan 2024 15:36

Instrument :
BNA_P
ClientSampleId :
C0AB6

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.0	5.9	8.9
100	5.8	4.6	7.0

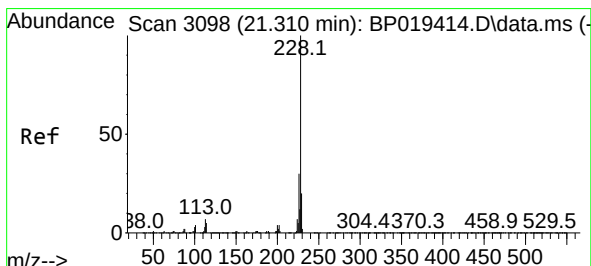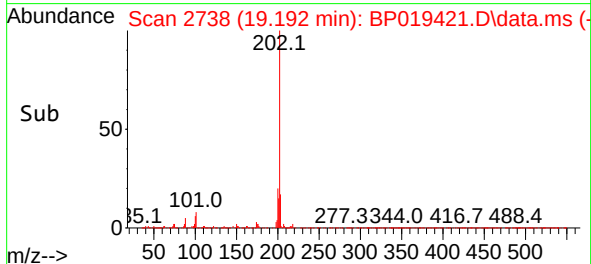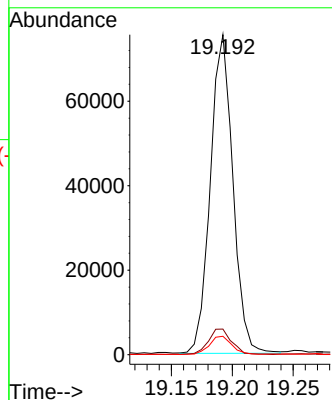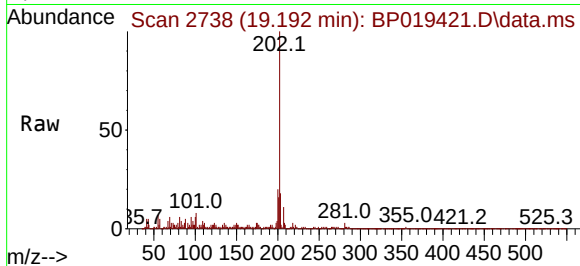

#87
Chrysene
Concen: 1.599 ng/ul
RT: 21.310 min Scan# 3098
Delta R.T. -0.006 min
Lab File: BP019421.D
Acq: 23 Jan 2024 15:36

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.3	23.9	35.9
229	22.0	15.5	23.3

