

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
 Data File : BP019417.D
 Acq On : 23 Jan 2024 13:20
 Operator : MA/JU
 Sample : PB158529BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK529

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	15	rVB	515009	523484	23.92%	4.884%
2	3.258	27	29	32	rBV3	8778	9994	0.46%	0.093%
3	3.434	57	59	61	rBV3	2267	2806	0.13%	0.026%
4	3.464	61	64	70	rVB4	11191	13619	0.62%	0.127%
5	3.946	142	146	151	rBV	10756	13624	0.62%	0.127%
6	4.093	168	171	177	rVB2	10973	14478	0.66%	0.135%
7	4.146	177	180	184	rBV	15194	19561	0.89%	0.182%
8	4.252	194	198	201	rBV2	12007	15027	0.69%	0.140%
9	4.293	201	205	211	rVB2	13190	17745	0.81%	0.166%
10	4.493	236	239	242	rVB5	2205	2985	0.14%	0.028%
11	4.893	304	307	311	rBV5	2708	3811	0.17%	0.036%
12	5.622	428	431	433	rVB4	1968	2268	0.10%	0.021%
13	6.387	557	561	562	rBV4	1880	2559	0.12%	0.024%
14	6.417	562	566	571	rVV2	5530	9179	0.42%	0.086%
15	6.569	586	592	596	rBV5	6015	10220	0.47%	0.095%
16	6.817	630	634	637	rBV5	1810	3197	0.15%	0.030%
17	7.769	787	796	812	rBV	602584	953955	43.59%	8.899%
18	10.563	1263	1271	1292	rBV	726370	1234326	56.40%	11.515%
19	11.310	1394	1398	1403	rVB7	1689	3051	0.14%	0.028%
20	11.804	1479	1482	1486	rBV6	1651	2831	0.13%	0.026%
21	14.416	1918	1926	1943	rBV	1245115	1842191	84.17%	17.186%
22	15.251	2065	2068	2070	rBV4	1966	2947	0.13%	0.027%
23	15.375	2085	2089	2093	rBV6	1783	2850	0.13%	0.027%
24	15.428	2093	2098	2103	rBV8	2023	3922	0.18%	0.037%
25	15.545	2114	2118	2121	rBV6	1882	2973	0.14%	0.028%
26	15.781	2155	2158	2160	rBV3	2695	3213	0.15%	0.030%
27	16.634	2298	2303	2309	rVB9	1894	3815	0.17%	0.036%
28	16.963	2351	2359	2364	rBV4	3517	8568	0.39%	0.080%
29	17.169	2388	2394	2409	rBV	1425354	2188569	100.00%	20.417%
30	17.469	2441	2445	2446	rBV4	2103	2864	0.13%	0.027%
31	17.710	2482	2486	2490	rBV7	2345	2901	0.13%	0.027%
32	18.069	2544	2547	2552	rBV6	11503	16952	0.77%	0.158%
33	18.292	2583	2585	2590	rBV5	3024	2860	0.13%	0.027%
34	19.304	2754	2757	2766	rBV10	8278	17123	0.78%	0.160%
35	21.275	3087	3092	3102	rVB	1516326	1935670	88.44%	18.058%
36	23.622	3484	3491	3502	rVB	887440	1823169	83.30%	17.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
Data File : BP019417.D
Acq On : 23 Jan 2024 13:20
Operator : MA/JU
Sample : PB158529BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK529

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 10719307

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
Data File : BP019417.D
Acq On : 23 Jan 2024 13:20
Operator : MA/JU
Sample : PB158529BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK529

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

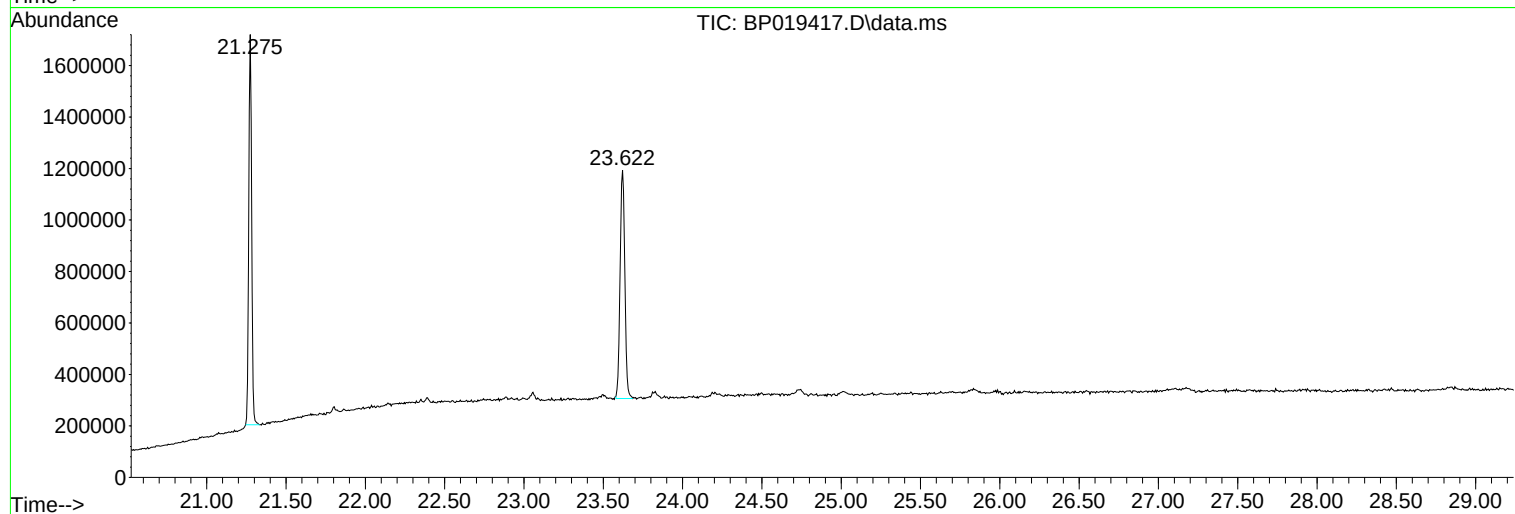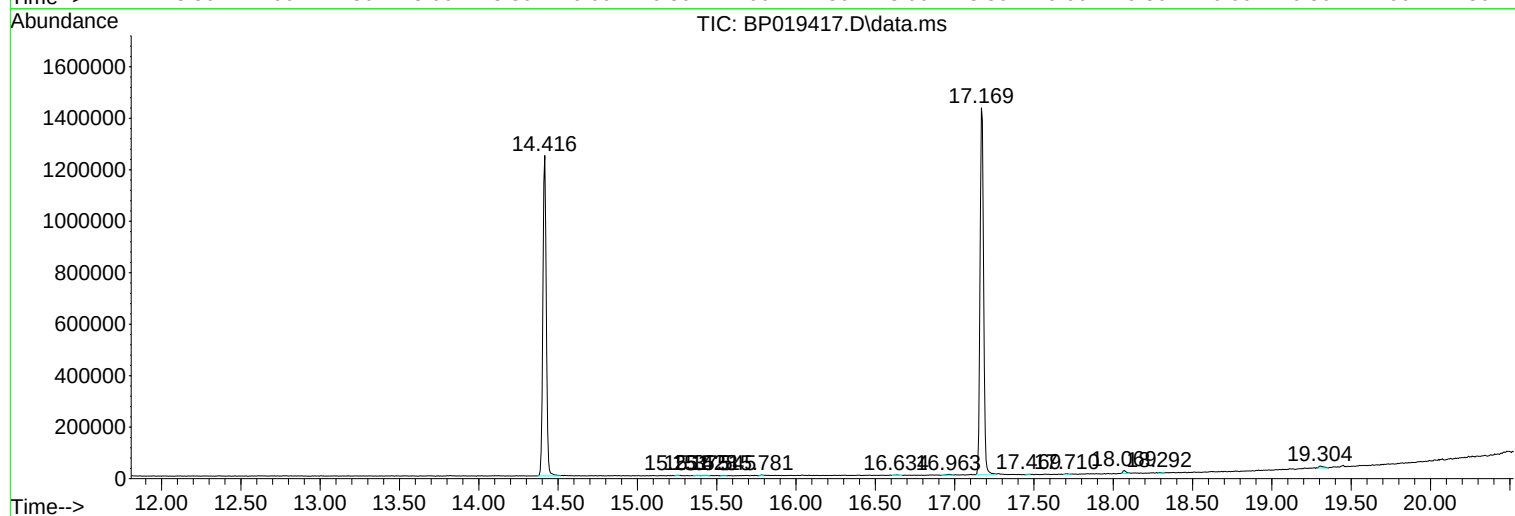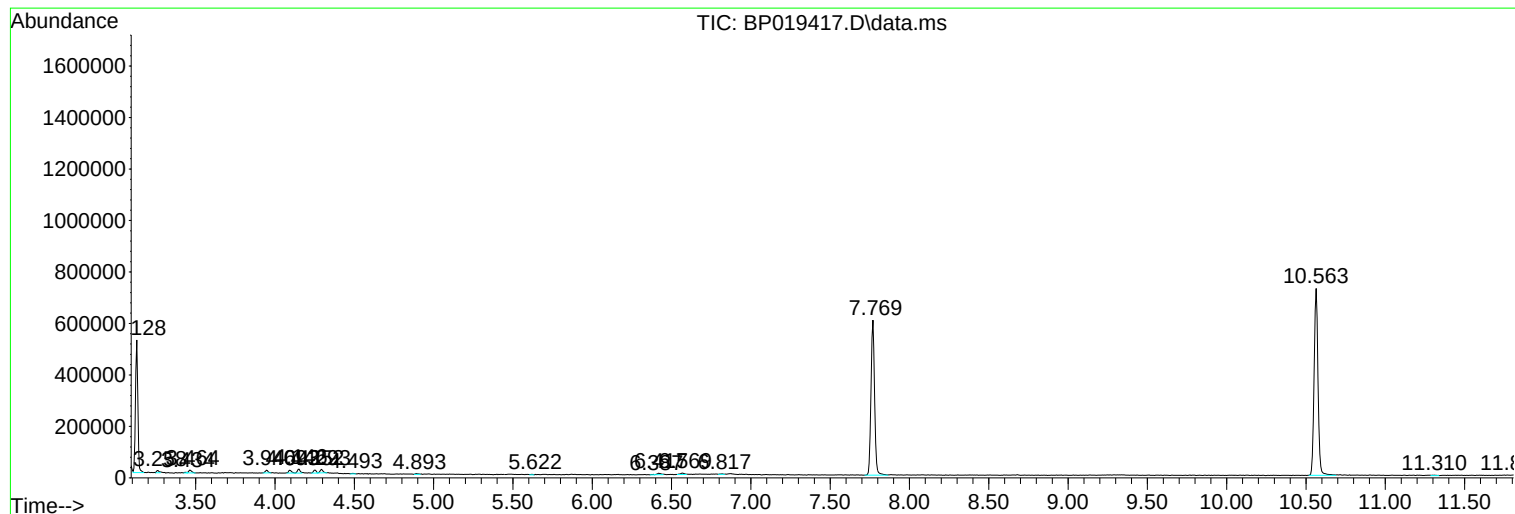

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
Data File : BP019417.D
Acq On : 23 Jan 2024 13:20
Operator : MA/JU
Sample : PB158529BL
Misc :
ALS Vial : 5 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
SBLK529

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
3.128	10.98 ng/ul	523484	1,4-Dichlorobenzene-d4		7.769	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Heptane		100	C7H16	000142-82-5	91
2	Heptane		100	C7H16	000142-82-5	90
3	Heptane		100	C7H16	000142-82-5	87
4	Heptane		100	C7H16	000142-82-5	86
5	Hexane, 3-methyl-		100	C7H16	000589-34-4	43

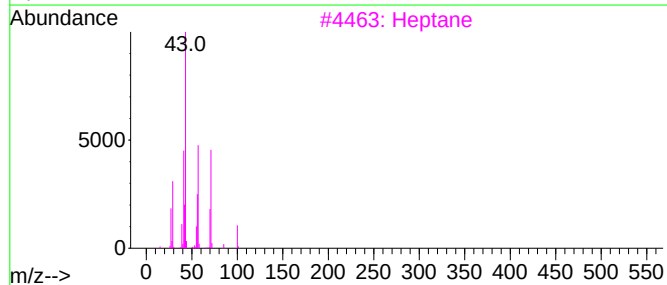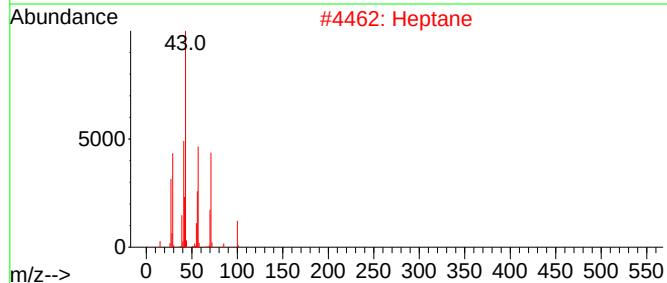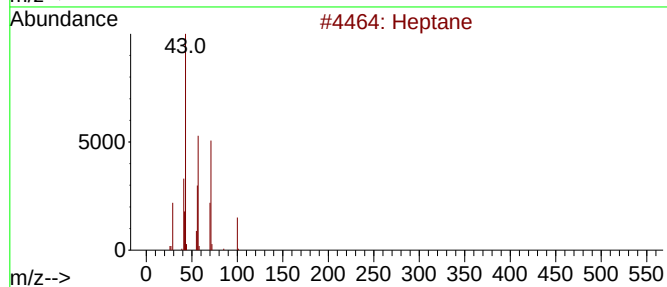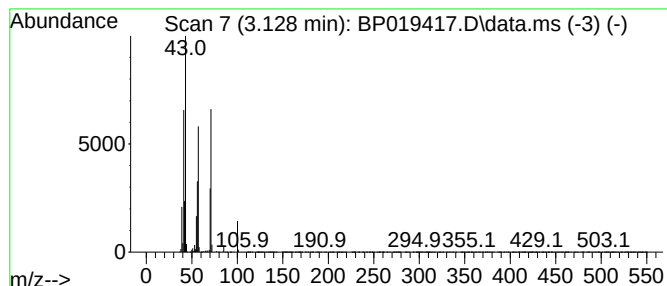

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
Data File : BP019417.D
Acq On : 23 Jan 2024 13:20
Operator : MA/JU
Sample : PB158529BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK529

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.128	11.0	ng/u1	523484	1	7.769	953955	20.0