

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
 Data File : BP019425.D
 Acq On : 23 Jan 2024 17:52
 Operator : MA/JU
 Sample : P1157-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	4	8	12	rVB	1021808	1060850	46.29%	6.250%
2	3.434	55	59	61	rBV5	4287	6029	0.26%	0.036%
3	3.469	61	65	69	rVB	24808	29810	1.30%	0.176%
4	3.946	142	146	152	rVB	12736	18573	0.81%	0.109%
5	4.387	220	221	230	rVB5	6735	8719	0.38%	0.051%
6	4.481	234	237	241	rBV6	2621	4276	0.19%	0.025%
7	4.587	253	255	260	rVV6	3416	4337	0.19%	0.026%
8	4.699	267	274	281	rVV9	4959	11511	0.50%	0.068%
9	4.787	285	289	295	rVB	10424	14540	0.63%	0.086%
10	5.275	368	372	377	rVB8	2857	4717	0.21%	0.028%
11	5.405	388	394	400	rBV8	3826	9536	0.42%	0.056%
12	5.769	453	456	463	rVB3	4873	6920	0.30%	0.041%
13	6.022	495	499	503	rVB7	2143	3700	0.16%	0.022%
14	6.252	530	538	544	rVB2	8475	14440	0.63%	0.085%
15	6.316	544	549	551	rBV6	2070	3302	0.14%	0.019%
16	6.852	637	640	643	rBV5	2567	3553	0.16%	0.021%
17	6.893	643	647	652	rVB7	2262	4897	0.21%	0.029%
18	6.987	660	663	669	rVB8	3231	4529	0.20%	0.027%
19	7.410	730	735	740	rVB4	4500	6812	0.30%	0.040%
20	7.769	787	796	806	rBV	654747	1040728	45.41%	6.131%
21	7.881	811	815	820	rVB8	2924	6040	0.26%	0.036%
22	8.134	854	858	859	rBV4	2879	3278	0.14%	0.019%
23	8.287	881	884	886	rBV4	2153	2699	0.12%	0.016%
24	8.722	955	958	961	rBV5	1517	2734	0.12%	0.016%
25	9.122	1020	1026	1027	rBV6	1544	2459	0.11%	0.014%
26	9.393	1070	1072	1076	rBV5	2281	2888	0.13%	0.017%
27	9.969	1164	1170	1171	rBV4	2065	2400	0.10%	0.014%
28	10.234	1210	1215	1218	rBV6	1938	2642	0.12%	0.016%
29	10.563	1262	1271	1286	rBV	827694	1423028	62.09%	8.383%
30	10.669	1286	1289	1291	rBV3	2086	2559	0.11%	0.015%
31	10.946	1334	1336	1338	rBV3	2119	2425	0.11%	0.014%
32	11.822	1483	1485	1489	rVB4	1845	2418	0.11%	0.014%
33	12.240	1553	1556	1564	rVB8	3415	6660	0.29%	0.039%
34	12.457	1590	1593	1599	rVB7	3773	6222	0.27%	0.037%
35	13.251	1722	1728	1729	rBV6	2675	5191	0.23%	0.031%
36	13.581	1776	1784	1785	rBV7	3894	5959	0.26%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
 Data File : BP019425.D
 Acq On : 23 Jan 2024 17:52
 Operator : MA/JU
 Sample : P1157-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

37	13.740	1807	1811	1817	rBV8	5384	8897	0.39%	0.052%
38	13.804	1817	1822	1823	rBV5	3008	4685	0.20%	0.028%
39	13.975	1848	1851	1856	rVB6	1590	2524	0.11%	0.015%
40	14.134	1874	1878	1881	rBV5	3423	5004	0.22%	0.029%

41	14.234	1892	1895	1899	rVB5	2798	2897	0.13%	0.017%
42	14.410	1919	1925	1933	rBV	1343199	2008956	87.66%	11.835%
43	14.475	1933	1936	1941	rVB2	11249	17665	0.77%	0.104%
44	14.539	1946	1947	1955	rVB8	3054	4468	0.19%	0.026%
45	14.722	1973	1978	1983	rBV9	3504	6858	0.30%	0.040%

46	14.822	1987	1995	2002	rVV	20338	36934	1.61%	0.218%
47	14.892	2005	2007	2011	rVB5	2760	3811	0.17%	0.022%
48	15.045	2027	2033	2036	rBV7	3881	6321	0.28%	0.037%
49	15.198	2054	2059	2064	rBV9	3999	8733	0.38%	0.051%
50	15.257	2064	2069	2074	rBV9	4272	8379	0.37%	0.049%

51	15.469	2100	2105	2109	rBV	21398	32718	1.43%	0.193%
52	15.545	2116	2118	2121	rVB4	2323	2503	0.11%	0.015%
53	15.592	2121	2126	2127	rBV5	2789	3850	0.17%	0.023%
54	15.628	2129	2132	2136	rVV5	4446	7416	0.32%	0.044%
55	15.675	2136	2140	2144	rVB3	19940	29138	1.27%	0.172%

56	15.769	2151	2156	2162	rVB3	8044	16704	0.73%	0.098%
57	15.916	2178	2181	2182	rBV3	4927	5329	0.23%	0.031%
58	16.128	2215	2217	2219	rBV3	3699	3831	0.17%	0.023%
59	16.233	2232	2235	2236	rBV3	3233	3794	0.17%	0.022%
60	16.404	2261	2264	2269	rVB6	6338	8710	0.38%	0.051%

61	16.481	2272	2277	2280	rBV7	6763	10684	0.47%	0.063%
62	16.704	2310	2315	2319	rBV6	14224	24783	1.08%	0.146%
63	16.922	2349	2352	2356	rVB6	7973	11222	0.49%	0.066%
64	16.992	2360	2364	2369	rVB	12407	20586	0.90%	0.121%
65	17.045	2369	2373	2377	rBV2	33011	47370	2.07%	0.279%

66	17.081	2377	2379	2386	rVB5	17945	26100	1.14%	0.154%
67	17.169	2388	2394	2398	rBV	1655481	2291877	100.00%	13.502%
68	17.210	2398	2401	2412	rVB	295207	412511	18.00%	2.430%
69	17.345	2421	2424	2430	rVB2	40184	55317	2.41%	0.326%
70	17.628	2469	2472	2475	rBV4	10497	13458	0.59%	0.079%

71	17.775	2490	2497	2506	rBV3	97054	192727	8.41%	1.135%
72	17.892	2512	2517	2522	rVB5	25882	42986	1.88%	0.253%
73	18.016	2535	2538	2540	rBV2	29242	37831	1.65%	0.223%
74	18.045	2540	2543	2545	rVV	35149	51447	2.24%	0.303%
75	18.092	2548	2551	2558	rVB	44360	66989	2.92%	0.395%

76	18.228	2570	2574	2578	rBV2	155776	214414	9.36%	1.263%
----	--------	------	------	------	------	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
 Data File : BP019425.D
 Acq On : 23 Jan 2024 17:52
 Operator : MA/JU
 Sample : P1157-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

77	18.286	2578	2584	2588	rVV3	63027	116823	5.10%	0.688%
78	18.328	2588	2591	2597	rVB5	30987	45981	2.01%	0.271%
79	18.433	2605	2609	2616	rVB2	61905	84936	3.71%	0.500%
80	18.504	2617	2621	2624	rBV	74498	97458	4.25%	0.574%
81	18.610	2635	2639	2643	rBV	97978	125648	5.48%	0.740%
82	18.675	2647	2650	2656	rVB	36735	47075	2.05%	0.277%
83	18.757	2660	2664	2670	rVV2	77761	107709	4.70%	0.635%
84	18.980	2699	2702	2706	rBV4	31764	38954	1.70%	0.229%
85	19.027	2706	2710	2711	rVV2	75975	81802	3.57%	0.482%
86	19.051	2711	2714	2721	rVB4	105258	183560	8.01%	1.081%
87	19.186	2732	2737	2743	rBV	586325	807349	35.23%	4.756%
88	19.251	2744	2748	2753	rVV7	39682	99512	4.34%	0.586%
89	19.327	2757	2761	2765	rVV	135733	182550	7.97%	1.075%
90	19.386	2768	2771	2775	rVV5	43176	55216	2.41%	0.325%
91	19.516	2789	2793	2794	rBV	88335	108640	4.74%	0.640%
92	19.545	2794	2798	2802	rVB	240641	326866	14.26%	1.926%
93	19.657	2814	2817	2821	rVB5	43494	50577	2.21%	0.298%
94	19.763	2832	2835	2841	rVB	118066	144993	6.33%	0.854%
95	20.022	2875	2879	2884	rVB2	81850	152744	6.66%	0.900%
96	20.069	2884	2887	2892	rVB2	80203	92069	4.02%	0.542%
97	20.286	2922	2924	2928	rVB4	54210	53311	2.33%	0.314%
98	21.274	3085	3092	3096	rBV2	1485125	2269839	99.04%	13.372%
99	21.310	3096	3098	3108	rVB	260006	325606	14.21%	1.918%
100	23.615	3485	3490	3501	rVB	942383	1873317	81.74%	11.036%


Sum of corrected areas: 16974343

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
Data File : BP019425.D
Acq On : 23 Jan 2024 17:52
Operator : MA/JU
Sample : P1157-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

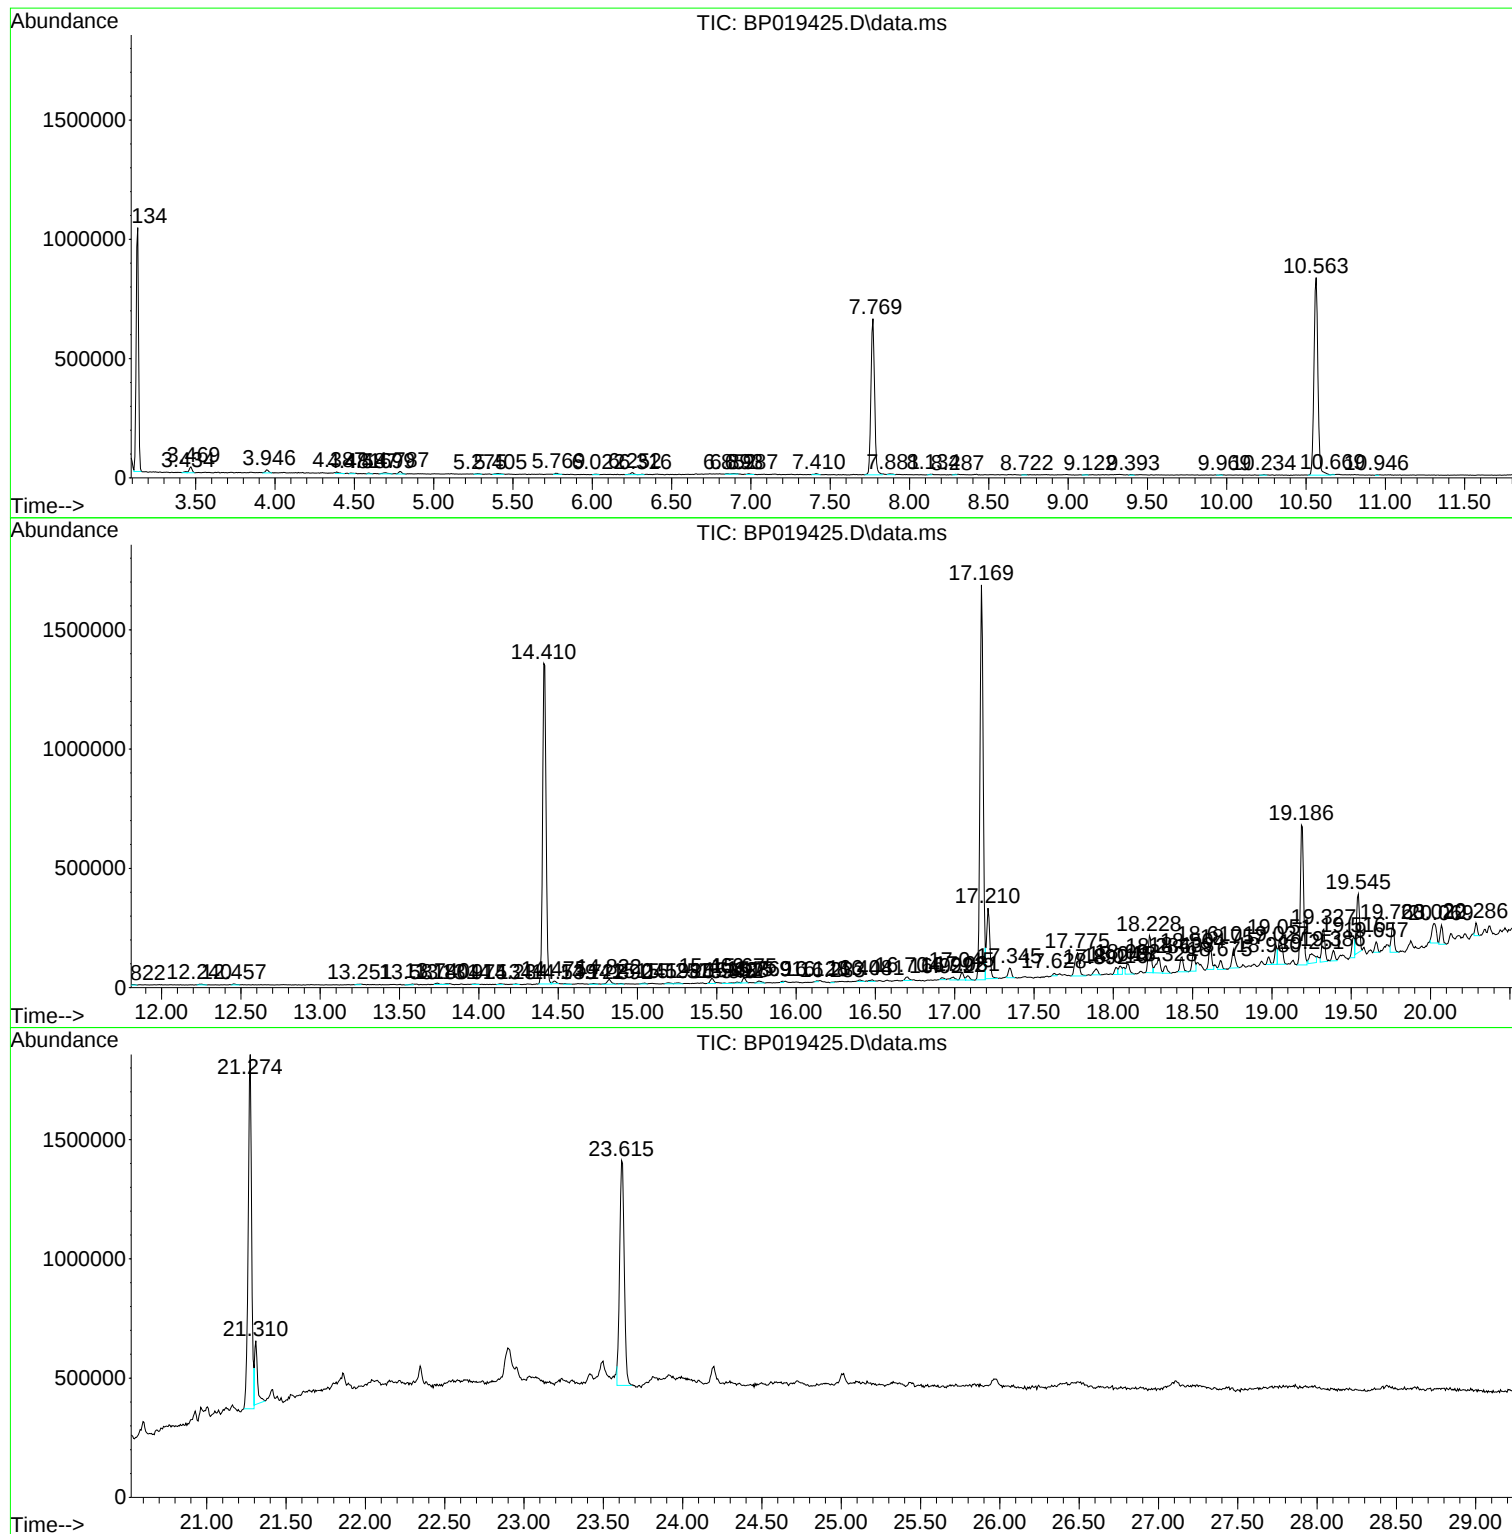

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
Data File : BP019425.D
Acq On : 23 Jan 2024 17:52
Operator : MA/JU
Sample : P1157-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.134	20.39 ng/ul	1060850	1,4-Dichlorobenzene-d4	7.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	91
2			Heptane	100	C7H16	000142-82-5	91
3			Heptane	100	C7H16	000142-82-5	90
4			Heptane	100	C7H16	000142-82-5	87
5			Hexane, 3-methyl-	100	C7H16	000589-34-4	50

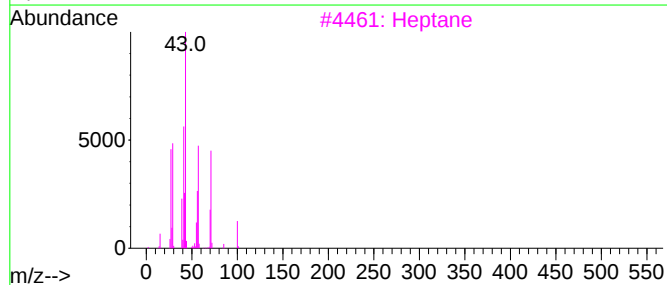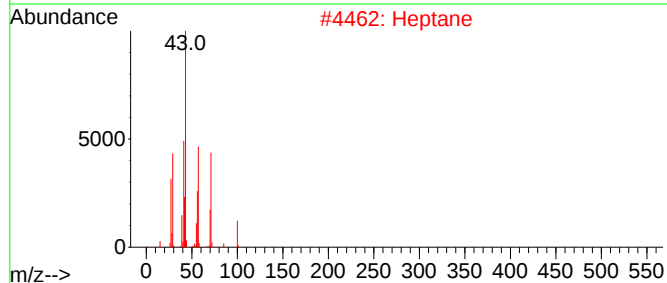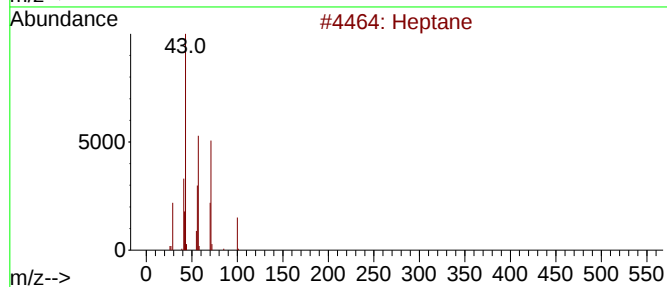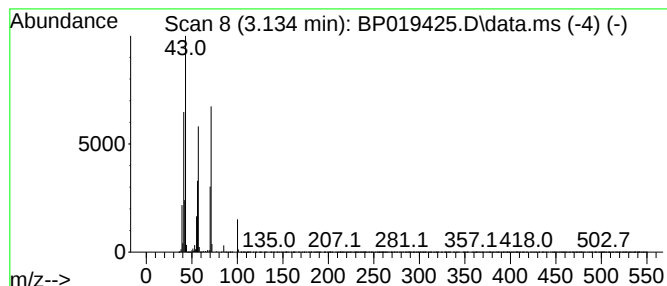

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
Data File : BP019425.D
Acq On : 23 Jan 2024 17:52
Operator : MA/JU
Sample : P1157-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.134	20.4	ng/u1	1060850	1	7.769	1040730	20.0