

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
 Data File : BP019426.D
 Acq On : 23 Jan 2024 18:26
 Operator : MA/JU
 Sample : P1157-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.134	4	8	13	rVB	1102256	1142552	53.43%	8.015%
2	3.440	57	60	61	rBV2	4816	4906	0.23%	0.034%
3	3.470	61	65	69	rVB	28345	35234	1.65%	0.247%
4	3.852	127	130	136	rVB7	4555	6996	0.33%	0.049%
5	3.946	142	146	153	rVB	34133	47208	2.21%	0.331%
6	4.052	161	164	167	rVB5	3197	3914	0.18%	0.027%
7	4.387	218	221	227	rVB	13339	21258	0.99%	0.149%
8	4.552	246	249	251	rBV4	2833	3113	0.15%	0.022%
9	4.587	253	255	259	rVB5	3136	3976	0.19%	0.028%
10	4.699	269	274	276	rBV6	4141	5207	0.24%	0.037%
11	4.787	285	289	293	rVB	11155	13366	0.63%	0.094%
12	5.087	337	340	342	rBV3	2588	3687	0.17%	0.026%
13	5.269	367	371	379	rVB	12996	20340	0.95%	0.143%
14	5.340	380	383	388	rVB6	3268	4555	0.21%	0.032%
15	5.405	388	394	403	rBV	20685	40537	1.90%	0.284%
16	5.775	453	457	461	rVB	17245	24405	1.14%	0.171%
17	6.252	533	538	545	rVV	21115	31198	1.46%	0.219%
18	6.305	545	547	552	rVB6	2015	2764	0.13%	0.019%
19	6.746	618	622	625	rVV6	5818	8333	0.39%	0.058%
20	6.793	628	630	635	rVV6	1787	3598	0.17%	0.025%
21	6.852	635	640	644	rVV2	11868	21329	1.00%	0.150%
22	6.893	644	647	648	rVV3	7304	8127	0.38%	0.057%
23	6.911	648	650	654	rVV5	7128	9576	0.45%	0.067%
24	6.987	657	663	670	rVB	16722	26275	1.23%	0.184%
25	7.152	682	691	698	rBV3	8202	20618	0.96%	0.145%
26	7.240	700	706	713	rVV3	5284	13145	0.61%	0.092%
27	7.311	716	718	724	rVV6	2601	4950	0.23%	0.035%
28	7.411	724	735	743	rVV	24988	47213	2.21%	0.331%
29	7.463	743	744	752	rVB8	2241	3419	0.16%	0.024%
30	7.658	771	777	783	rBV7	5766	10012	0.47%	0.070%
31	7.769	786	796	809	rBV	693848	1102667	51.57%	7.736%
32	7.875	809	814	824	rVV4	12196	28801	1.35%	0.202%
33	7.981	829	832	836	rBV5	2043	2467	0.12%	0.017%
34	8.063	844	846	851	rVB6	1857	2474	0.12%	0.017%
35	8.134	854	858	866	rVB3	6425	10572	0.49%	0.074%
36	8.258	875	879	884	rBV7	4477	9464	0.44%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
 Data File : BP019426.D
 Acq On : 23 Jan 2024 18:26
 Operator : MA/JU
 Sample : P1157-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

37	8.310	884	888	893	rVV6	4120	7559	0.35%	0.053%
38	8.405	899	904	910	rBV4	9905	18189	0.85%	0.128%
39	8.663	946	948	953	rVB6	1744	2626	0.12%	0.018%
40	8.722	953	958	962	rVV7	4163	6422	0.30%	0.045%
41	8.769	962	966	971	rVV8	3480	6429	0.30%	0.045%
42	8.840	971	978	979	rVV7	2586	3091	0.14%	0.022%
43	8.863	979	982	990	rVB5	7549	14317	0.67%	0.100%
44	8.963	995	999	1000	rVV4	2278	2805	0.13%	0.020%
45	8.987	1000	1003	1006	rVB4	5054	7076	0.33%	0.050%
46	9.069	1012	1017	1020	rBV7	1925	4132	0.19%	0.029%
47	9.110	1020	1024	1031	rVB9	4758	8062	0.38%	0.057%
48	9.399	1069	1073	1077	rBV6	3671	6956	0.33%	0.049%
49	9.457	1077	1083	1090	rVB7	5081	11919	0.56%	0.084%
50	9.622	1106	1111	1113	rBV5	2071	3204	0.15%	0.022%
51	9.816	1139	1144	1146	rBV6	2377	3967	0.19%	0.028%
52	9.963	1163	1169	1175	rBV9	5668	12005	0.56%	0.084%
53	10.028	1177	1180	1184	rVB6	2414	3213	0.15%	0.023%
54	10.340	1229	1233	1237	rVB7	2019	3514	0.16%	0.025%
55	10.428	1244	1248	1253	rBV8	4790	10514	0.49%	0.074%
56	10.563	1257	1271	1279	rBV	871575	1499979	70.15%	10.523%
57	11.234	1381	1385	1386	rBV4	2463	2735	0.13%	0.019%
58	11.469	1422	1425	1430	rVB6	2995	5472	0.26%	0.038%
59	11.587	1440	1445	1447	rBV6	3723	5870	0.27%	0.041%
60	11.628	1449	1452	1459	rVB9	3353	6335	0.30%	0.044%
61	11.840	1482	1488	1490	rBV7	1560	2684	0.13%	0.019%
62	11.981	1510	1512	1513	rBV2	3295	2765	0.13%	0.019%
63	12.128	1532	1537	1538	rBV5	2645	3323	0.16%	0.023%
64	12.240	1552	1556	1561	rBV4	6546	11998	0.56%	0.084%
65	12.287	1562	1564	1567	rVB4	2775	2716	0.13%	0.019%
66	12.381	1576	1580	1583	rVB6	2597	3666	0.17%	0.026%
67	12.457	1585	1593	1596	rBV4	10931	21513	1.01%	0.151%
68	12.610	1615	1619	1621	rBV5	3965	6398	0.30%	0.045%
69	12.757	1641	1644	1649	rVB7	3419	6341	0.30%	0.044%
70	12.840	1654	1658	1663	rVV6	8026	10875	0.51%	0.076%
71	12.893	1664	1667	1672	rVV6	3716	6475	0.30%	0.045%
72	12.946	1672	1676	1680	rVB6	5150	8210	0.38%	0.058%
73	12.998	1680	1685	1690	rVB8	8125	14443	0.68%	0.101%
74	13.075	1696	1698	1702	rBV5	2114	2557	0.12%	0.018%
75	13.181	1710	1716	1720	rBV5	16202	33327	1.56%	0.234%
76	13.328	1739	1741	1743	rVB2	4313	3238	0.15%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
 Data File : BP019426.D
 Acq On : 23 Jan 2024 18:26
 Operator : MA/JU
 Sample : P1157-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
 Title : SVOA CALIBRATION

77	13.816	1821	1824	1829	rVB2	39459	53812	2.52%	0.378%
78	13.893	1833	1837	1840	rBV6	11740	17028	0.80%	0.119%
79	13.934	1840	1844	1847	rBV6	11862	18935	0.89%	0.133%
80	14.004	1854	1856	1860	rVB4	6784	7604	0.36%	0.053%
81	14.140	1875	1879	1885	rBV7	27780	52919	2.47%	0.371%
82	14.228	1890	1894	1902	rVB3	60622	102472	4.79%	0.719%
83	14.310	1902	1908	1912	rBV8	19666	40124	1.88%	0.281%
84	14.369	1912	1918	1920	rBV3	27830	47982	2.24%	0.337%
85	14.416	1920	1926	1933	rVV	1352985	2002489	93.65%	14.048%
86	14.481	1933	1937	1943	rVV8	21206	45594	2.13%	0.320%
87	14.816	1992	1994	1998	rBV	15391	17246	0.81%	0.121%
88	15.122	2042	2046	2052	rVB8	23254	46558	2.18%	0.327%
89	15.192	2054	2058	2063	rVV2	60015	91913	4.30%	0.645%
90	15.463	2102	2104	2109	rVB4	22147	29790	1.39%	0.209%
91	15.675	2137	2140	2147	rVB8	31296	48754	2.28%	0.342%
92	17.169	2389	2394	2399	rBV	1530495	2138301	100.00%	15.001%
93	17.210	2399	2401	2408	rVB	180096	234085	10.95%	1.642%
94	18.233	2571	2575	2578	rBV2	125069	156530	7.32%	1.098%
95	18.610	2636	2639	2643	rBV3	99125	109067	5.10%	0.765%
96	19.192	2734	2738	2742	rVB	336476	423119	19.79%	2.968%
97	19.328	2758	2761	2766	rVB2	146842	181491	8.49%	1.273%
98	19.545	2795	2798	2802	rVB	144838	152026	7.11%	1.067%
99	21.275	3087	3092	3096	rBV	1348675	1834968	85.81%	12.873%
100	23.616	3485	3490	3503	rVB	922551	1856363	86.81%	13.023%

Sum of corrected areas: 14254346

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
Data File : BP019426.D
Acq On : 23 Jan 2024 18:26
Operator : MA/JU
Sample : P1157-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.134	20.72 ng/ul	1142550	1,4-Dichlorobenzene-d4	7.769

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	91
2			Heptane	100	C7H16	000142-82-5	90
3			Heptane	100	C7H16	000142-82-5	90
4			Heptane	100	C7H16	000142-82-5	87
5			Hexane, 3-methyl-	100	C7H16	000589-34-4	50

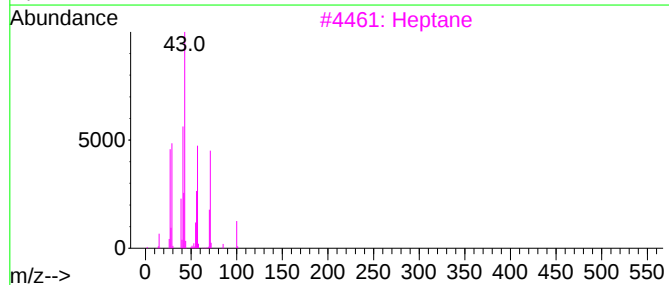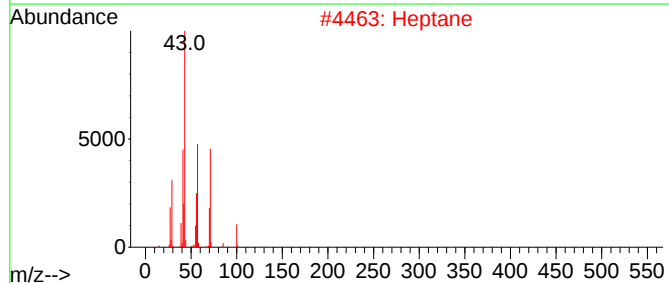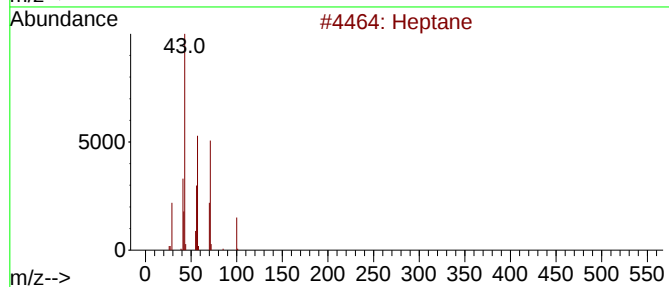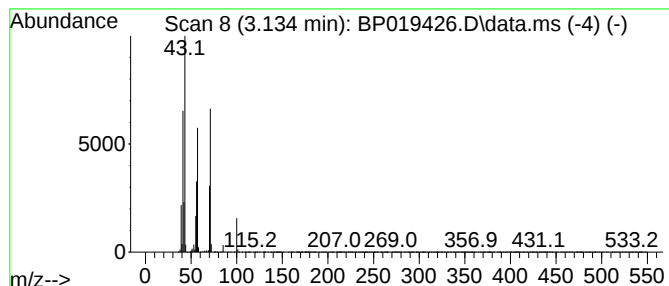

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012324\
Data File : BP019426.D
Acq On : 23 Jan 2024 18:26
Operator : MA/JU
Sample : P1157-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP010824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.134	20.7	ng/u1	1142550	1	7.769	1102670	20.0