
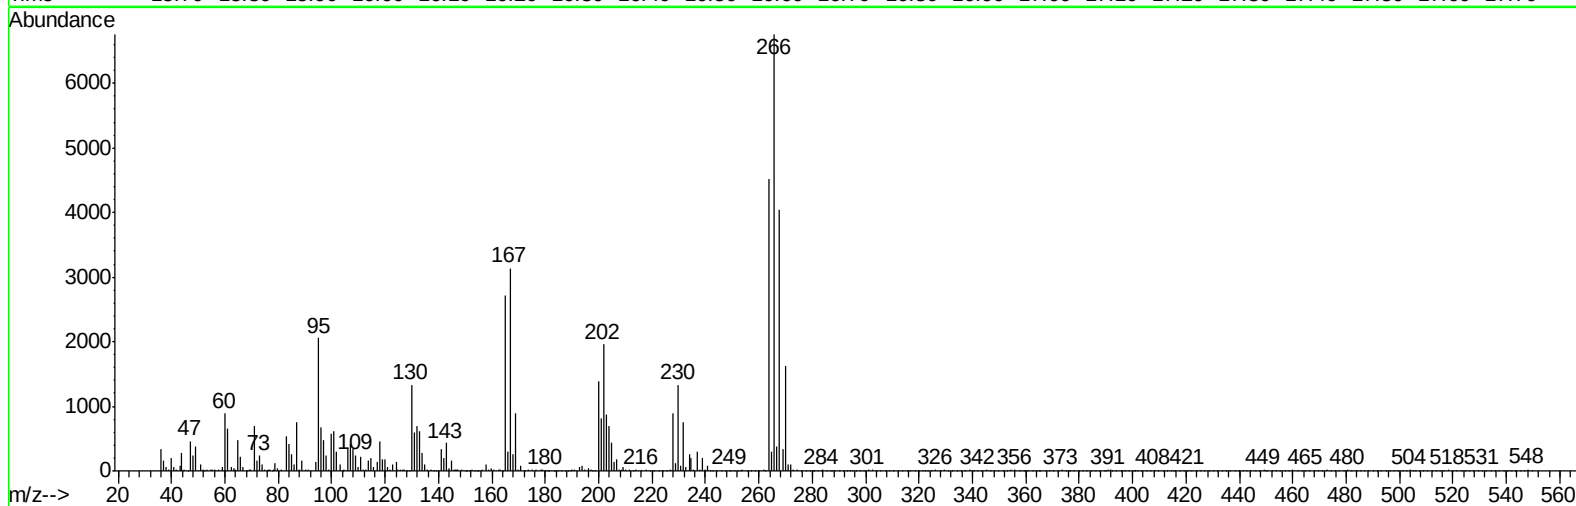


Data File : BP001676.D  
Acq On : 24 Jan 2020 12:22  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 04:37:58 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP010820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 24 22:23:46 2020  
Response via : Initial Calibration

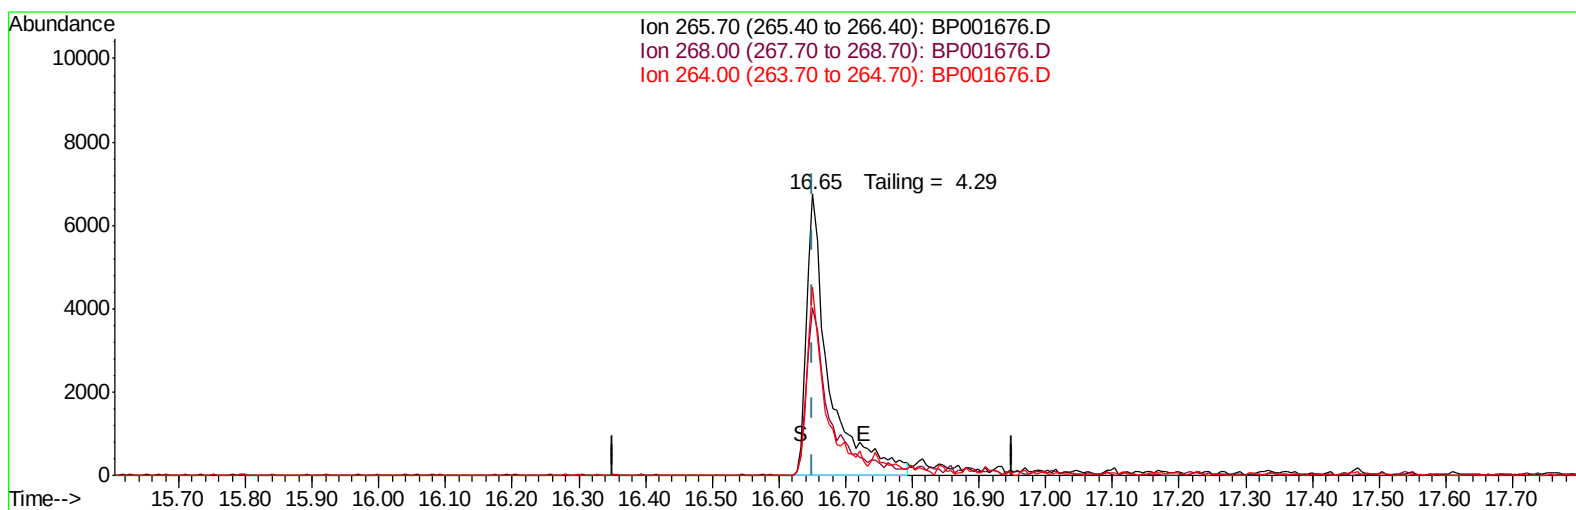

TIC: BP001676.D

(70) Pentachlorophenol (C)



16.651min (-0.000) 97001.43ng

response 15447

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.10 | 59.75 |
| 264.00 | 63.60 | 66.81 |
| 0.00   | 0.00  | 0.00  |

Data File : BP001676.D  
Acq On : 24 Jan 2020 12:22  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 04:37:58 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP010820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jan 24 22:23:46 2020  
Response via : Initial Calibration

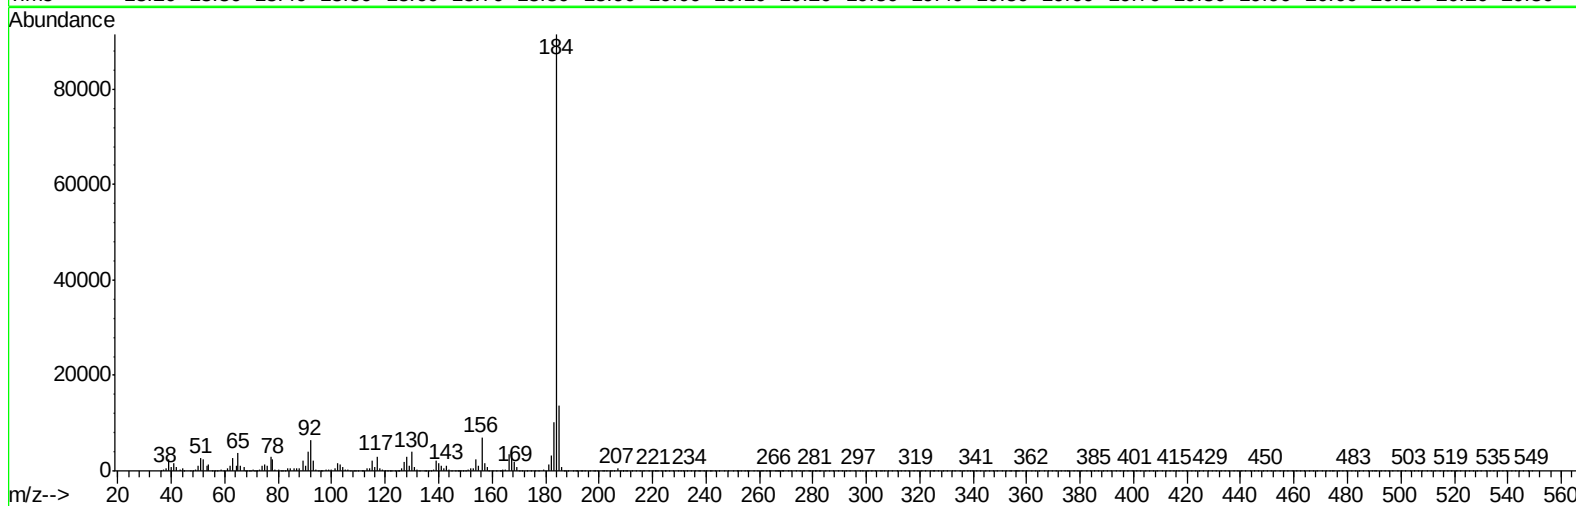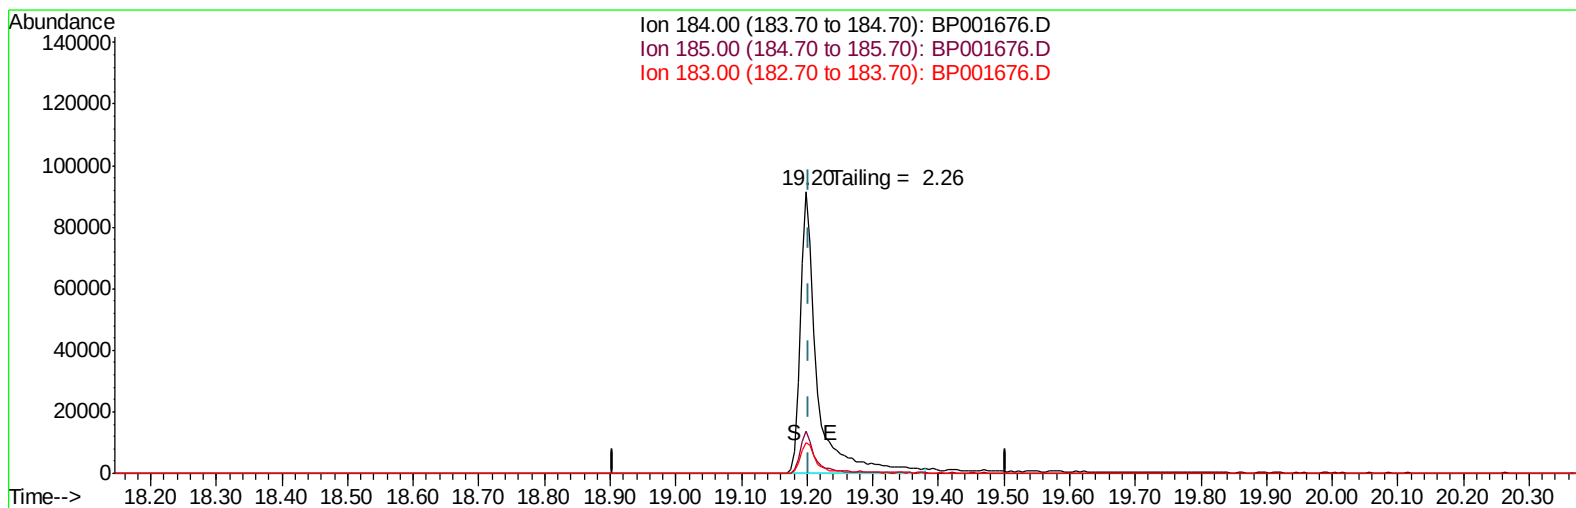

TIC: BP001676.D

(77) Benzidine

19.198min (-0.006) 34070.17ng

response 164146

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.30 | 14.93 |
| 183.00 | 11.70 | 11.03 |
| 0.00   | 0.00  | 0.00  |