


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP012420\
 Data File : BP001676.D
 Acq On : 24 Jan 2020 12:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 24 22:23:46 2020

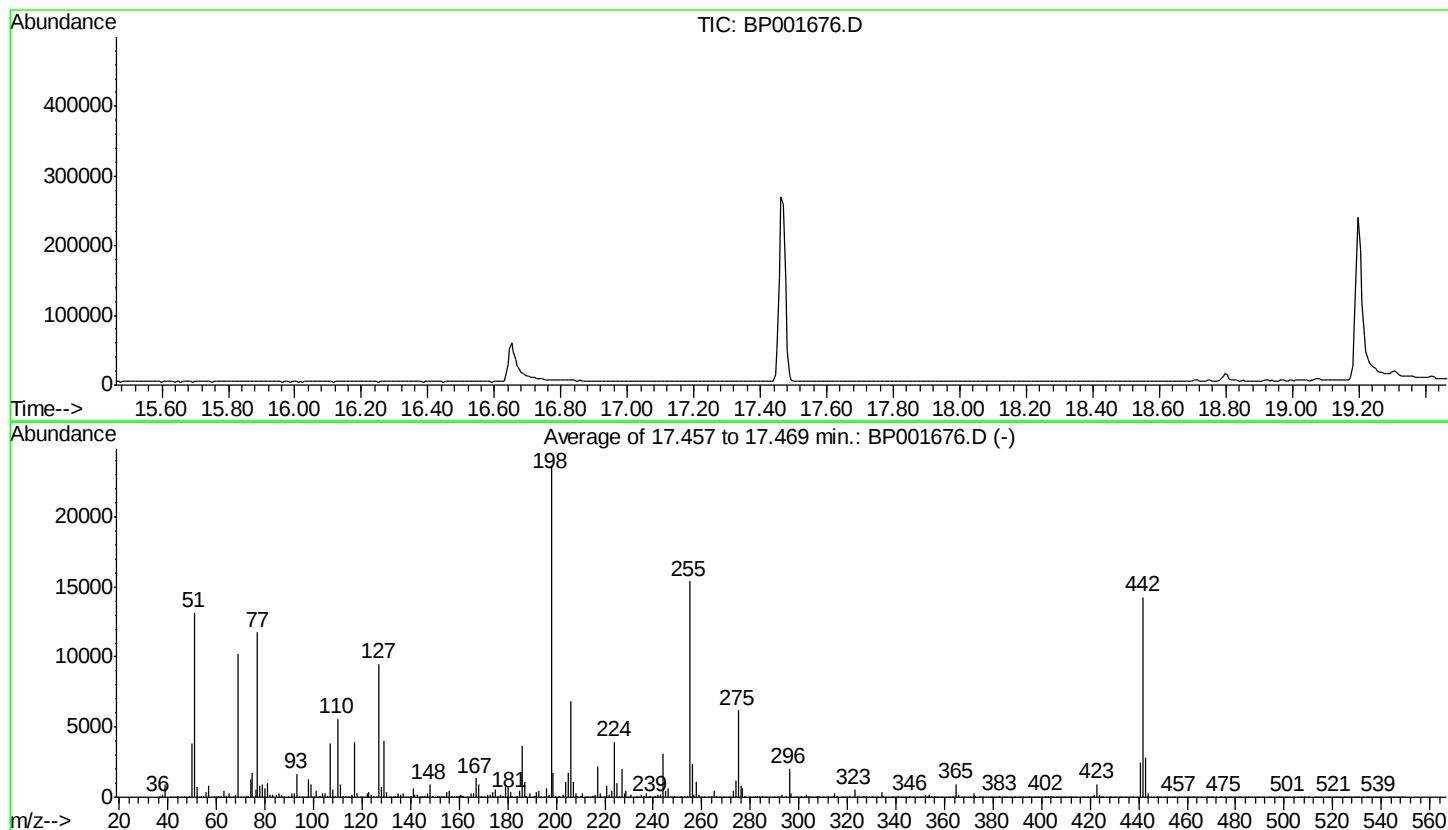

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.7	13170	PASS
68	69	0.00	2	1.7	175	PASS
69	198	0.00	100	43.2	10212	PASS
70	69	0.00	2	0.4	44	PASS
127	198	10	80	40.3	9534	PASS
197	198	0.00	2	0.6	140	PASS
198	198	100	100	100.0	23650	PASS
199	198	5	9	7.2	1714	PASS
275	198	10	60	26.1	6176	PASS
365	198	1	100	3.9	921	PASS
441	198	0.01	100	10.4	2467	PASS
442	198	50	100	60.3	14258	PASS
443	442	15	24	20.0	2848	PASS