
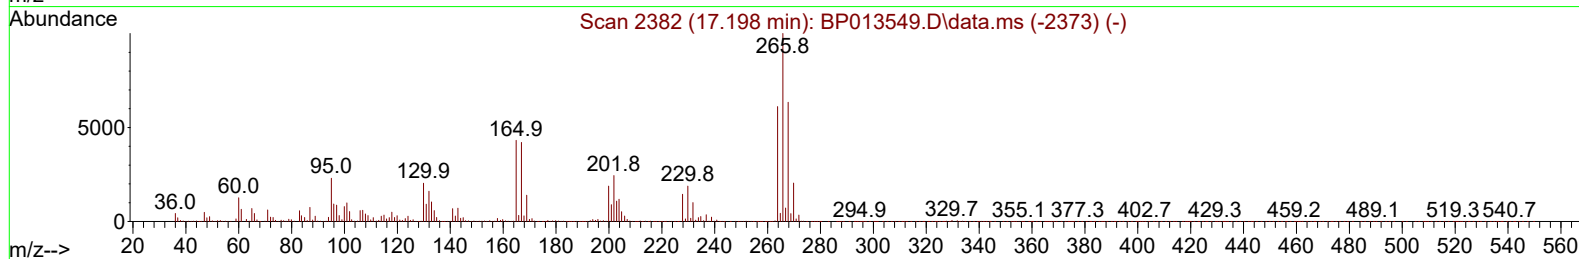
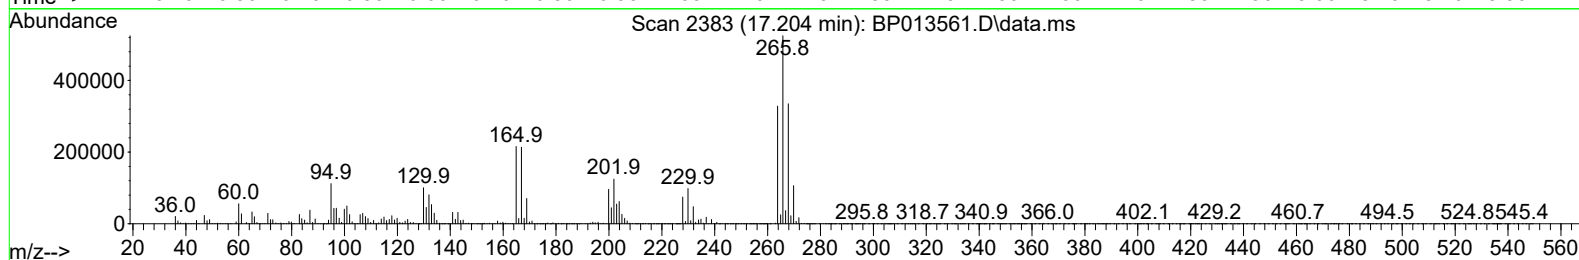


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012423\
Data File : BP013561.D
Acq On : 24 Jan 2023 09:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 05:54:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 03:43:27 2023
Response via : Initial Calibration

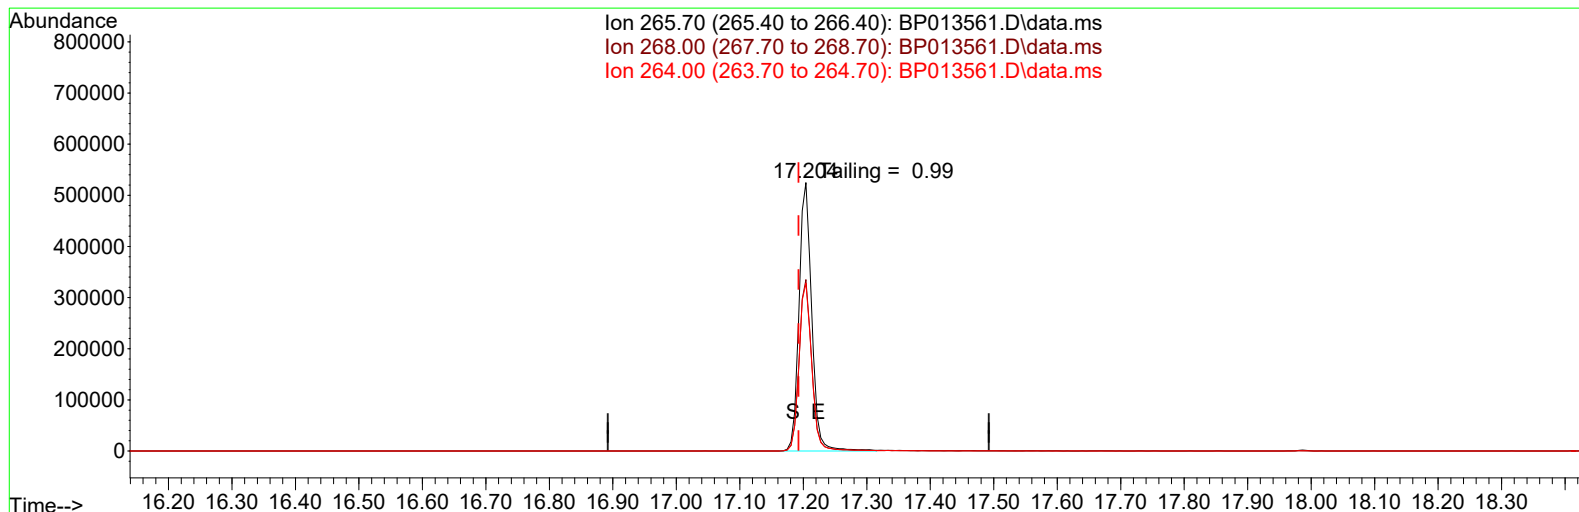

TIC: BP013561.D\data.ms

(70) Pentachlorophenol (C)




17.204min (+ 0.012) 507480.60 ng

response 738098

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.85
264.00	61.10	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012423\
Data File : BP013561.D
Acq On : 24 Jan 2023 09:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 05:54:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 03:43:27 2023
Response via : Initial Calibration

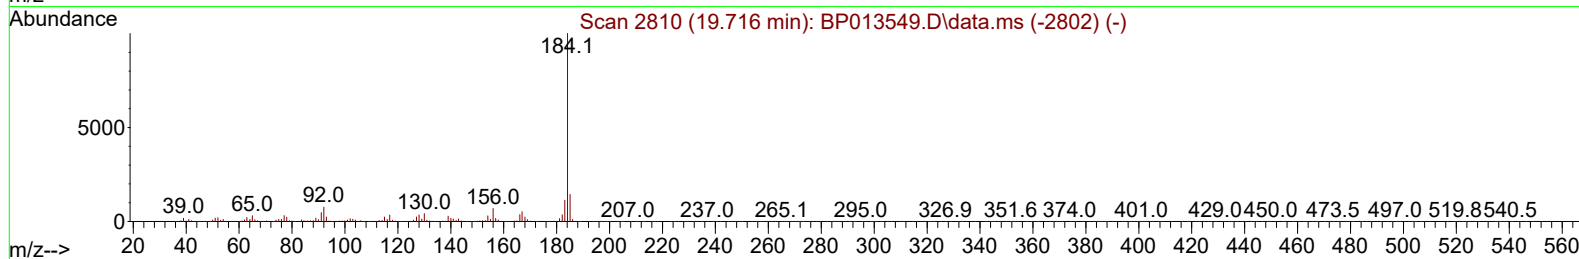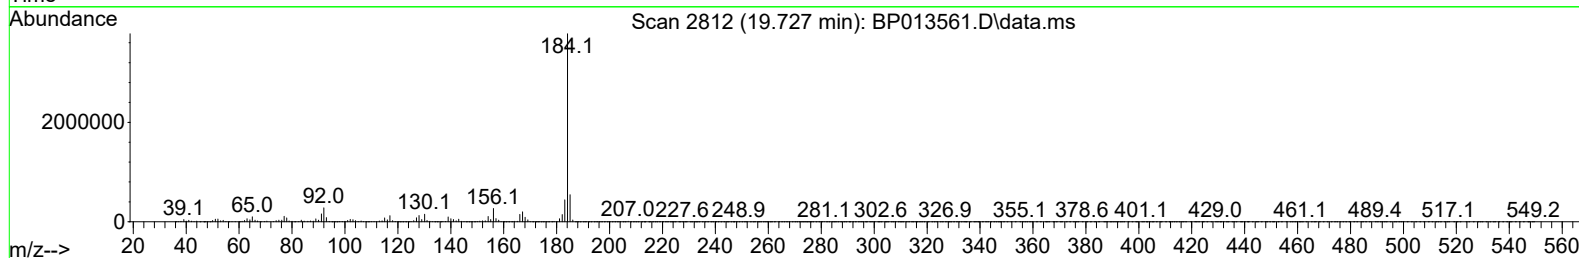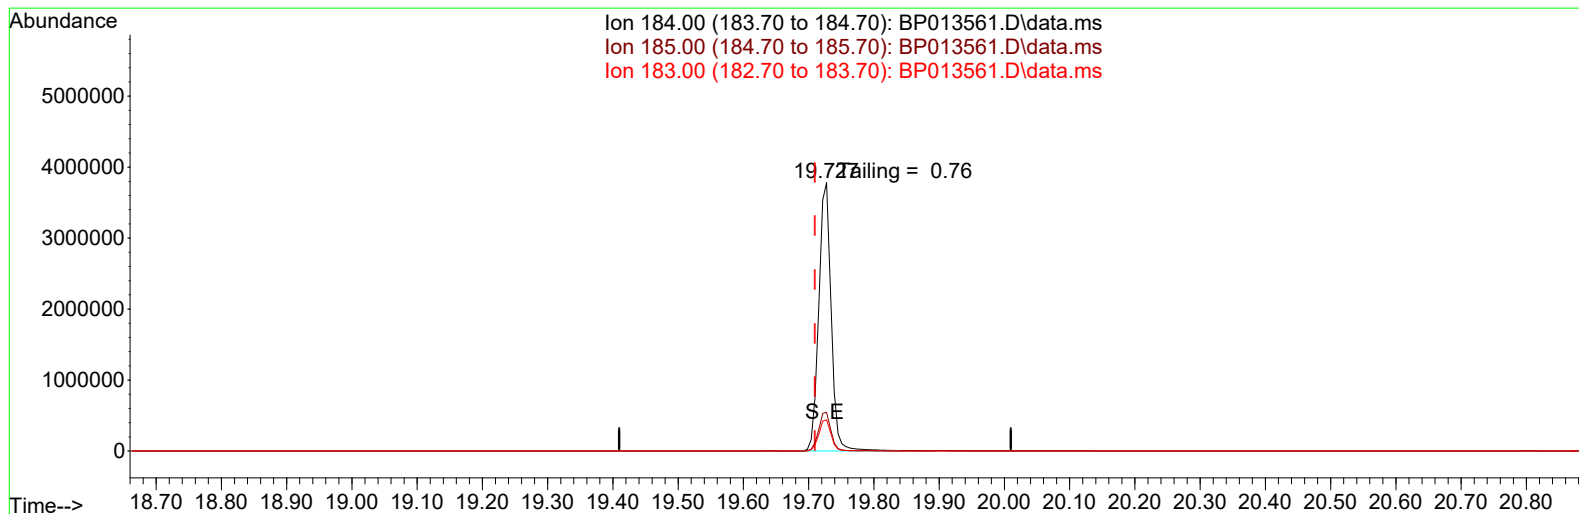

TIC: BP013561.D\data.ms

(77) Benzidine**19.727min (+ 0.017) 12021.93 ng****response 5000716**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.42
183.00	11.30	11.62
0.00	0.00	0.00