
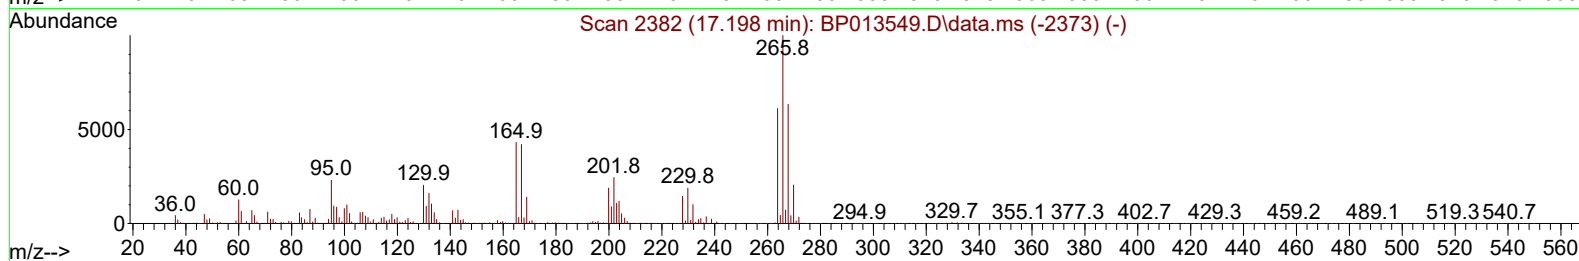
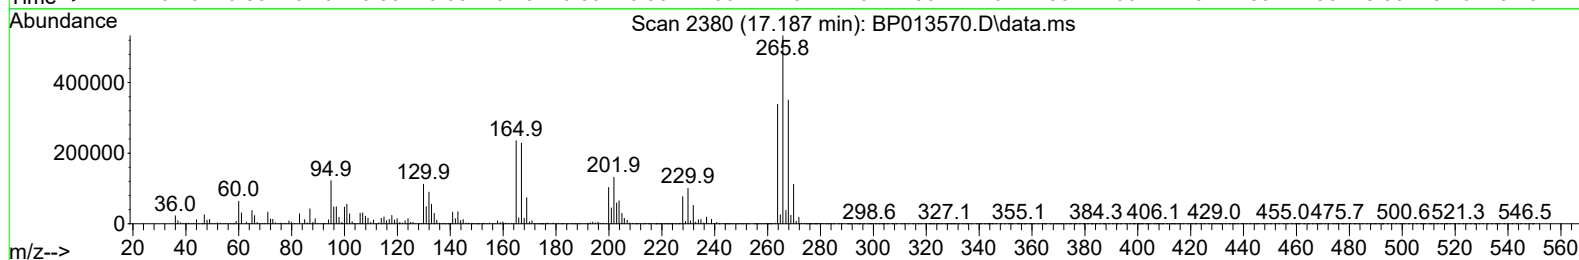


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012423\
 Data File : BP013570.D
 Acq On : 24 Jan 2023 14:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 05:55:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 03:43:27 2023
 Response via : Initial Calibration

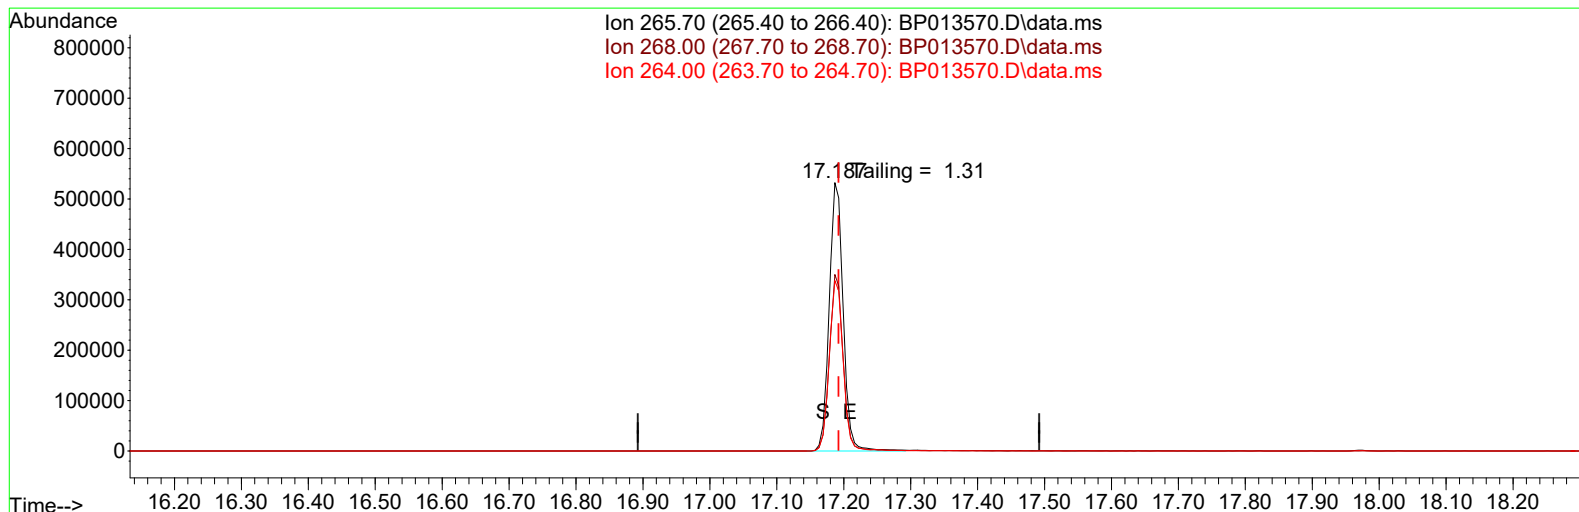

TIC: BP013570.D\data.ms

(70) Pentachlorophenol (C)




17.187min (-0.006) 3605533.60 ng

response 771186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	65.77
264.00	61.10	63.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012423\
Data File : BP013570.D
Acq On : 24 Jan 2023 14:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 25 05:55:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 03:43:27 2023
Response via : Initial Calibration

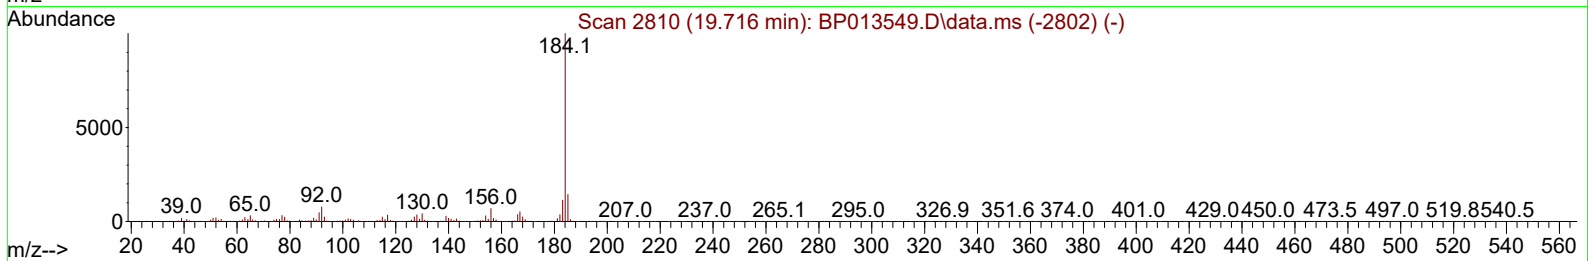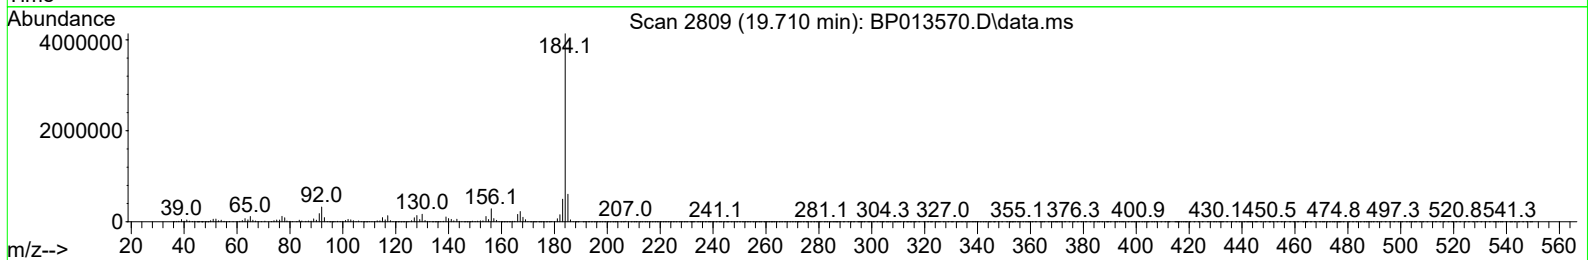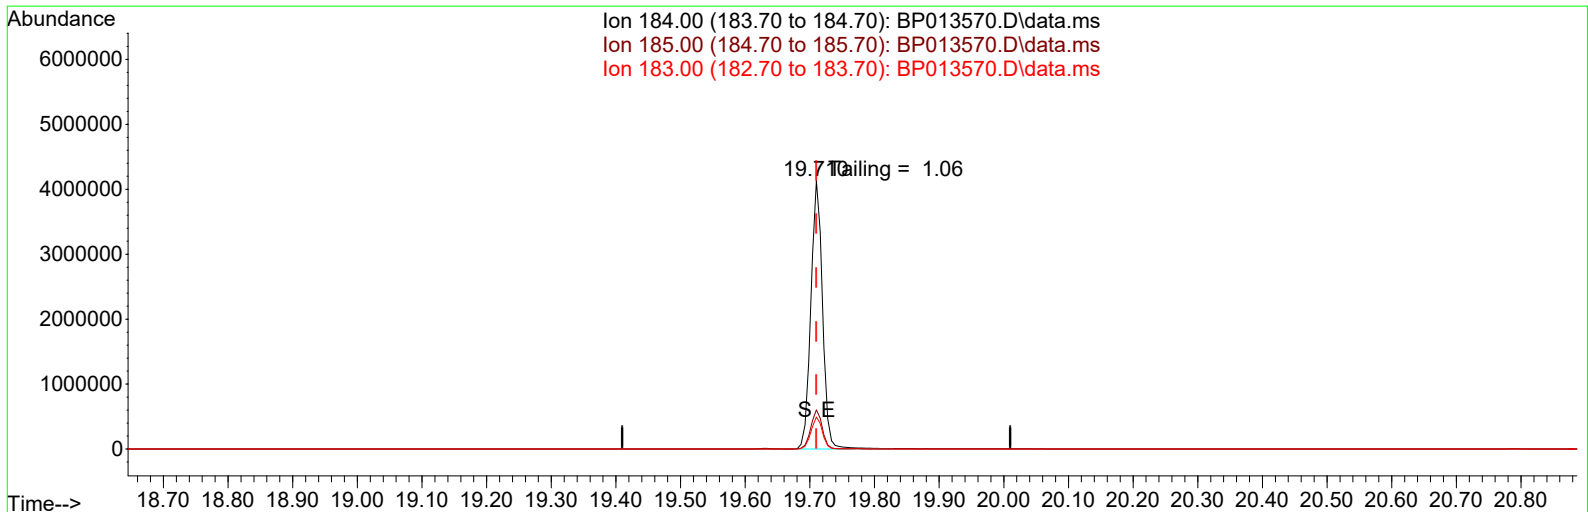

TIC: BP013570.D\data.ms

(77) Benzidine**19.710min (-0.000) 7395893.28 ng****response 5208315**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.60
183.00	11.30	11.97
0.00	0.00	0.00