

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
 Data File : BP023724.D
 Acq On : 24 Jan 2025 21:22
 Operator : RC/JU
 Sample : Q1147-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YE8C9

Quant Time: Jan 24 22:27:08 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 23 00:03:00 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	528949	20.000	ng/ul	0.00
20) Naphthalene-d8	10.569	136	2283543	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.416	164	1467480	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.216	188	2944706	20.000	ng/ul	0.00
79) Chrysene-d12	21.668	240	2771433	20.000	ng/ul	0.02
88) Perylene-d12	25.062	264	2798457	20.000	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	72076	5.488	ng/uL	0.00
4) Pyridine-d5	3.705	84	785215	20.720	ng/ul	0.00
7) Phenol-d5	6.952	99	1298000	29.001	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	775975	30.694	ng/ul	0.00
11) 2-Chlorophenol-d4	7.328	132	1034369	30.399	ng/ul	0.00
15) 4-Methylphenol-d8	8.481	113	1014313	28.820	ng/ul	0.00
21) Nitrobenzene-d5	8.934	128	505425	29.377	ng/ul	0.00
24) 2-Nitrophenol-d4	9.651	143	471848	29.914	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	948881	28.620	ng/ul	0.00
31) 4-Chloroaniline-d4	10.698	131	1429035	26.951	ng/ul	0.00
46) Dimethylphthalate-d6	13.816	166	3228550	30.592	ng/ul	0.00
49) Acenaphthylene-d8	14.104	160	3845217	31.481	ng/ul	0.00
54) 4-Nitrophenol-d4	14.598	143	492557	23.227	ng/ul	0.00
60) Fluorene-d10	15.416	176	2893983	32.034	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.533	200	267699	18.460	ng/ul	0.00
73) Anthracene-d10	17.316	188	4524044	32.001	ng/ul	0.00
81) Pyrene-d10	19.692	212	5125833	36.347	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.821	264	4489950	32.055	ng/ul	0.01
Target Compounds						Qvalue
8) Phenol	6.975	94	58596	1.251	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
Data File : BP023724.D
Acq On : 24 Jan 2025 21:22
Operator : RC/JU
Sample : Q1147-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE8C9

Quant Time: Jan 24 22:27:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 23 00:03:00 2025
Response via : Initial Calibration

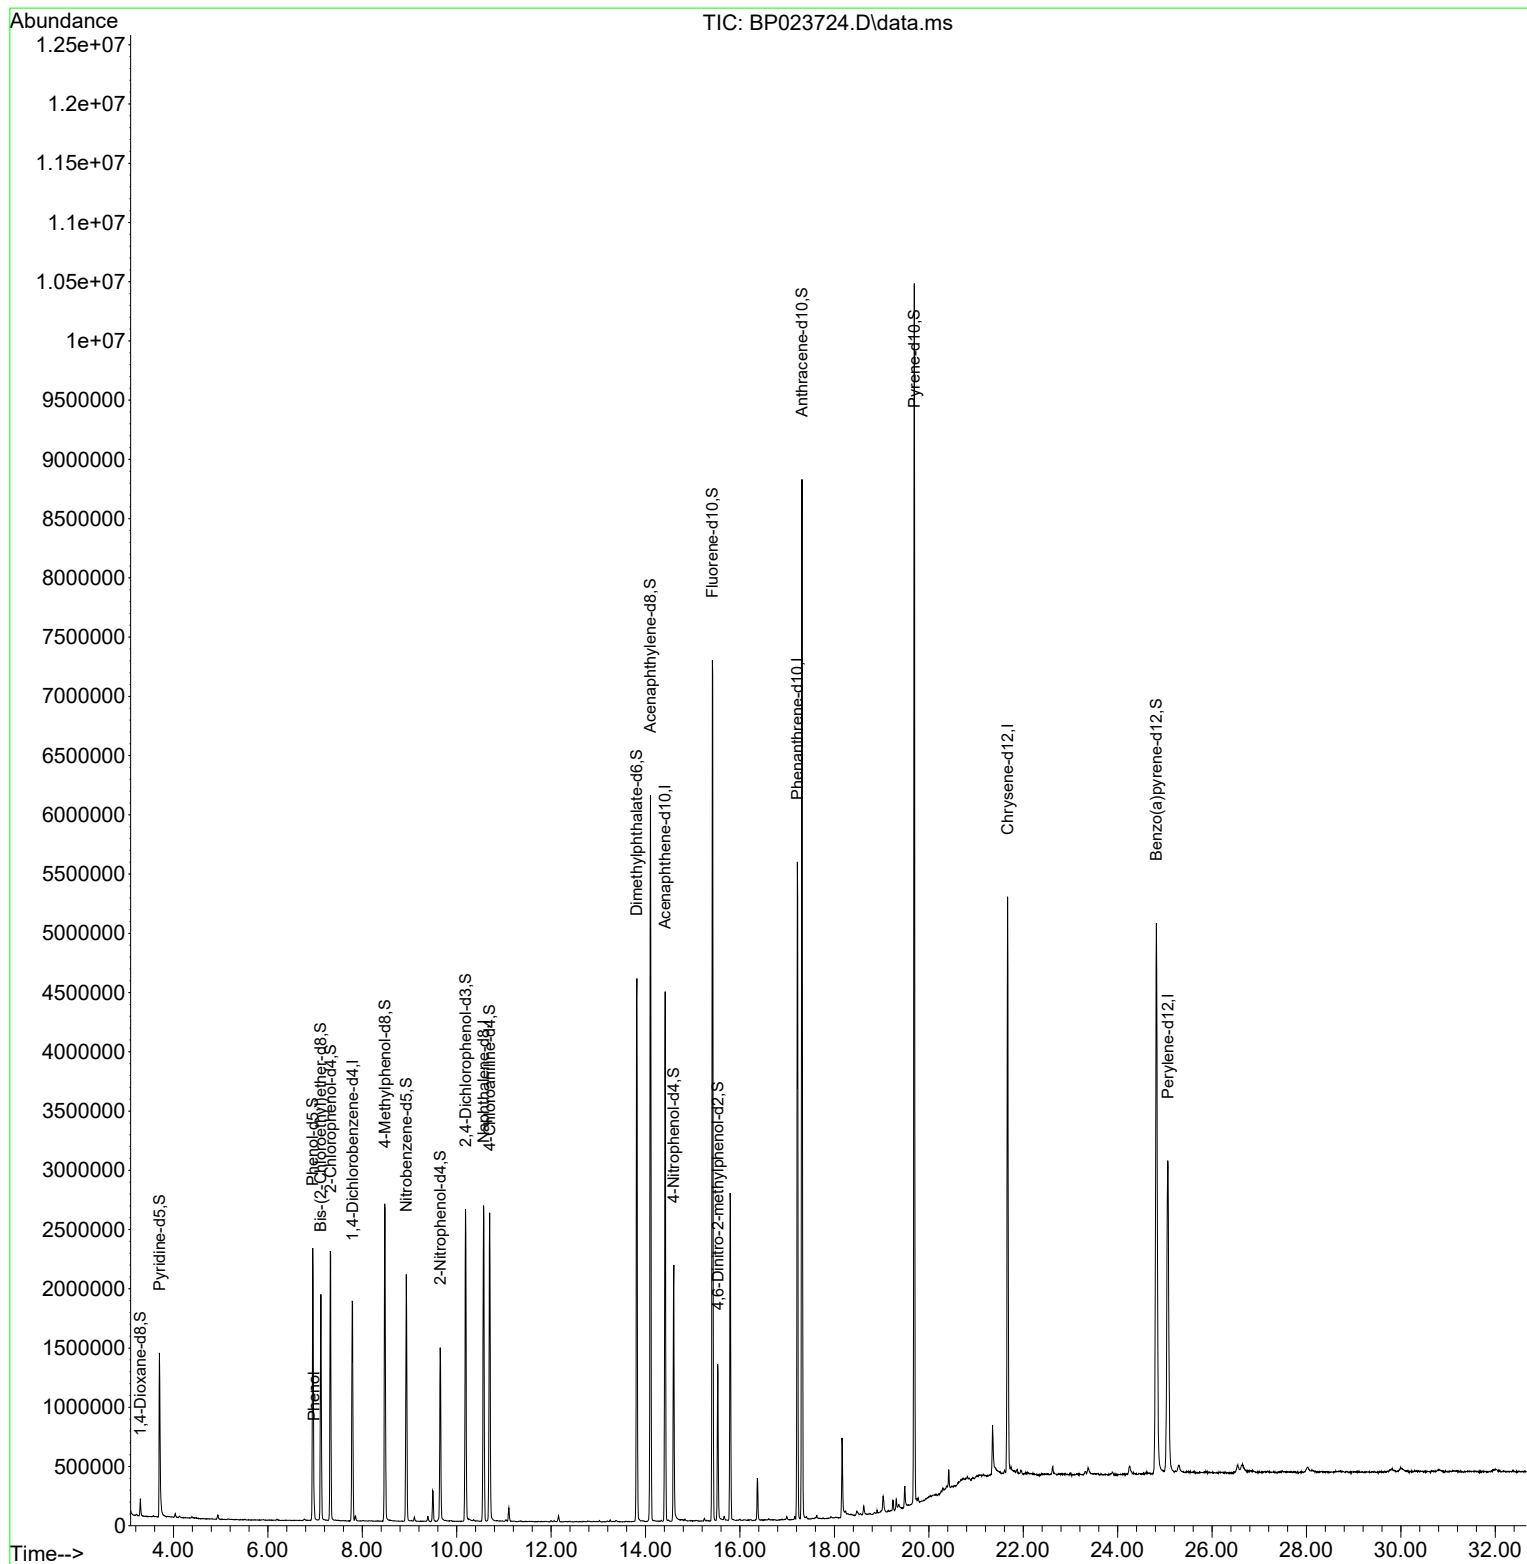

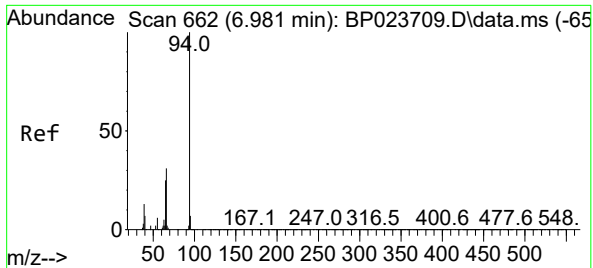

#8
Phenol
Concen: 1.251 ng/ul
RT: 6.975 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP023724.D
Acq: 24 Jan 2025 21:22

Instrument :
BNA_P
ClientSampleId :
YE8C9

Tgt Ion:	94	Resp:	58596
Ion	Ratio	Lower	Upper
94	100		
65	27.9	20.2	30.2
66	40.3	26.0	39.0

