

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
 Data File : BP023722.D
 Acq On : 24 Jan 2025 20:01
 Operator : RC/JU
 Sample : Q1147-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YE8D4

Quant Time: Jan 24 22:26:37 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 23 00:03:00 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.793	152	394317	20.000	ng/u1	0.00
20) Naphthalene-d8	10.569	136	1659155	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.410	164	1035829	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.204	188	2079231	20.000	ng/u1	0.00
79) Chrysene-d12	21.651	240	1945320	20.000	ng/u1	0.00
88) Perylene-d12	25.039	264	1934038	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	47226	4.824	ng/uL	0.00
4) Pyridine-d5	3.705	84	543947	19.254	ng/u1	0.00
7) Phenol-d5	6.957	99	809677	24.267	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.122	67	503973	26.741	ng/u1	0.00
11) 2-Chlorophenol-d4	7.328	132	654078	25.786	ng/u1	0.00
15) 4-Methylphenol-d8	8.481	113	622826	23.739	ng/u1	0.00
21) Nitrobenzene-d5	8.934	128	308167	24.652	ng/u1	0.00
24) 2-Nitrophenol-d4	9.651	143	283450	24.733	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.187	165	578293	24.006	ng/u1	0.00
31) 4-Chloroaniline-d4	10.693	131	898408	23.320	ng/u1	0.00
46) Dimethylphthalate-d6	13.816	166	2011554	27.003	ng/u1	0.00
49) Acenaphthylene-d8	14.104	160	2308127	26.771	ng/u1	0.00
54) 4-Nitrophenol-d4	14.598	143	277781	18.558	ng/u1	0.00
60) Fluorene-d10	15.416	176	1784804	27.989	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.528	200	133385	13.027	ng/u1	0.00
73) Anthracene-d10	17.304	188	2793113	27.981	ng/u1	0.00
81) Pyrene-d10	19.674	212	3165376	31.978	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.804	264	2654956	27.426	ng/u1	0.00
Target Compounds						
					Qvalue	
8) Phenol	6.981	94	38428	1.101	ng/u1	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
Data File : BP023722.D
Acq On : 24 Jan 2025 20:01
Operator : RC/JU
Sample : Q1147-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YE8D4

Quant Time: Jan 24 22:26:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 23 00:03:00 2025
Response via : Initial Calibration

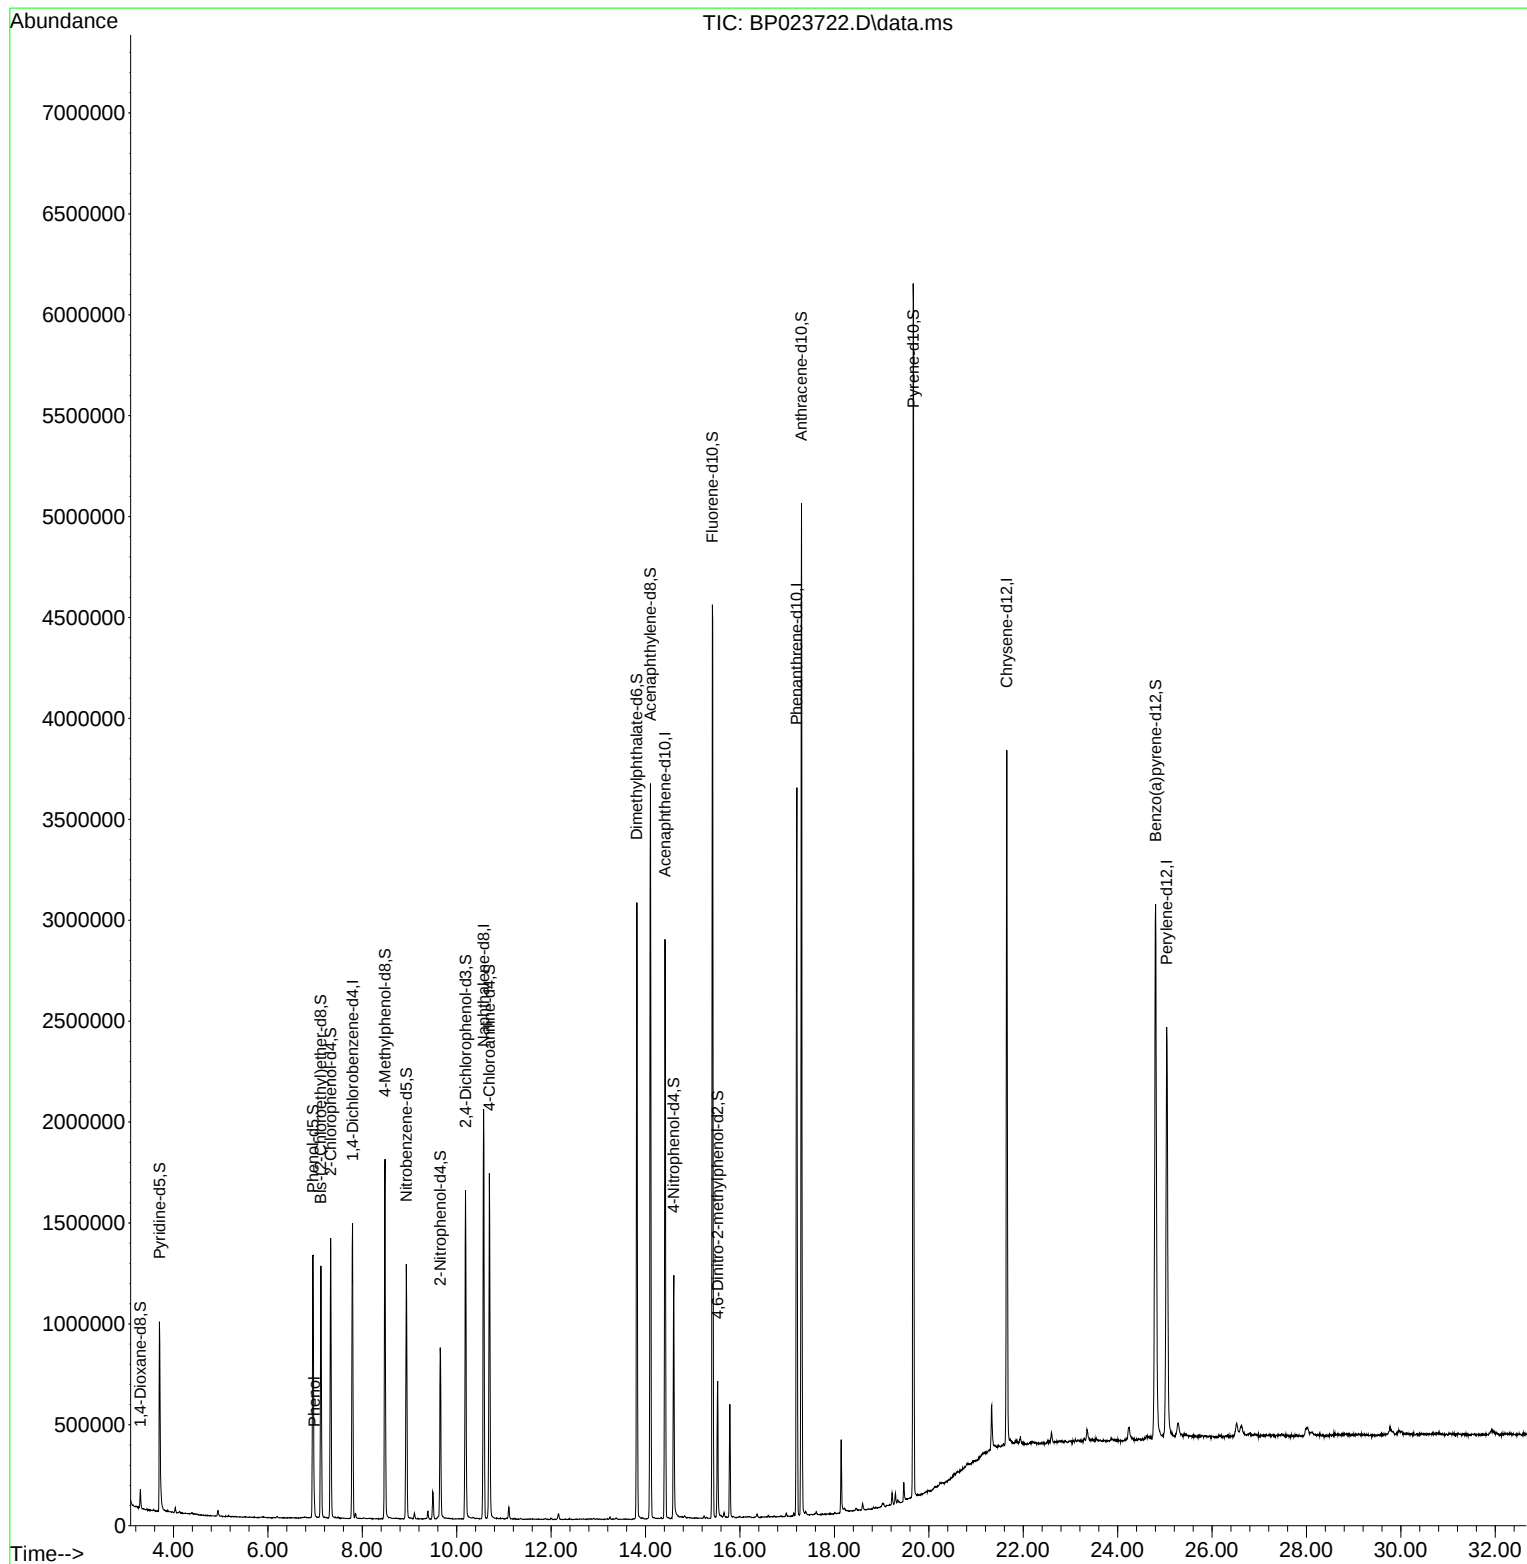

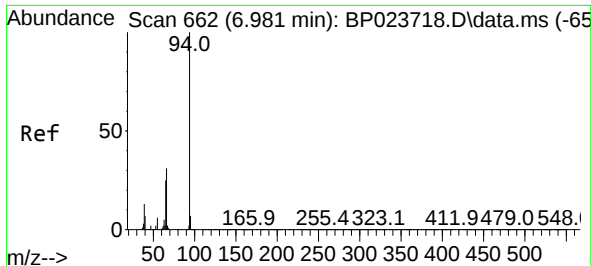

#8

Phenol

Concen: 1.101 ng/ul

RT: 6.981 min Scan# 6

Delta R.T. 0.000 min

Lab File: BP023722.D


Acq: 24 Jan 2025 20:01

Instrument :

BNA_P

ClientSampleId :

YE8D4

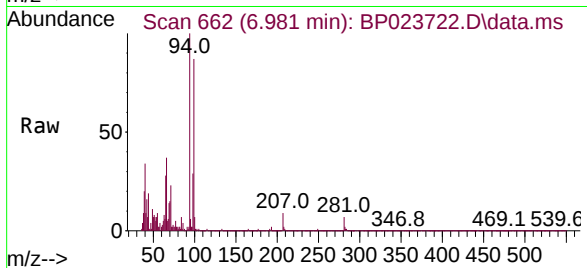

Tgt Ion: 94	Resp:	38428
Ion	Ratio	Lower Upper
94	100	
65	28.5	20.2 30.2
66	36.6	26.0 39.0

