

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
 Data File : BP023710.D
 Acq On : 24 Jan 2025 10:11
 Operator : RC/JU
 Sample : PB166118BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK118

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	47	rVB	148259	194988	1.67%	0.177%
2	3.705	101	105	128	rBV	1807051	2667397	22.86%	2.420%
3	4.034	158	161	169	rVB	20489	28801	0.25%	0.026%
4	6.958	649	658	671	rBV	2125369	3181852	27.27%	2.887%
5	7.128	680	687	698	rBV	1672595	2547969	21.83%	2.312%
6	7.328	714	721	729	rBV	2115275	3216040	27.56%	2.918%
7	7.793	791	800	808	rBV	1344068	2018991	17.30%	1.832%
8	8.481	908	917	929	rBV	2595499	3958901	33.92%	3.592%
9	8.934	985	994	1002	rBV	1679750	2785735	23.87%	2.527%
10	9.652	1108	1116	1125	rBV	1157144	1903883	16.31%	1.727%
11	10.187	1199	1207	1229	rBV	2463235	3811186	32.66%	3.458%
12	10.575	1265	1273	1285	rVB	1564042	2722953	23.33%	2.470%
13	10.699	1285	1294	1318	rBV	2127976	3607274	30.91%	3.273%
14	12.157	1535	1542	1551	rBV	35799	64278	0.55%	0.058%
15	13.816	1817	1824	1837	rBV	4049831	5696929	48.82%	5.168%
16	14.104	1864	1873	1883	rBV	4743696	6813350	58.38%	6.181%
17	14.416	1919	1926	1935	rBV	2293537	3646391	31.25%	3.308%
18	14.593	1948	1956	1976	rBV	1838670	2657741	22.77%	2.411%
19	15.251	2064	2068	2073	rBV4	7016	12577	0.11%	0.011%
20	15.428	2089	2098	2109	rBV	6055218	8759591	75.06%	7.947%
21	15.528	2109	2115	2127	rBV	1310209	1642666	14.08%	1.490%
22	15.669	2135	2139	2146	rVB4	24510	42484	0.36%	0.039%
23	16.228	2230	2234	2239	rVB6	7986	12899	0.11%	0.012%
24	16.998	2360	2365	2369	rBV4	13248	21505	0.18%	0.020%
25	17.216	2394	2402	2412	rBV	3345846	4522713	38.76%	4.103%
26	17.316	2412	2419	2432	rBV	6972730	9725971	83.34%	8.823%
27	17.692	2479	2483	2487	rBV7	5746	12572	0.11%	0.011%
28	18.151	2557	2561	2568	rBV7	18424	37910	0.32%	0.034%
29	19.228	2740	2744	2750	rBV4	65371	95547	0.82%	0.087%
30	19.298	2752	2756	2764	rVV	62555	100839	0.86%	0.091%
31	19.681	2815	2821	2832	rBV	9294606	11669852	100.00%	10.587%
32	21.651	3150	3156	3167	rBV	3109774	5058355	43.35%	4.589%
33	24.804	3683	3692	3711	rVB	4613622	11606709	99.46%	10.530%
34	25.027	3723	3730	3754	rVB2	1820904	5381262	46.11%	4.882%

Sum of corrected areas: 110228111




Instrument :
BNA_P
ClientSampleId :
SBLK118

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
Data File : BP023710.D
Acq On : 24 Jan 2025 10:11
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

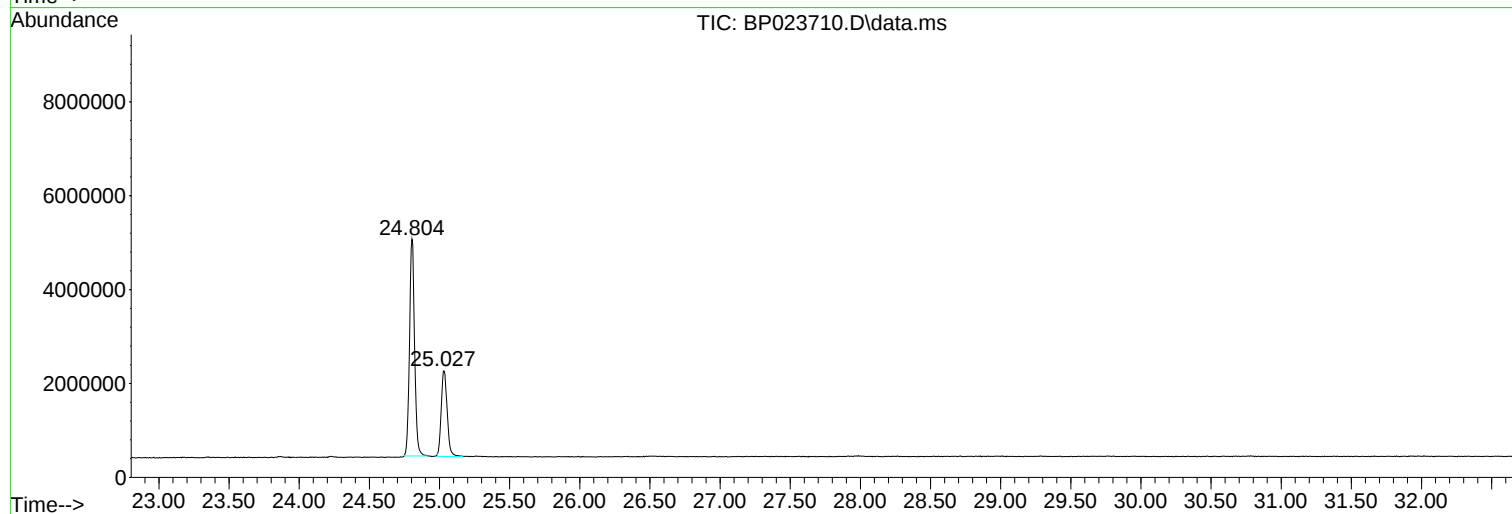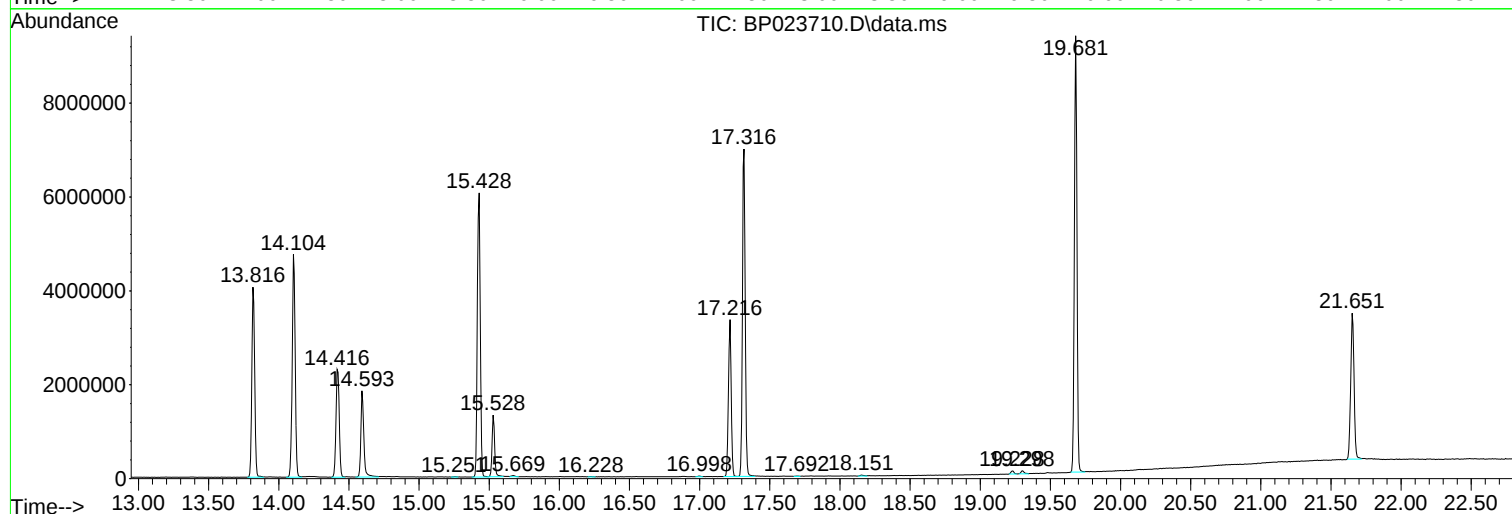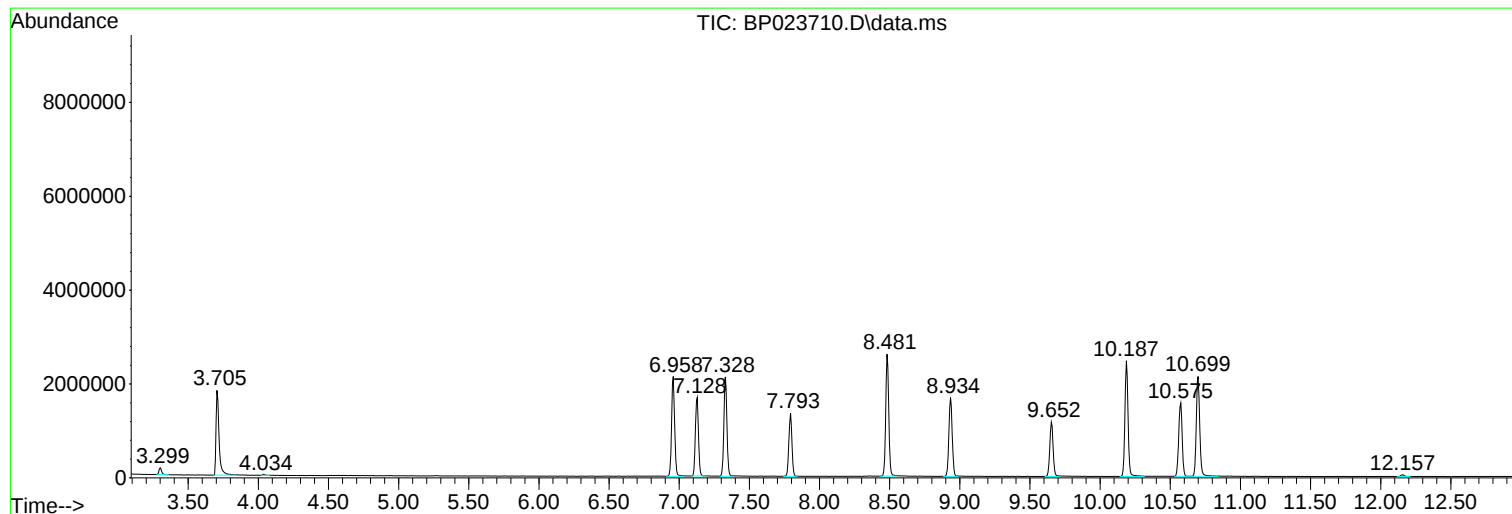

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
Data File : BP023710.D
Acq On : 24 Jan 2025 10:11
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012425\
Data File : BP023710.D
Acq On : 24 Jan 2025 10:11
Operator : RC/JU
Sample : PB166118BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK118

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP012225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc